
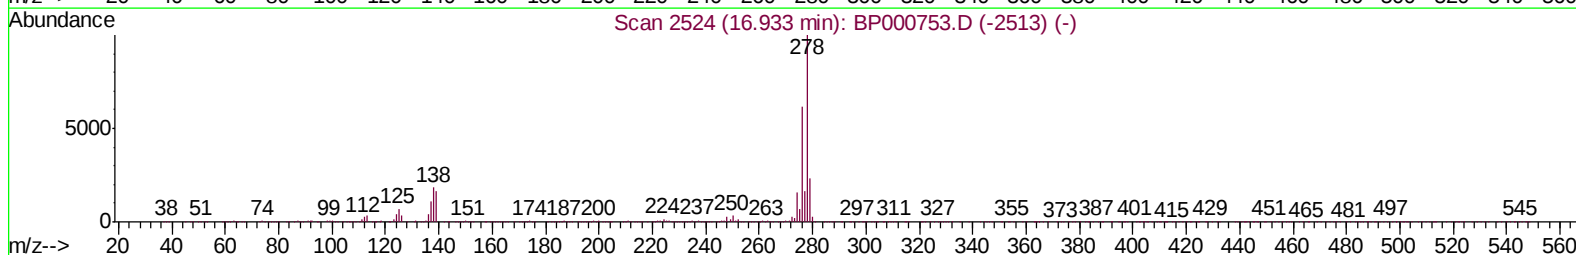
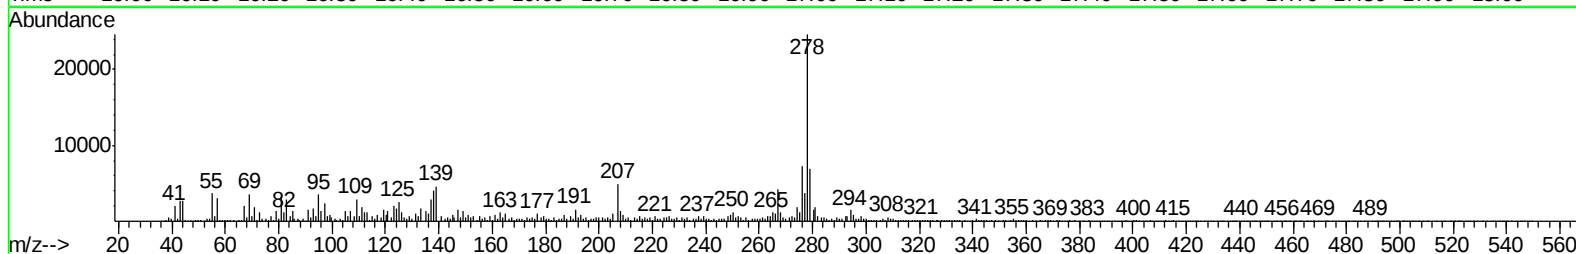


Data File : BP000760.D
Acq On : 15 Oct 2019 12:56
Operator : JU
Sample : K5175-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Oct 16 02:26:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 02:22:01 2019
Response via : Initial Calibration

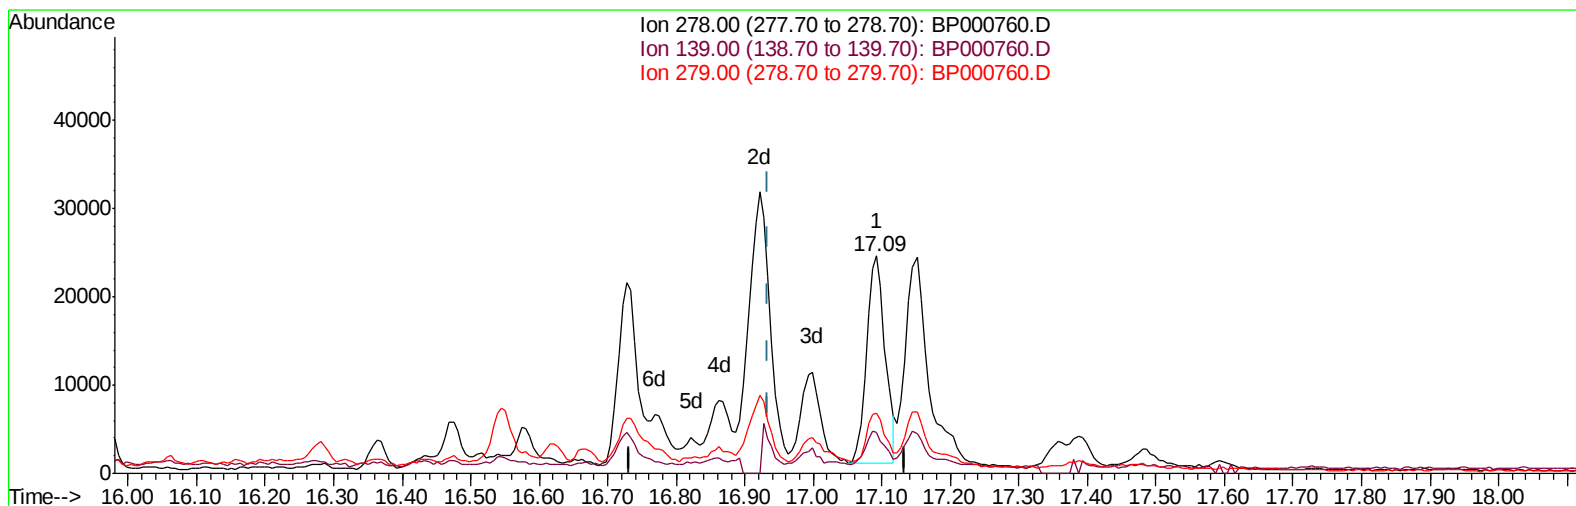

TIC: BP000760.D

(93) Dibenzo(a,h)anthracene

17.092min (+0.159) 1.11ng/ul

response 44078

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	18.72
279.00	24.00	27.90
0.00	0.00	0.00