

Data File : BP000760.D

Acq On : 15 Oct 2019 12:56

Operator : JU

Sample : K5175-09

Misc :

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Oct 16 02:26:31 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Oct 16 02:22:01 2019

Response via : Initial Calibration

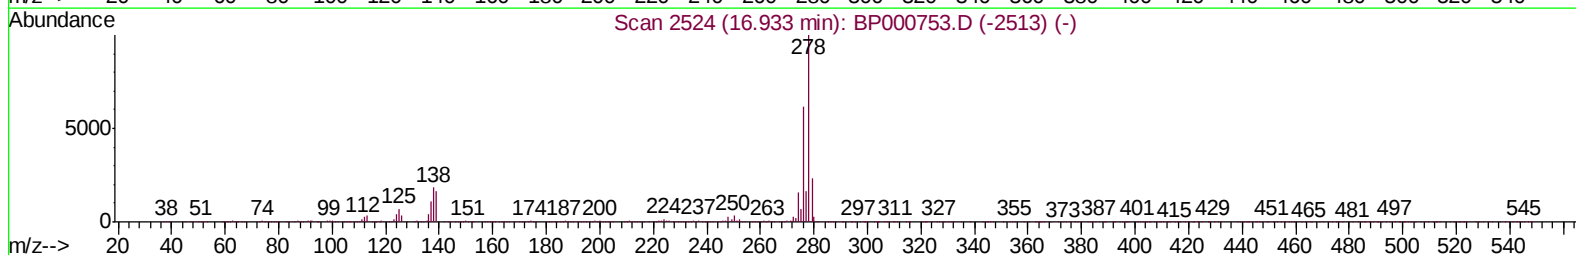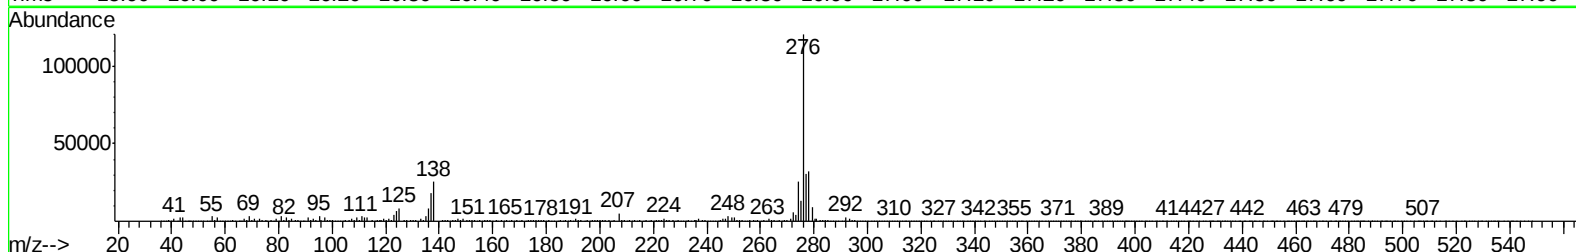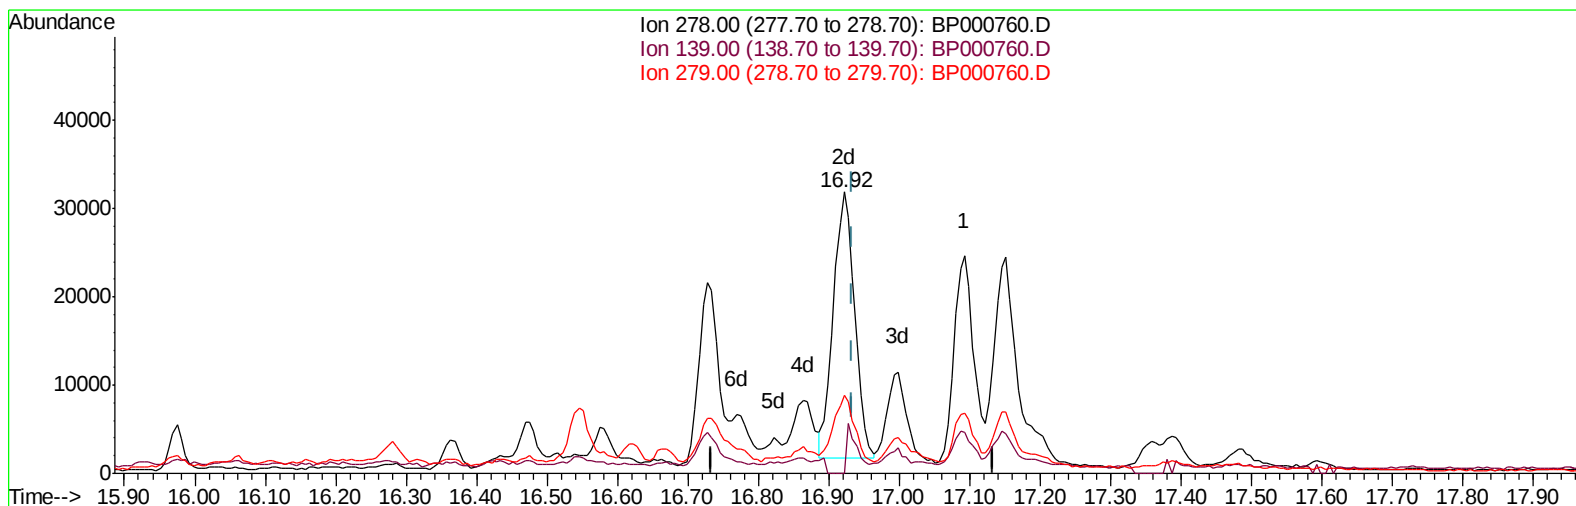

TIC: BP000760.D

(93) Dibenzo(a,h)anthracene

16.922min (-0.012) 1.58ng/ul m

response 62808

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	0.00#
279.00	24.00	27.53
0.00	0.00	0.00