
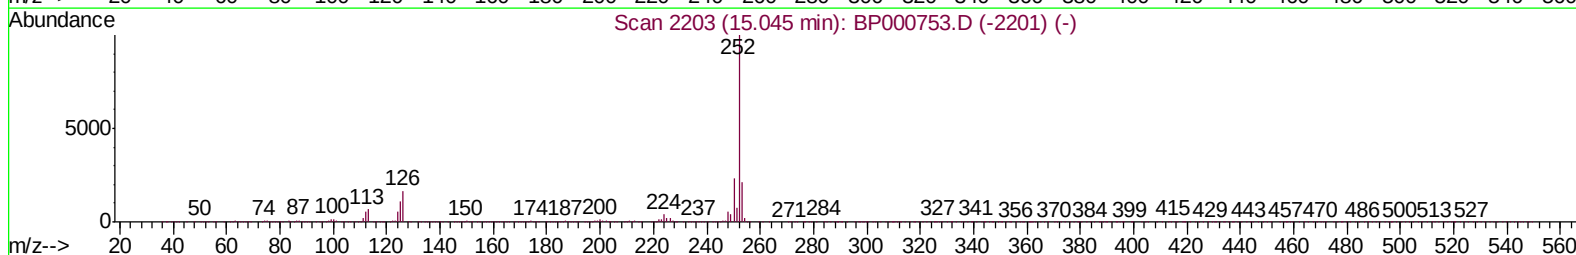
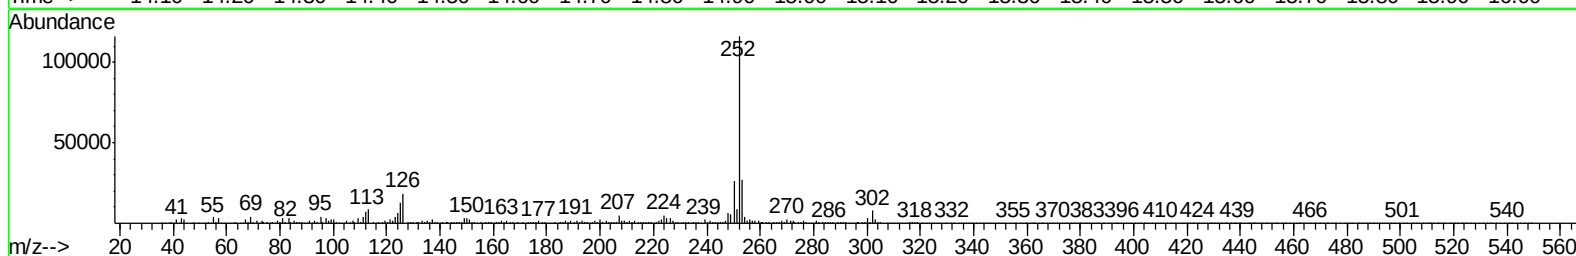


Data File : BP000761.D
Acq On : 15 Oct 2019 13:21
Operator : JU
Sample : K5175-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Oct 16 02:26:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 02:22:01 2019
Response via : Initial Calibration

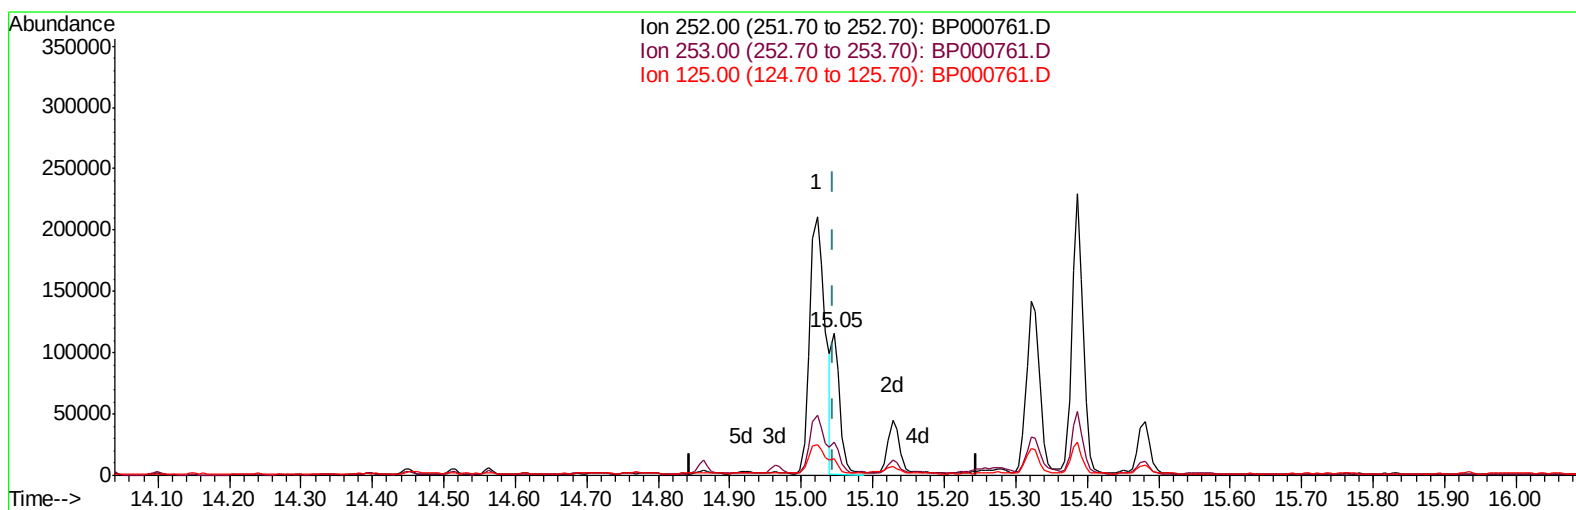

TIC: BP000761.D

(89) Benzo(k)fluoranthene

15.045min (+0.000) 1.91ng/ul m

response 88987

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	23.59
125.00	10.30	11.32
0.00	0.00	0.00