
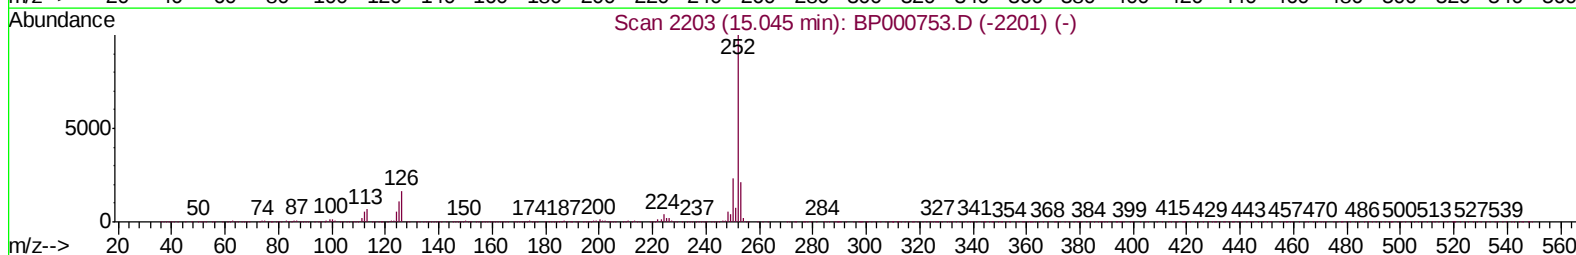
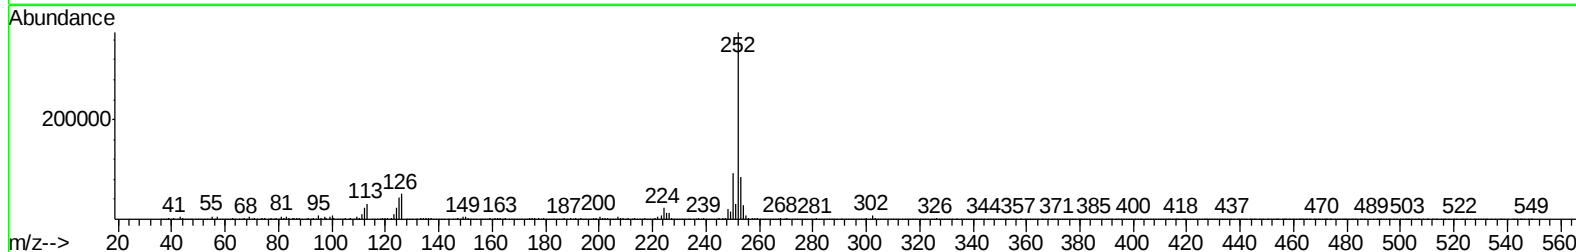


Data File : BP000762.D  
Acq On : 15 Oct 2019 13:45  
Operator : JU  
Sample : K5175-11  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 16 02:27:18 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\SOM-EPA-BP100919MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Oct 16 02:22:01 2019  
Response via : Initial Calibration

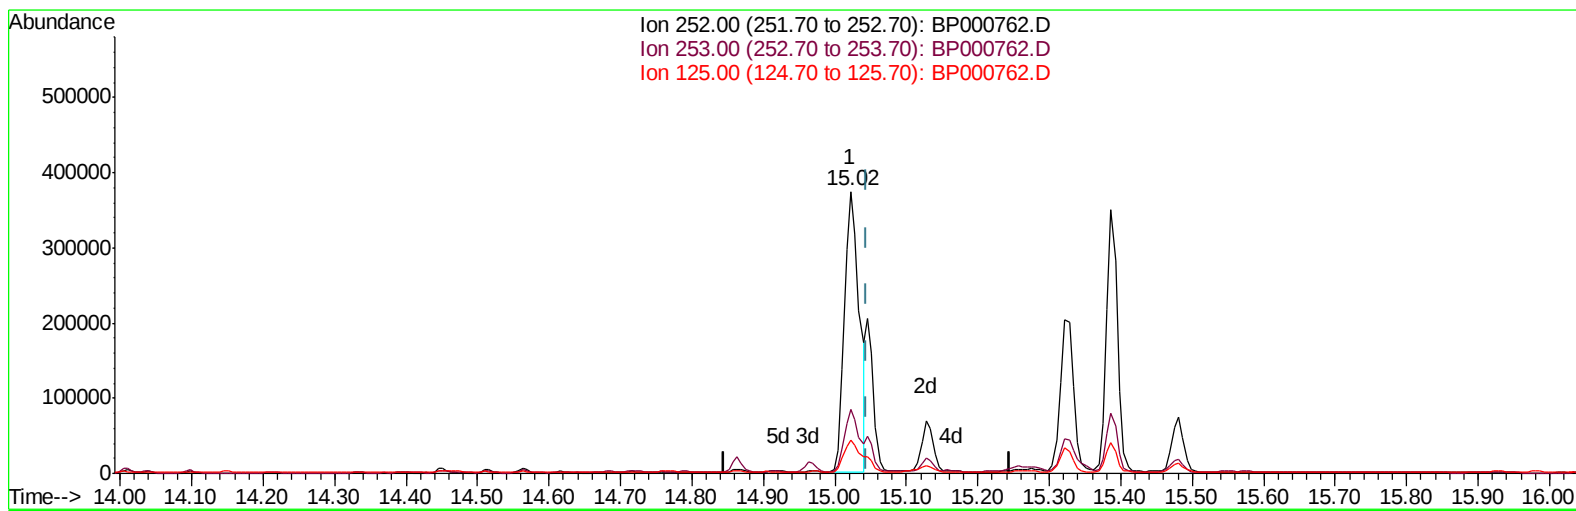

TIC: BP000762.D

(89) Benzo(k)fluoranthene

15.022min (-0.023) 13.93ng/ul

response 543861

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 22.20 | 22.73 |
| 125.00 | 10.30 | 11.66 |
| 0.00   | 0.00  | 0.00  |