
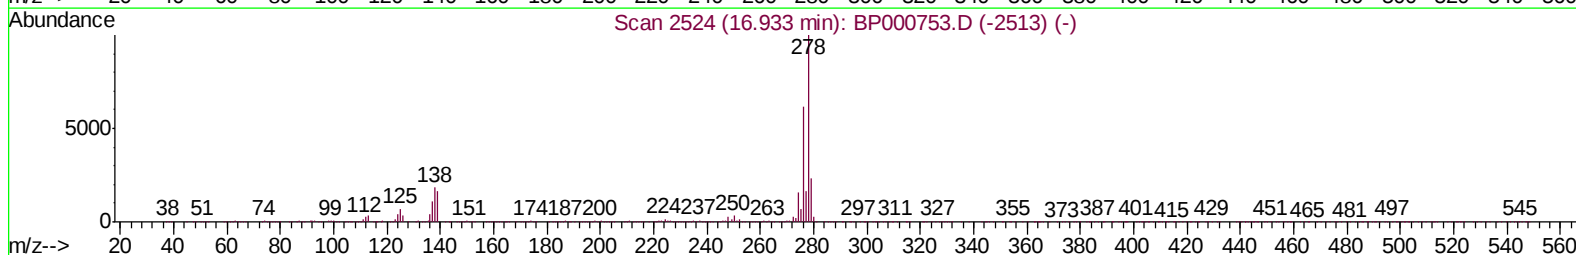
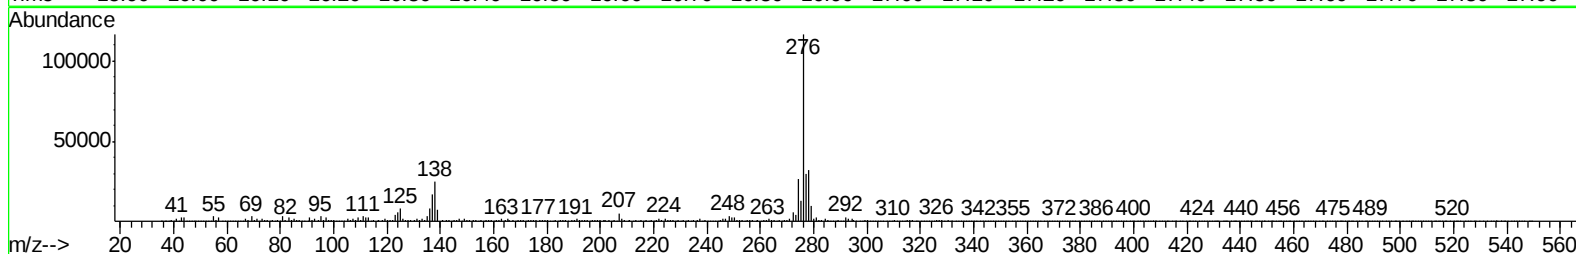


Data File : BP000762.D
Acq On : 15 Oct 2019 13:45
Operator : JU
Sample : K5175-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 16 02:27:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 02:22:01 2019
Response via : Initial Calibration

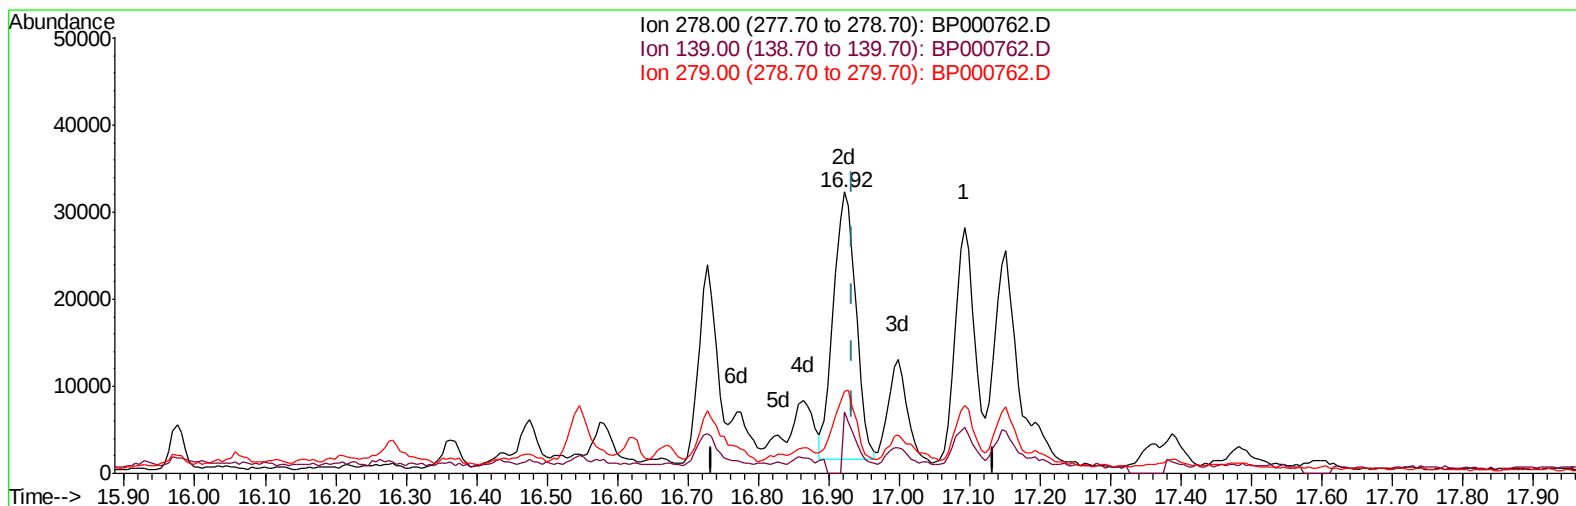

TIC: BP000762.D

(93) Dibenzo(a,h)anthracene

16.922min (-0.012) 1.86ng/ul m

response 67775

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	21.66#
279.00	24.00	29.03#
0.00	0.00	0.00