
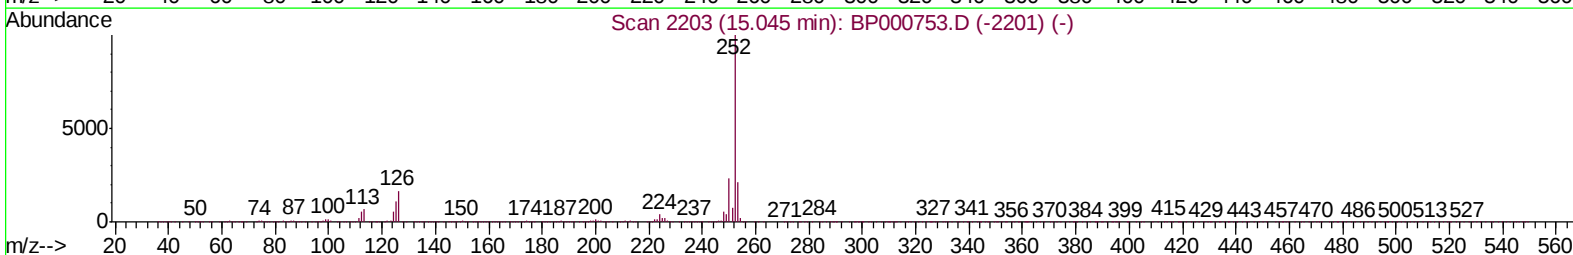
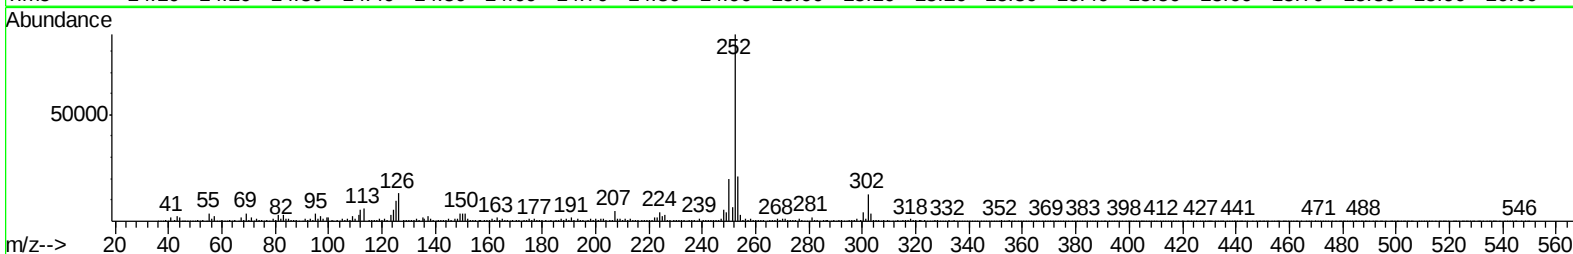


Data File : BP000767.D
Acq On : 15 Oct 2019 15:45
Operator : JU
Sample : K5175-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 16 02:28:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 02:22:01 2019
Response via : Initial Calibration

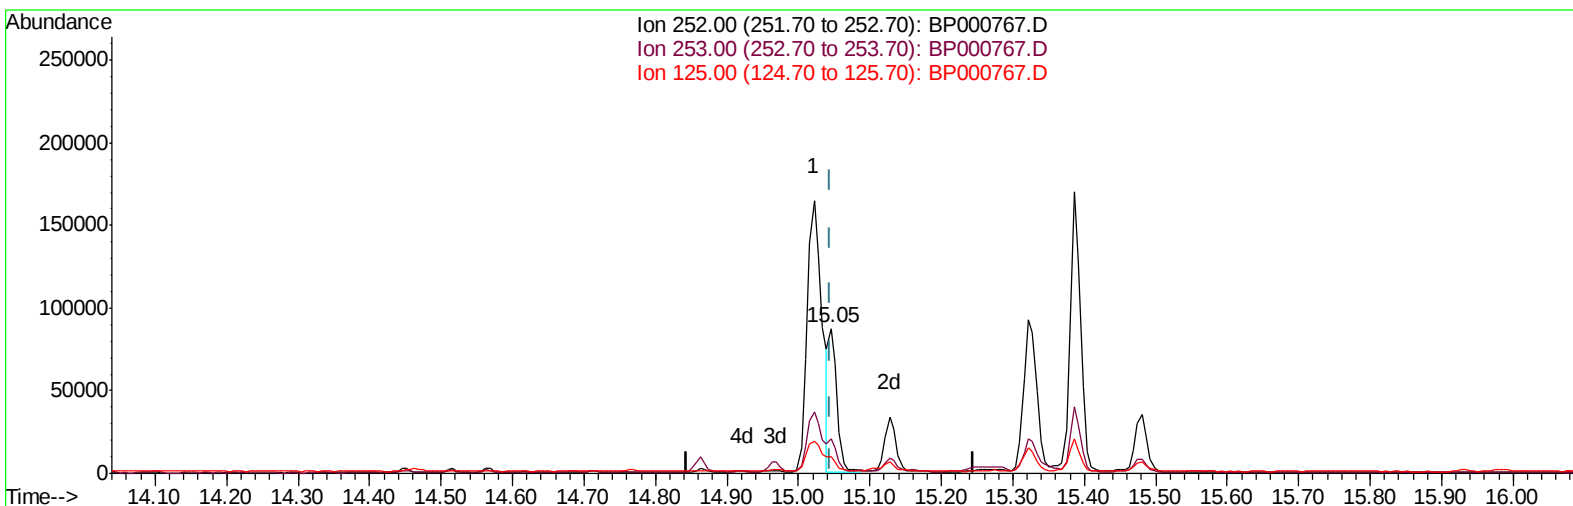

TIC: BP000767.D

(89) Benzo(k)fluoranthene

15.045min (+0.000) 1.64ng/ul m

response 65466

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	24.07
125.00	10.30	11.14
0.00	0.00	0.00