
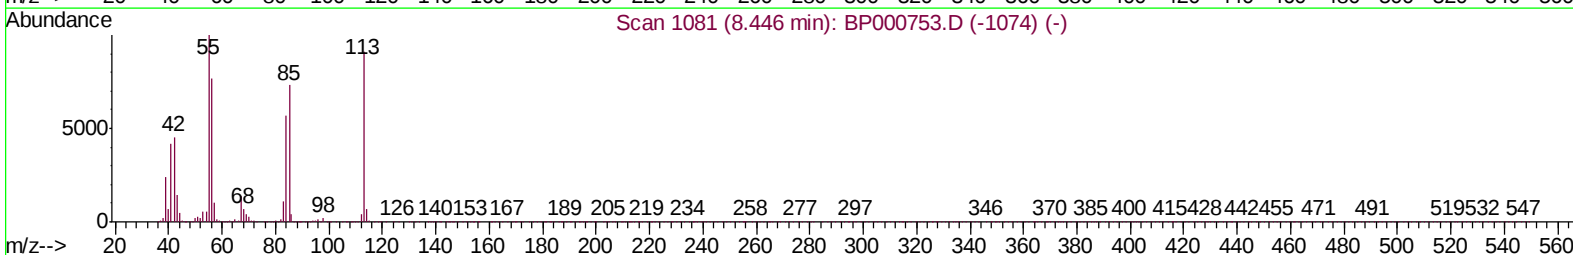
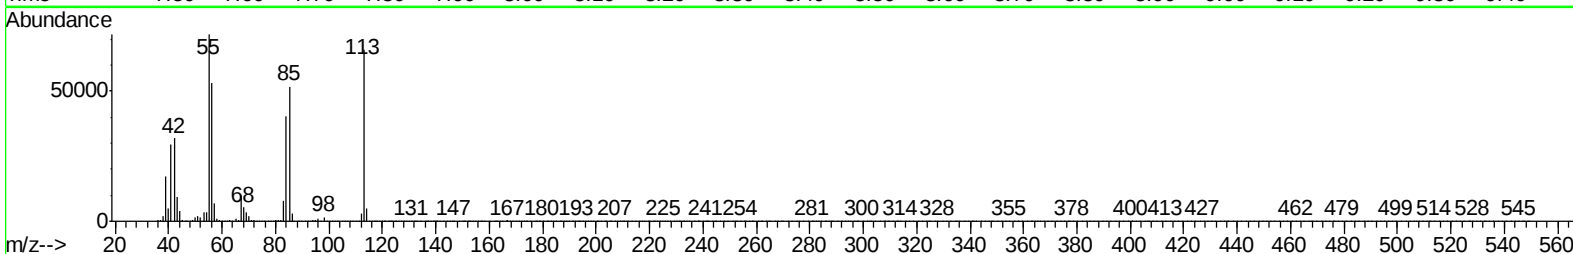


Data File : BP000775.D
Acq On : 15 Oct 2019 18:58
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 16 02:41:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 02:22:01 2019
Response via : Initial Calibration

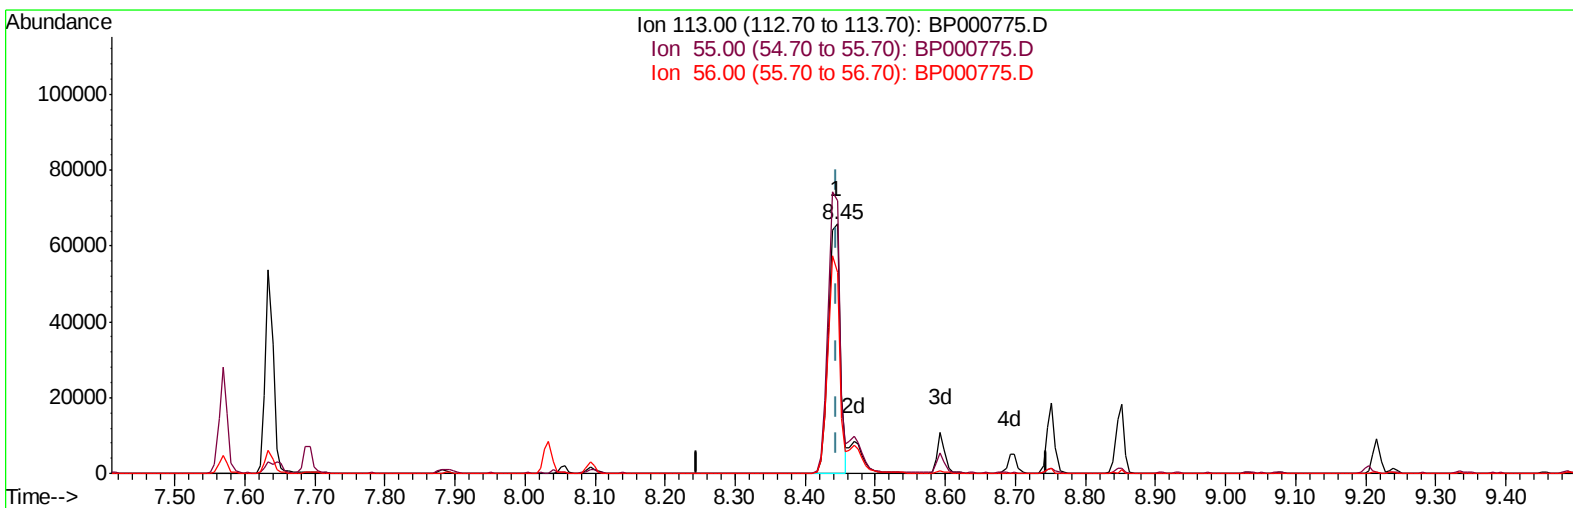

TIC: BP000775.D

(32) Caprolactam

8.446min (+0.000) 16.94ng/ul

response 75569

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	109.30
56.00	86.80	80.86
0.00	0.00	0.00