

Data File : BP000775.D

Acq On : 15 Oct 2019 18:58

Operator : JU

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Oct 16 02:41:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Oct 16 02:22:01 2019

Response via : Initial Calibration

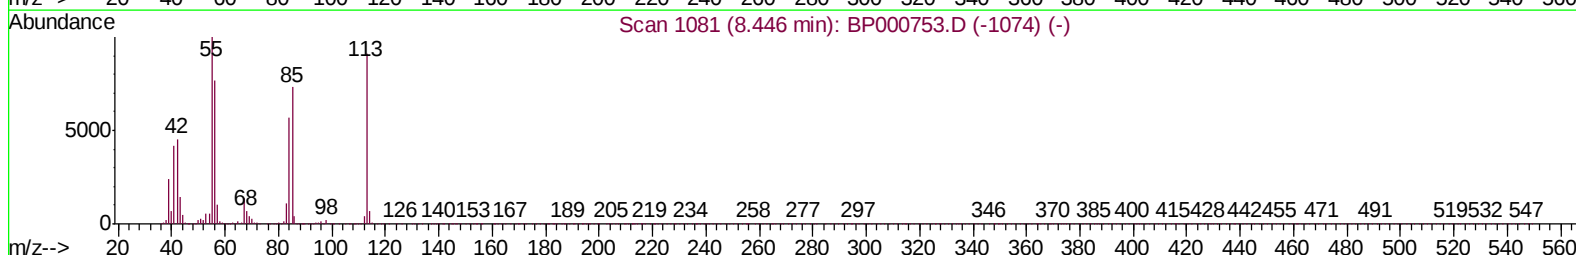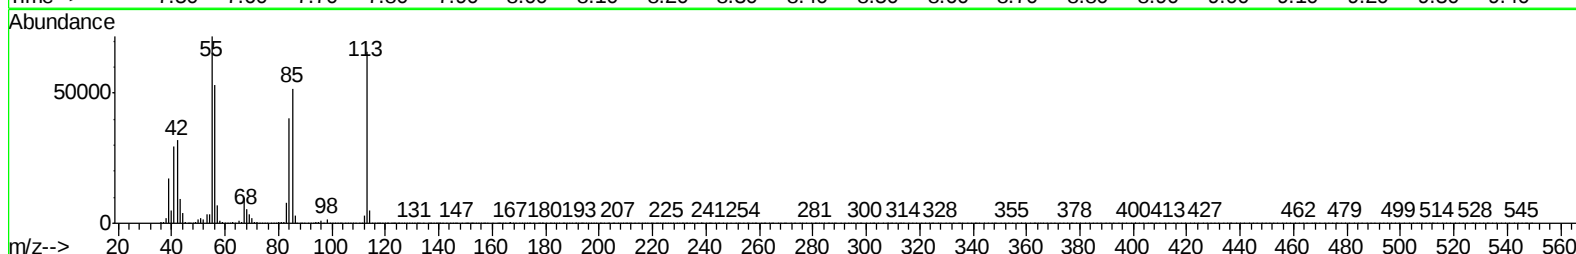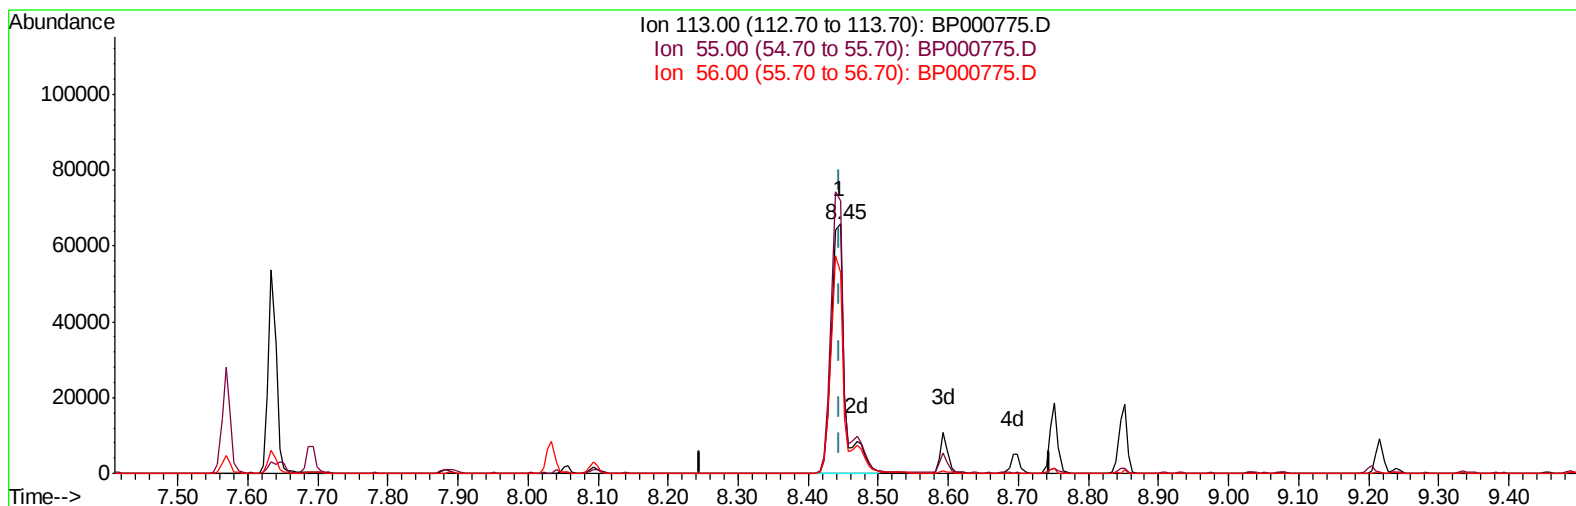

TIC: BP000775.D

(32) Caprolactam

8.446min (+0.000) 19.52ng/ul m

response 87114

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	109.30
56.00	86.80	80.86
0.00	0.00	0.00