

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
 Data File : BP000765.D
 Acq On : 15 Oct 2019 14:57
 Operator : JU
 Sample : K5175-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEPG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	44	47	56	rBV	47261	67000	1.98%	0.162%
2	3.517	238	243	255	rVB	9205	17662	0.52%	0.043%
3	3.675	262	270	274	rVB5	4130	7990	0.24%	0.019%
4	3.722	274	278	281	rBV	12383	16953	0.50%	0.041%
5	3.758	281	284	289	rVB	8646	11944	0.35%	0.029%
6	4.917	477	481	486	rBV	68357	68399	2.02%	0.165%
7	5.705	613	615	622	rBV	3947	4993	0.15%	0.012%
8	6.058	673	675	677	rBV	8149	7490	0.22%	0.018%
9	6.387	727	731	736	rBV	1296141	1256914	37.08%	3.040%
10	6.434	736	739	750	rVB	1145101	1018945	30.06%	2.464%
11	6.522	750	754	757	rBV	1478064	1311156	38.68%	3.171%
12	6.593	762	766	774	rVB2	11191	14850	0.44%	0.036%
13	6.746	789	792	796	rBV	1243891	1120586	33.06%	2.710%
14	6.816	801	804	811	rVB2	11010	11713	0.35%	0.028%
15	7.134	854	858	871	rBV	1406010	1233178	36.38%	2.982%
16	7.305	884	887	891	rBV	1362102	1122575	33.12%	2.715%
17	7.352	894	895	899	rVB2	5471	4889	0.14%	0.012%
18	7.522	920	924	928	rBV	24621	21859	0.64%	0.053%
19	7.634	939	943	954	rBV	1179713	920423	27.15%	2.226%
20	7.775	963	967	972	rVB5	5228	5582	0.16%	0.013%
21	7.846	976	979	982	rBV	26476	19397	0.57%	0.047%
22	7.881	982	985	994	rBV	1751690	1461567	43.12%	3.535%
23	8.034	1007	1011	1014	rBV	1788598	1460259	43.08%	3.531%
24	8.093	1018	1021	1043	rVB	1742468	1383162	40.80%	3.345%
25	8.540	1094	1097	1100	rVB	6167	5074	0.15%	0.012%
26	8.716	1124	1127	1131	rBV	27626	24339	0.72%	0.059%
27	8.810	1139	1143	1148	rVB2	3971	5500	0.16%	0.013%
28	8.987	1168	1173	1177	rBV2	4992	5456	0.16%	0.013%
29	9.105	1190	1193	1200	rVB2	5329	5859	0.17%	0.014%
30	9.205	1206	1210	1211	rBV2	5534	6051	0.18%	0.015%
31	9.234	1214	1215	1218	rVV	6019	5235	0.15%	0.013%
32	9.269	1218	1221	1226	rVB3	3571	6238	0.18%	0.015%
33	9.452	1249	1252	1255	rBV3	6369	6828	0.20%	0.017%
34	9.487	1255	1258	1260	rBV	2249816	1864527	55.01%	4.509%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
 Data File : BP000765.D
 Acq On : 15 Oct 2019 14:57
 Operator : JU
 Sample : K5175-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEPG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	9.510	1260	1262	1265	rVB	884409	609495	17.98%	1.474%
36	9.640	1281	1284	1288	rBV	3114096	2515608	74.21%	6.084%
37	9.799	1307	1311	1314	rBV	1903848	1707150	50.36%	4.128%
38	9.910	1327	1330	1340	rBV	505055	559832	16.52%	1.354%
39	10.005	1344	1346	1354	rVB2	64298	60732	1.79%	0.147%
40	10.210	1377	1381	1384	rBV2	7848	10243	0.30%	0.025%
41	10.240	1384	1386	1389	rVB	9875	6821	0.20%	0.016%
42	10.316	1396	1399	1403	rBV	3365199	2901527	85.60%	7.017%
43	10.393	1408	1412	1419	rBV	501401	459783	13.56%	1.112%
44	10.446	1419	1421	1429	rVV	51165	52419	1.55%	0.127%
45	10.693	1460	1463	1465	rBV2	4534	4828	0.14%	0.012%
46	10.716	1465	1467	1469	rVV	9126	8031	0.24%	0.019%
47	10.746	1469	1472	1476	rVB	16038	15208	0.45%	0.037%
48	11.034	1518	1521	1529	rVB	35365	31500	0.93%	0.076%
49	11.110	1531	1534	1537	rVB2	8179	7450	0.22%	0.018%
50	11.169	1541	1544	1547	rBV	11555	12177	0.36%	0.029%
51	11.251	1555	1558	1561	rBV4	5156	6204	0.18%	0.015%
52	11.293	1561	1565	1568	rBV	2166052	1778232	52.46%	4.300%
53	11.316	1568	1569	1571	rVB	36682	20386	0.60%	0.049%
54	11.351	1571	1575	1578	rBV	3424107	2812637	82.98%	6.802%
55	11.410	1583	1585	1592	rVB7	12645	13738	0.41%	0.033%
56	11.528	1600	1605	1612	rBV3	14744	32532	0.96%	0.079%
57	11.699	1630	1634	1637	rVB3	5363	6547	0.19%	0.016%
58	11.763	1642	1645	1648	rBV5	4802	7036	0.21%	0.017%
59	11.804	1649	1652	1654	rBV	5576	5398	0.16%	0.013%
60	11.840	1654	1658	1662	rBV2	90803	102329	3.02%	0.247%
61	11.916	1668	1671	1673	rBV2	9443	7775	0.23%	0.019%
62	12.016	1685	1688	1690	rBV2	9700	11823	0.35%	0.029%
63	12.093	1699	1701	1702	rBV	9963	8084	0.24%	0.020%
64	12.363	1744	1747	1749	rBV	7481	7423	0.22%	0.018%
65	12.404	1752	1754	1758	rVB3	8952	10056	0.30%	0.024%
66	12.451	1759	1762	1765	rVB5	8329	9945	0.29%	0.024%
67	12.504	1767	1771	1772	rBV	41241	37915	1.12%	0.092%
68	12.522	1772	1774	1777	rVB	80102	60868	1.80%	0.147%
69	12.634	1788	1793	1795	rBV3	7422	12754	0.38%	0.031%
70	12.663	1795	1798	1804	rVV	41516	46198	1.36%	0.112%
71	12.734	1806	1810	1816	rVV	3545767	3389609	100.00%	8.197%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
 Data File : BP000765.D
 Acq On : 15 Oct 2019 14:57
 Operator : JU
 Sample : K5175-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEPG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

72	12.781	1816	1818	1820	rVV	14696	15244	0.45%	0.037%
73	12.804	1820	1822	1827	rVB4	10096	12898	0.38%	0.031%
74	12.875	1832	1834	1836	rVV	5548	4962	0.15%	0.012%
75	12.898	1836	1838	1846	rVB2	6738	12183	0.36%	0.029%
76	13.087	1868	1870	1873	rVB	13181	11933	0.35%	0.029%
77	13.122	1873	1876	1878	rBV4	12494	15961	0.47%	0.039%
78	13.146	1878	1880	1885	rVV2	21017	25791	0.76%	0.062%
79	13.193	1886	1888	1891	rVB2	8789	8083	0.24%	0.020%
80	13.287	1902	1904	1907	rVB	9270	7161	0.21%	0.017%
81	13.316	1907	1909	1914	rVB2	6961	6280	0.19%	0.015%
82	13.393	1920	1922	1928	rVB5	11762	13250	0.39%	0.032%
83	13.493	1936	1939	1942	rBV	26230	21364	0.63%	0.052%
84	13.604	1956	1958	1965	rVB	8101	8562	0.25%	0.021%
85	13.769	1984	1986	1991	rBV2	8276	10523	0.31%	0.025%
86	13.816	1991	1994	2010	rBV	528815	699324	20.63%	1.691%
87	13.969	2016	2020	2024	rBV	2128919	1938272	57.18%	4.687%
88	14.145	2047	2050	2054	rBV	72021	75500	2.23%	0.183%
89	14.457	2100	2103	2111	rBV2	114798	153738	4.54%	0.372%
90	14.769	2152	2156	2163	rBV	108894	119316	3.52%	0.289%
91	14.840	2165	2168	2176	rVB	193476	187252	5.52%	0.453%
92	14.969	2187	2190	2194	rVB	44501	45677	1.35%	0.110%
93	15.022	2195	2199	2202	rBV	45168	65912	1.94%	0.159%
94	15.104	2210	2213	2225	rBV2	133018	184001	5.43%	0.445%
95	15.357	2251	2256	2266	rVB	2671410	3389708	100.00%	8.198%
96	15.445	2266	2271	2276	rVV	1553127	1980679	58.43%	4.790%
97	15.487	2276	2278	2287	rVB	127402	169961	5.01%	0.411%
98	15.928	2349	2353	2358	rBV	102382	147582	4.35%	0.357%
99	15.981	2359	2362	2364	rBV3	31174	44082	1.30%	0.107%
100	16.434	2435	2439	2452	rVB2	61354	120384	3.55%	0.291%


Sum of corrected areas: 41350469

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
Data File : BP000765.D
Acq On : 15 Oct 2019 14:57
Operator : JU
Sample : K5175-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
BEPG1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

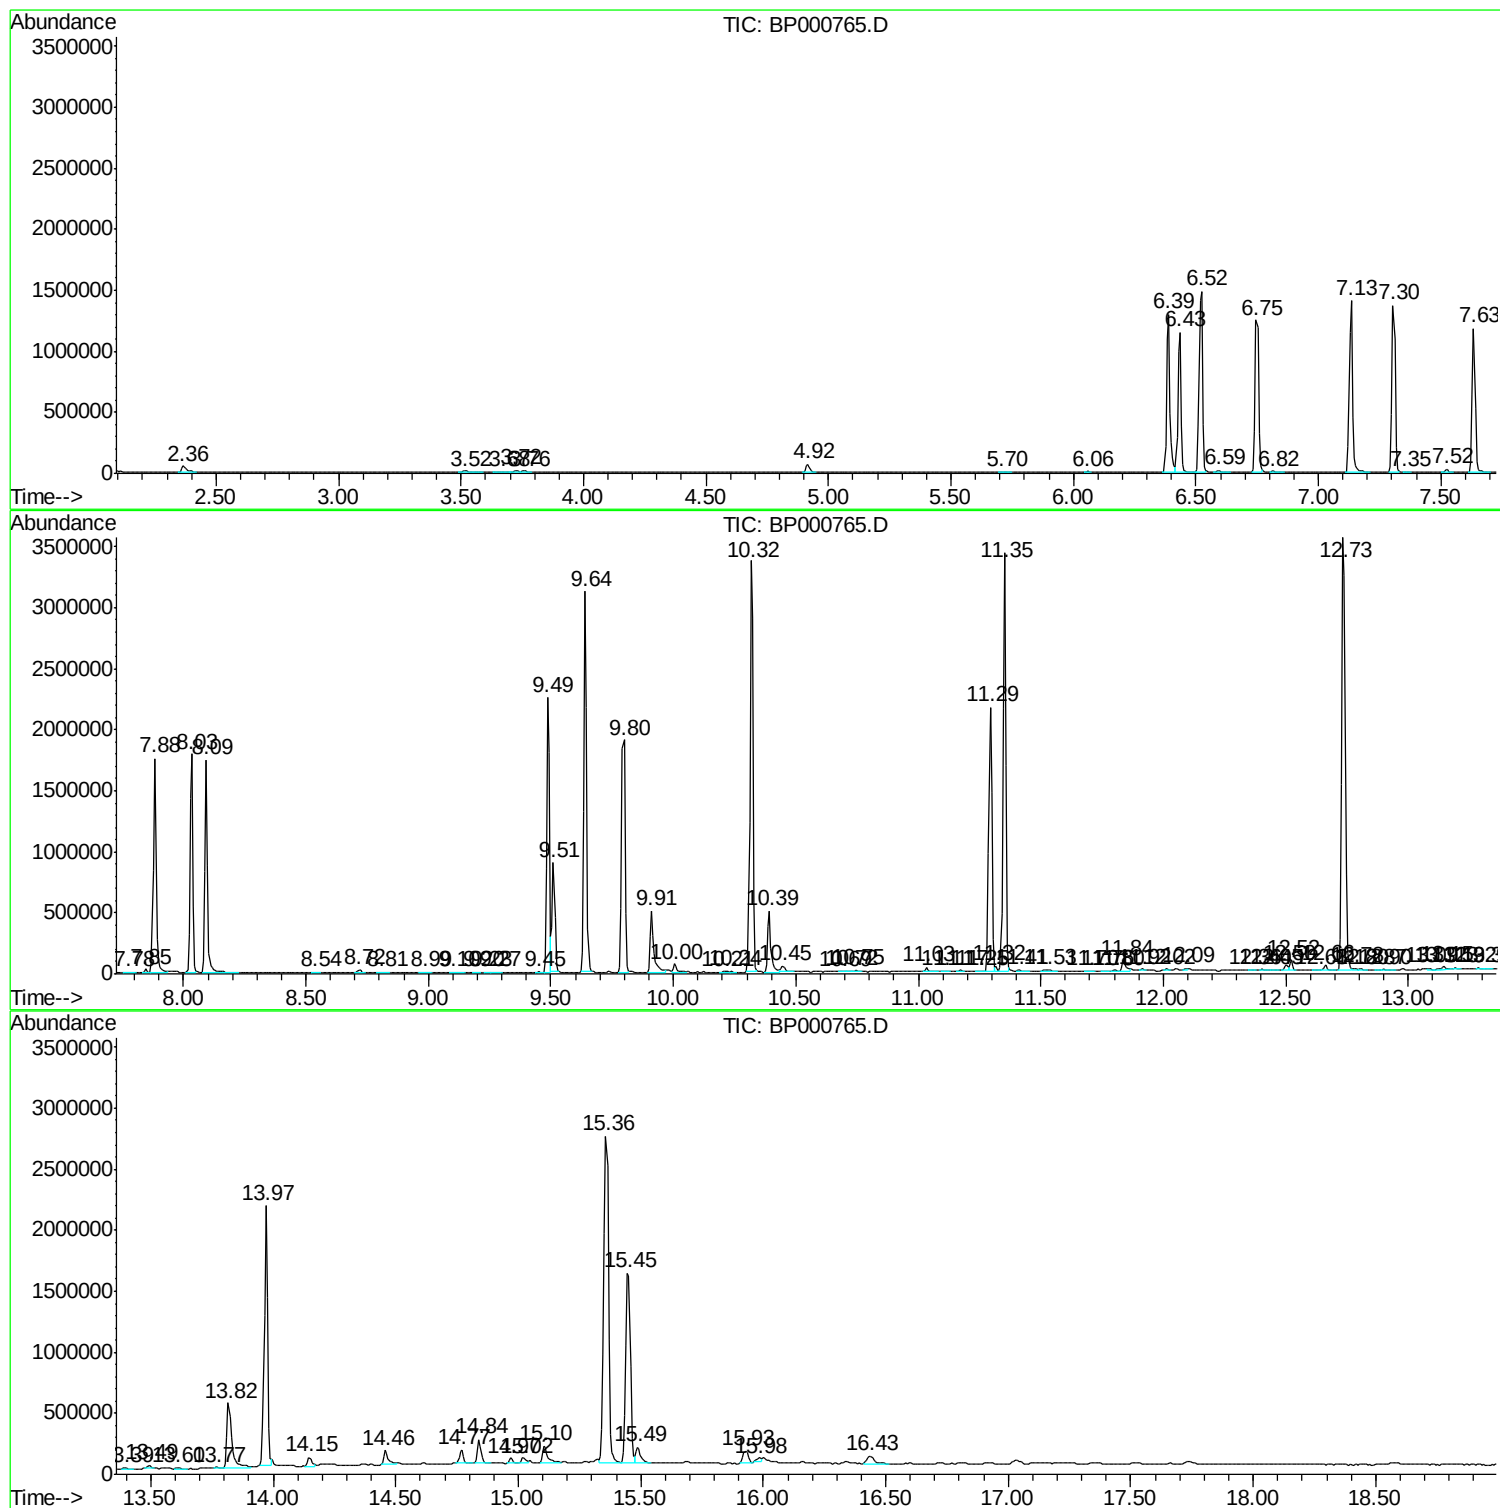

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
Data File : BP000765.D
Acq On : 15 Oct 2019 14:57
Operator : JU
Sample : K5175-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BEPG1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic13.82 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.82	7.22 ng/ul	699324	Chrysene-d12	13.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentadecane	210	C15H30	000295-48-7	95
2		1-Nonadecene	266	C19H38	018435-45-5	94
3		1-Heneicosyl formate	340	C22H44O2	077899-03-7	93
4		2-Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	93
5		3-Eicosene, (E)-	280	C20H40	074685-33-9	91

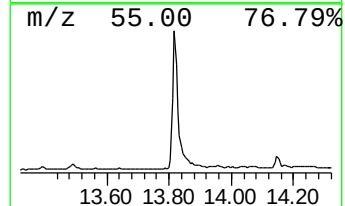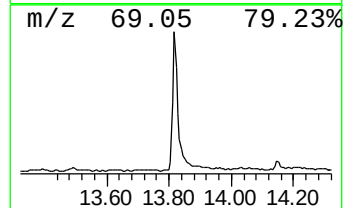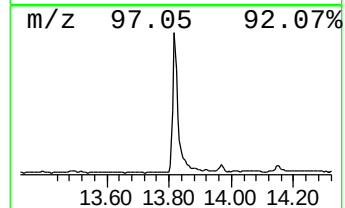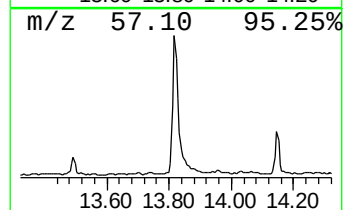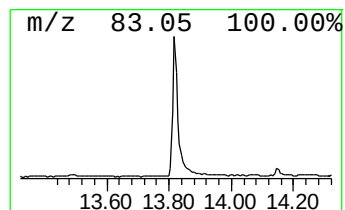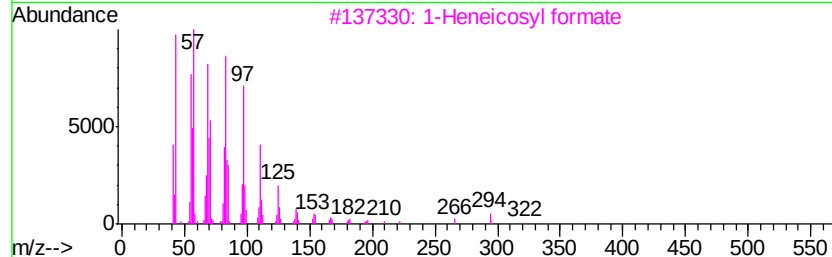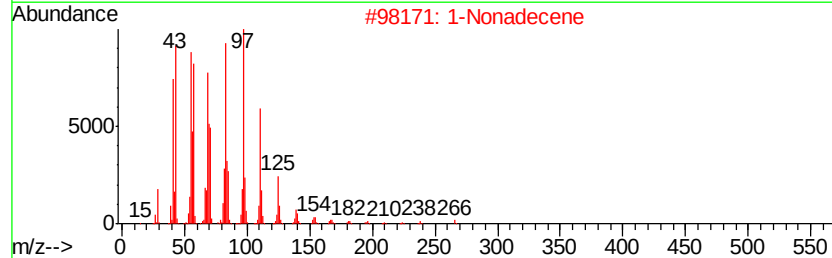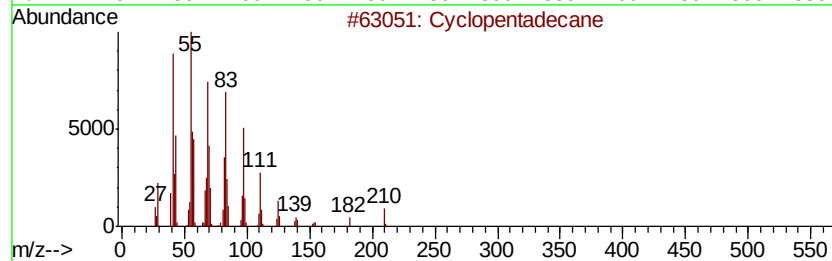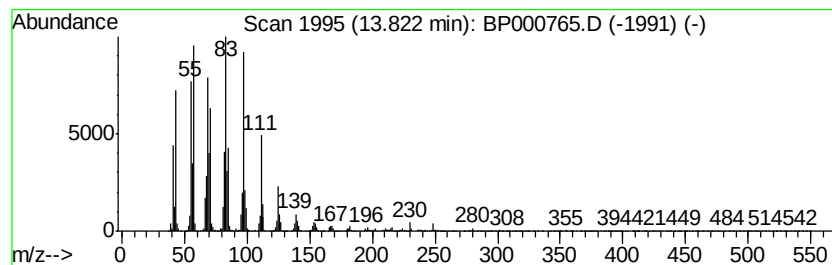

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101619\
Data File : BP000765.D
Acq On : 15 Oct 2019 14:57
Operator : JU
Sample : K5175-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BEPG1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	13.82	7.2	ng/ul	699324	5	13.97	1938270	20.0