

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
 Data File : BP000796.D
 Acq On : 16 Oct 2019 03:26
 Operator : JU
 Sample : PB123690BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	43	47	58	rBV	44741	63119	2.21%	0.179%
2	3.758	280	284	290	rVB	6606	9282	0.33%	0.026%
3	5.005	492	496	502	rBV4	1541	3270	0.11%	0.009%
4	6.387	727	731	735	rBV	1207429	1024941	35.93%	2.903%
5	6.434	735	739	750	rVV	905181	879037	30.81%	2.490%
6	6.522	750	754	768	rVB	1282217	1164090	40.80%	3.298%
7	6.746	789	792	810	rVB	1227549	1093295	38.32%	3.097%
8	7.134	854	858	872	rBV	1611969	1335608	46.82%	3.783%
9	7.304	884	887	891	rBV	1121620	949433	33.28%	2.689%
10	7.634	940	943	956	rVB	1008727	773936	27.13%	2.192%
11	7.881	982	985	1007	rBV	1569738	1327395	46.53%	3.760%
12	8.034	1007	1011	1014	rVV	1786166	1444635	50.64%	4.092%
13	8.093	1018	1021	1046	rVB	1650100	1306316	45.79%	3.700%
14	8.716	1124	1127	1137	rBV	19542	22368	0.78%	0.063%
15	9.487	1255	1258	1261	rBV	2019493	1630589	57.16%	4.619%
16	9.640	1280	1284	1288	rBV	2714893	2210297	77.48%	6.261%
17	9.798	1307	1311	1314	rBV	1983723	1761432	61.74%	4.990%
18	9.910	1327	1330	1345	rBV	507490	599185	21.00%	1.697%
19	10.004	1345	1346	1355	rVB6	8039	9902	0.35%	0.028%
20	10.210	1377	1381	1387	rVB2	3135	4195	0.15%	0.012%
21	10.316	1396	1399	1403	rBV	3018555	2555847	89.59%	7.240%
22	10.393	1408	1412	1418	rBV	456024	410713	14.40%	1.163%
23	10.445	1418	1421	1431	rVB	45257	47189	1.65%	0.134%
24	10.745	1469	1472	1477	rVB	12291	11362	0.40%	0.032%
25	11.110	1531	1534	1538	rVB	6323	5452	0.19%	0.015%
26	11.169	1541	1544	1550	rVB	6997	7426	0.26%	0.021%
27	11.293	1561	1565	1569	rBV	2205201	1885743	66.10%	5.342%
28	11.351	1571	1575	1579	rBV	3167522	2558145	89.67%	7.247%
29	11.516	1600	1603	1609	rVB	3237	3918	0.14%	0.011%
30	12.022	1685	1689	1691	rBV3	3655	5287	0.19%	0.015%
31	12.110	1702	1704	1709	rVB6	2587	3505	0.12%	0.010%
32	12.504	1767	1771	1776	rBV	30982	29316	1.03%	0.083%
33	12.657	1794	1797	1802	rBV	26692	26930	0.94%	0.076%
34	12.734	1806	1810	1814	rBV	3138297	2852833	100.00%	8.081%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
Data File : BP000796.D
Acq On : 16 Oct 2019 03:26
Operator : JU
Sample : PB123690BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

35	13.439	1928	1930	1933	rBV4	7897	9449	0.33%	0.027%
36	13.822	1988	1995	1998	rBV4	53513	117259	4.11%	0.332%
37	13.969	2016	2020	2024	rBV	2100962	1850424	64.86%	5.242%
38	14.145	2048	2050	2053	rVB2	12253	9830	0.34%	0.028%
39	14.457	2100	2103	2109	rVB2	26320	29385	1.03%	0.083%
40	14.763	2152	2155	2166	rVB2	62313	84174	2.95%	0.238%
41	14.969	2187	2190	2193	rBV	36699	42246	1.48%	0.120%
42	15.104	2209	2213	2226	rVB3	90999	162826	5.71%	0.461%
43	15.357	2251	2256	2265	rVB	2255571	2714354	95.15%	7.689%
44	15.445	2266	2271	2275	rVV	1634905	1891387	66.30%	5.358%
45	15.486	2275	2278	2291	rVB	90598	140790	4.94%	0.399%
46	15.922	2348	2352	2359	rVB	69315	103600	3.63%	0.293%
47	16.433	2434	2439	2453	rVB	65780	129837	4.55%	0.368%


Sum of corrected areas: 35301552

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101619\
Data File : BP000796.D
Acq On : 16 Oct 2019 03:26
Operator : JU
Sample : PB123690BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

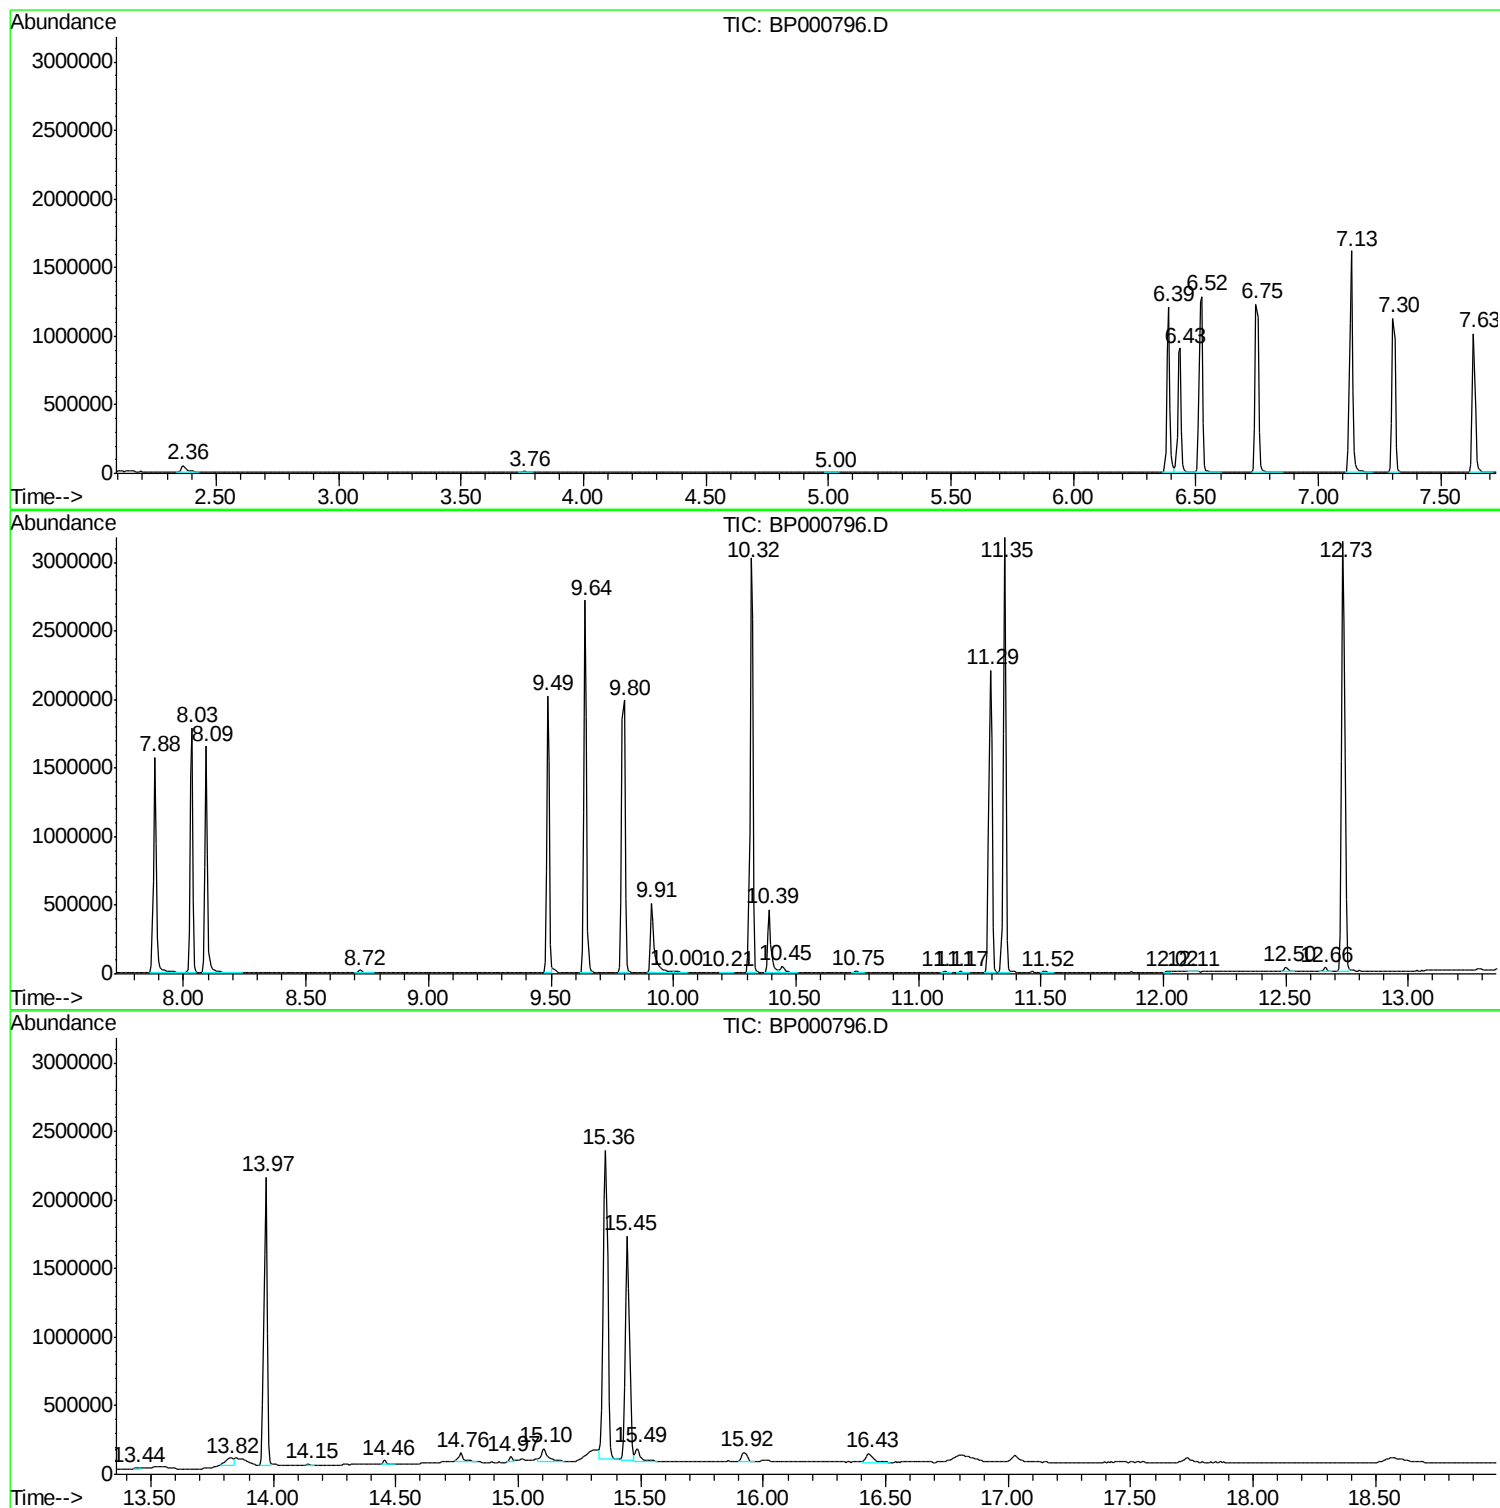

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101619\
Data File : BP000796.D
Acq On : 16 Oct 2019 03:26
Operator : JU
Sample : PB123690BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101619\
Data File : BP000796.D
Acq On : 16 Oct 2019 03:26
Operator : JU
Sample : PB123690BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc