

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
 Data File : BP017675.D
 Acq On : 16 Oct 2023 10:33
 Operator : MA/JU
 Sample : PB156260BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	41	rVB	37293	56187	1.47%	0.178%
2	3.693	100	103	124	rBV	398933	625565	16.38%	1.986%
3	3.999	152	155	160	rBV4	7761	10108	0.26%	0.032%
4	4.481	235	237	241	rBV5	2997	4134	0.11%	0.013%
5	5.122	344	346	351	rBV6	2885	3891	0.10%	0.012%
6	6.228	530	534	537	rBV5	3152	6033	0.16%	0.019%
7	7.058	669	675	693	rVV	478145	782219	20.49%	2.483%
8	7.246	700	707	719	rBV	404118	629688	16.49%	1.999%
9	7.422	730	737	751	rBV	521794	859242	22.50%	2.728%
10	7.593	762	766	770	rVB7	2943	5086	0.13%	0.016%
11	7.899	812	818	828	rBV	405189	658217	17.24%	2.090%
12	8.622	934	941	958	rBV	564456	973582	25.50%	3.091%
13	9.052	1012	1014	1017	rBV4	3443	3867	0.10%	0.012%
14	9.111	1017	1024	1039	rVV	462521	789402	20.68%	2.506%
15	9.828	1139	1146	1161	rBV	390592	652550	17.09%	2.072%
16	10.357	1228	1236	1258	rBV	488314	974937	25.53%	3.095%
17	10.740	1293	1301	1310	rBV	529319	883014	23.13%	2.803%
18	10.910	1323	1330	1348	rBV	547603	1010257	26.46%	3.207%
19	12.352	1569	1575	1578	rBV6	8139	14278	0.37%	0.045%
20	13.440	1756	1760	1765	rVB6	8225	13449	0.35%	0.043%
21	14.022	1850	1859	1880	rBV	1007745	1479196	38.74%	4.696%
22	14.157	1880	1882	1885	rVV4	4019	5383	0.14%	0.017%
23	14.298	1899	1906	1922	rBV	1106835	1671453	43.78%	5.306%
24	14.504	1939	1941	1946	rVB6	4201	4045	0.11%	0.013%
25	14.604	1951	1958	1968	rBV	786130	1143306	29.94%	3.630%
26	14.857	1996	2001	2021	rBV	232765	638377	16.72%	2.027%
27	15.610	2122	2129	2139	rBV	1504943	2183723	57.19%	6.932%
28	15.757	2147	2154	2165	rBV	361751	592239	15.51%	1.880%
29	17.063	2373	2376	2380	rBV6	3712	5264	0.14%	0.017%
30	17.187	2393	2397	2402	rVB8	3368	5787	0.15%	0.018%
31	17.398	2426	2433	2444	rBV	1018641	1462731	38.31%	4.644%
32	17.498	2444	2450	2465	rVV	1794204	2507619	65.68%	7.961%
33	17.816	2501	2504	2506	rBV4	3227	5111	0.13%	0.016%
34	18.481	2614	2617	2618	rBV3	3605	4645	0.12%	0.015%
35	19.322	2758	2760	2764	rVB3	20699	23668	0.62%	0.075%
36	19.398	2769	2773	2780	rBV4	24984	39867	1.04%	0.127%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017675.D
Acq On : 16 Oct 2023 10:33
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	19.757	2828	2834	2848	rBV	2487491	3201686	83.85%	10.164%
38	21.539	3133	3137	3147	rBV	1274697	1783094	46.70%	5.661%
39	23.945	3538	3546	3558	rBV2	1802640	3818141	100.00%	12.121%
40	24.116	3568	3575	3591	rBV	901351	1968760	51.56%	6.250%




Sum of corrected areas: 31499801

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017675.D
Acq On : 16 Oct 2023 10:33
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

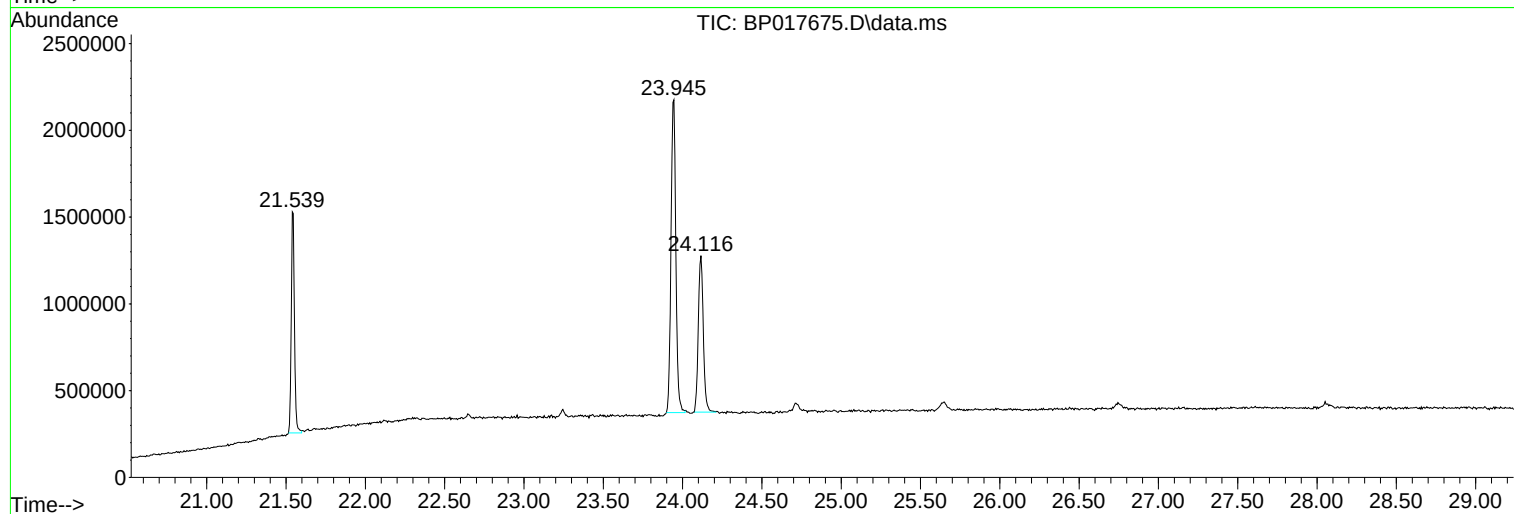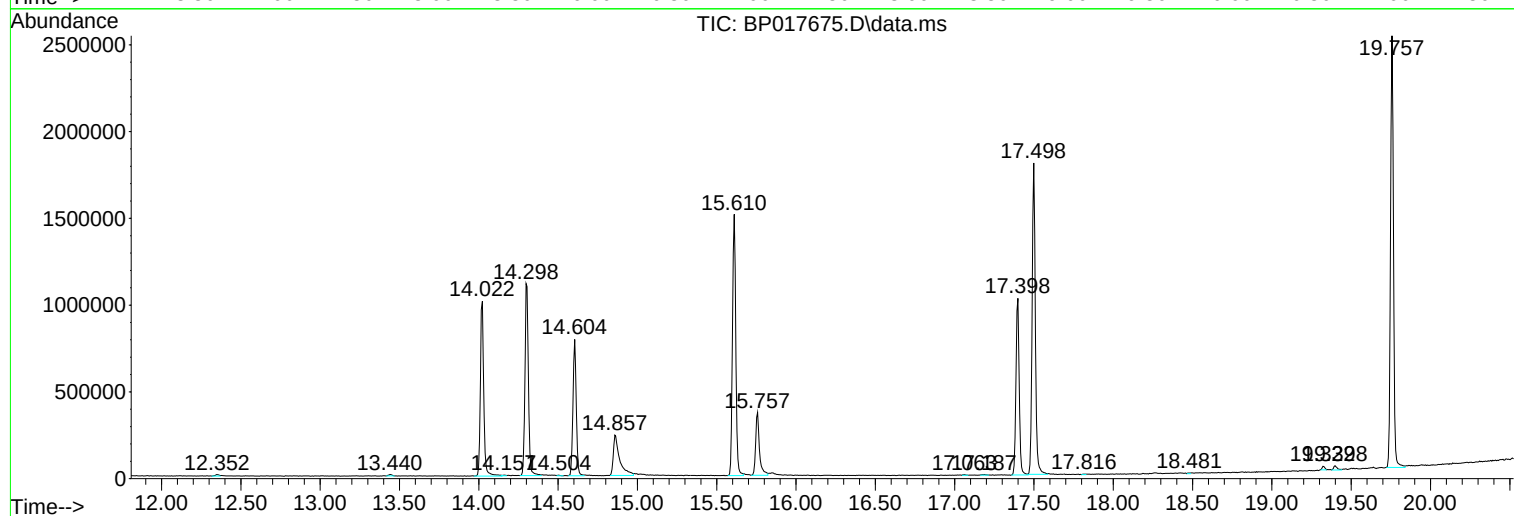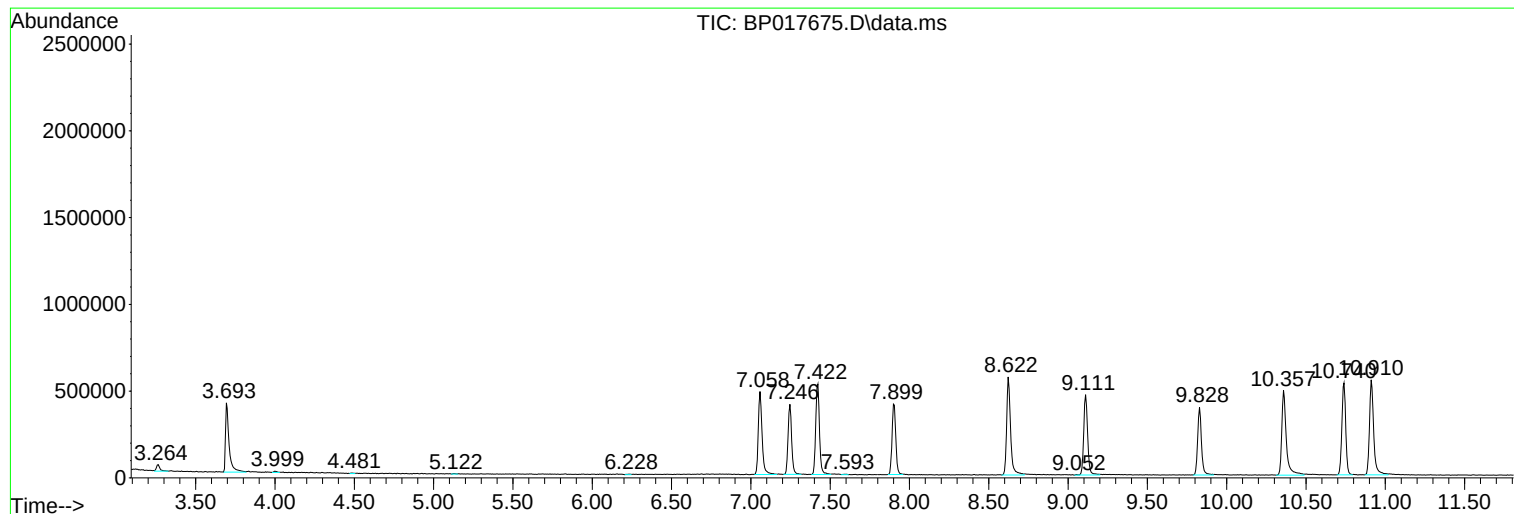

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017675.D
Acq On : 16 Oct 2023 10:33
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017675.D
Acq On : 16 Oct 2023 10:33
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc