

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
 Data File : BP017682.D
 Acq On : 16 Oct 2023 15:05
 Operator : MA/JU
 Sample : PB156264BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	26	30	38	rVB	41401	56024	1.49%	0.163%
2	3.699	100	104	124	rBV	410062	671269	17.80%	1.948%
3	3.999	153	155	161	rVB4	8082	11009	0.29%	0.032%
4	5.340	379	383	386	rBV6	2692	4758	0.13%	0.014%
5	5.875	471	474	479	rBV7	3109	4964	0.13%	0.014%
6	7.057	669	675	694	rBV	526804	869934	23.06%	2.524%
7	7.246	700	707	718	rBV	443541	676113	17.92%	1.962%
8	7.422	730	737	748	rBV	551976	894569	23.71%	2.595%
9	7.898	812	818	832	rVB	459276	759219	20.13%	2.203%
10	8.328	886	891	894	rVB6	3799	4490	0.12%	0.013%
11	8.622	935	941	958	rBV	602882	1039307	27.55%	3.015%
12	9.110	1016	1024	1032	rBV	508484	840076	22.27%	2.437%
13	9.769	1133	1136	1140	rBV6	2598	4309	0.11%	0.013%
14	9.828	1140	1146	1157	rBV	425349	703516	18.65%	2.041%
15	10.357	1228	1236	1257	rBV	536842	1063664	28.20%	3.086%
16	10.740	1293	1301	1311	rBV	618863	1028217	27.26%	2.983%
17	10.910	1323	1330	1349	rBV	591969	1096034	29.06%	3.180%
18	12.351	1567	1575	1583	rBV	8509	19413	0.51%	0.056%
19	12.975	1679	1681	1688	rVB8	2013	4007	0.11%	0.012%
20	13.439	1754	1760	1766	rBV3	12898	23692	0.63%	0.069%
21	14.022	1850	1859	1876	rBV	1145369	1625131	43.08%	4.715%
22	14.304	1899	1907	1925	rBV	1184451	1820893	48.27%	5.283%
23	14.604	1951	1958	1969	rBV	932088	1366755	36.23%	3.965%
24	14.857	1995	2001	2031	rBV	239902	718695	19.05%	2.085%
25	15.610	2122	2129	2139	rBV	1722025	2413425	63.98%	7.002%
26	15.757	2148	2154	2167	rBV	389515	632785	16.77%	1.836%
27	17.039	2370	2372	2374	rBV2	3270	4283	0.11%	0.012%
28	17.186	2394	2397	2405	rBV8	4853	9207	0.24%	0.027%
29	17.398	2427	2433	2444	rBV	1236677	1718286	45.55%	4.985%
30	17.498	2444	2450	2468	rVV	1941504	2711022	71.87%	7.865%
31	18.257	2576	2579	2583	rBV6	5988	8727	0.23%	0.025%
32	19.327	2758	2761	2765	rVB3	25146	29088	0.77%	0.084%
33	19.398	2770	2773	2777	rVV3	20860	27253	0.72%	0.079%
34	19.633	2811	2813	2816	rBV4	8045	9027	0.24%	0.026%
35	19.757	2829	2834	2845	rBV	2559415	3360090	89.08%	9.748%
36	21.545	3133	3138	3148	rBV	1572280	2160515	57.27%	6.268%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017682.D
Acq On : 16 Oct 2023 15:05
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	23.945	3539	3546	3558	rVB	1835539	3772201	100.00%	10.944%
38	24.115	3568	3575	3586	rBV	1095480	2306105	61.13%	6.691%




Sum of corrected areas: 34468072

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017682.D
Acq On : 16 Oct 2023 15:05
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

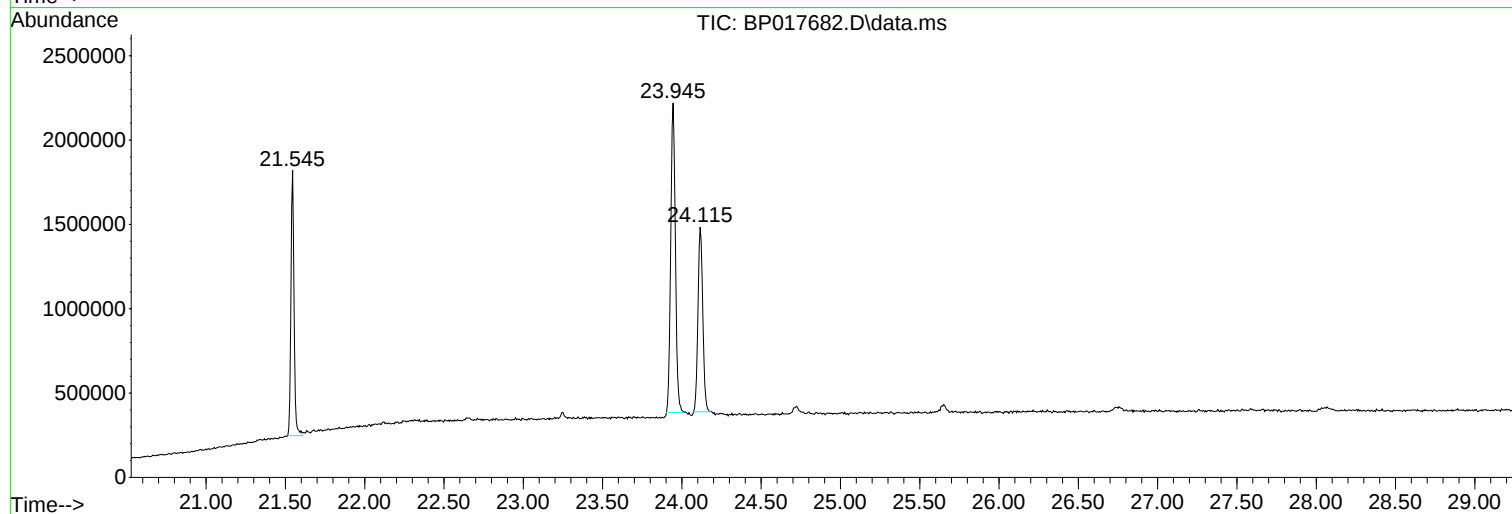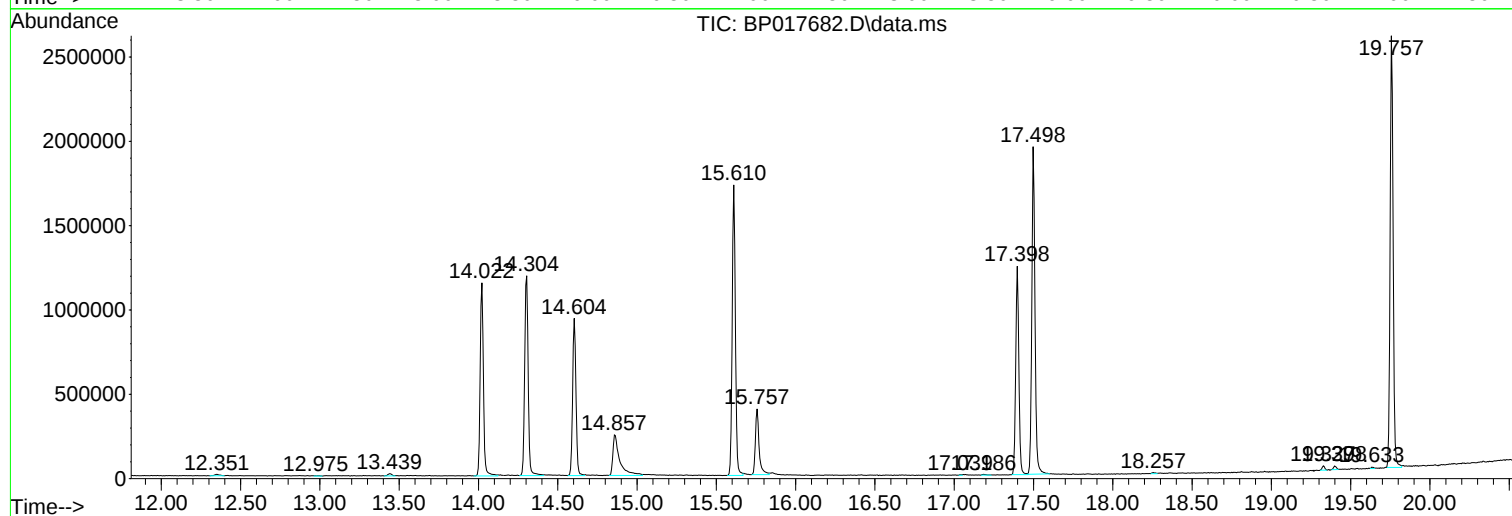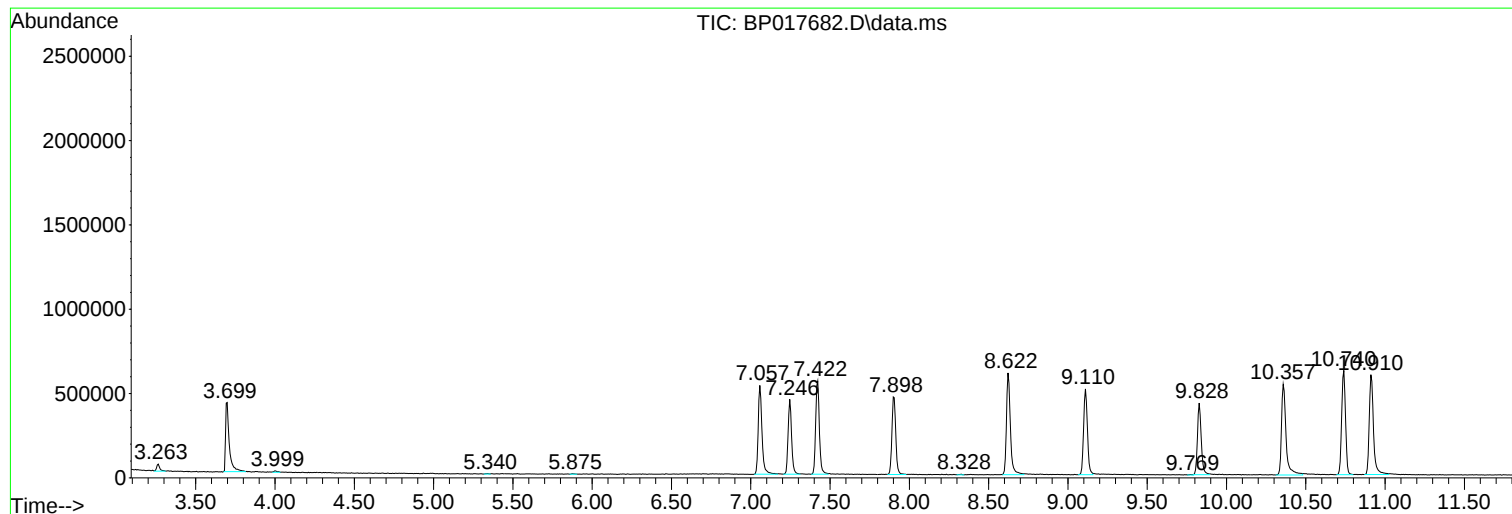

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017682.D
Acq On : 16 Oct 2023 15:05
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017682.D
Acq On : 16 Oct 2023 15:05
Operator : MA/JU
Sample : PB156264BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK264

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------