

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
 Data File : BP017684.D
 Acq On : 16 Oct 2023 16:13
 Operator : MA/JU
 Sample : PB156296BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	35	rBV	39055	43299	0.92%	0.112%
2	3.699	100	104	122	rBV	446308	741620	15.70%	1.922%
3	3.999	153	155	157	rBV3	5601	4890	0.10%	0.013%
4	7.057	668	675	686	rBV	523135	877963	18.58%	2.275%
5	7.246	699	707	720	rBV	445538	706868	14.96%	1.832%
6	7.422	730	737	753	rBV	565602	943488	19.97%	2.445%
7	7.905	812	819	831	rBV	459023	778124	16.47%	2.017%
8	8.622	933	941	960	rBV	638712	1103334	23.35%	2.859%
9	9.110	1016	1024	1033	rBV	536033	889343	18.83%	2.305%
10	9.828	1136	1146	1158	rBV	443146	745065	15.77%	1.931%
11	10.357	1228	1236	1255	rBV	576167	1109107	23.48%	2.874%
12	10.740	1292	1301	1315	rBV	649687	1068501	22.62%	2.769%
13	10.910	1320	1330	1351	rBV	674126	1230488	26.05%	3.189%
14	12.351	1569	1575	1578	rBV6	8658	15231	0.32%	0.039%
15	13.440	1756	1760	1765	rVB8	7145	11004	0.23%	0.029%
16	14.022	1852	1859	1871	rBV	1271765	1761956	37.30%	4.566%
17	14.298	1900	1906	1916	rBV	1337969	1985279	42.02%	5.145%
18	14.604	1952	1958	1974	rBV	1024294	1475854	31.24%	3.825%
19	14.857	1995	2001	2025	rBV	303045	837825	17.73%	2.171%
20	15.610	2121	2129	2143	rBV	1852446	2669750	56.51%	6.919%
21	15.757	2147	2154	2168	rVV	478243	788897	16.70%	2.044%
22	15.851	2168	2170	2174	rVB4	10230	12751	0.27%	0.033%
23	17.398	2426	2433	2444	rBV	1374358	1899854	40.21%	4.924%
24	17.498	2444	2450	2467	rVB	2149857	3043966	64.43%	7.889%
25	18.263	2574	2580	2584	rBV7	9485	20577	0.44%	0.053%
26	18.575	2629	2633	2634	rBV4	4940	6491	0.14%	0.017%
27	19.327	2757	2761	2765	rBV4	23752	32916	0.70%	0.085%
28	19.398	2769	2773	2777	rBV	30006	39846	0.84%	0.103%
29	19.757	2828	2834	2844	rBV	2942028	3851301	81.52%	9.981%
30	21.545	3133	3138	3145	rBV	1779705	2423965	51.31%	6.282%
31	23.945	3538	3546	3557	rBV2	2238899	4724258	100.00%	12.243%
32	24.115	3568	3575	3586	rVB	1350190	2742562	58.05%	7.108%




Sum of corrected areas: 38586373

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017684.D
Acq On : 16 Oct 2023 16:13
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

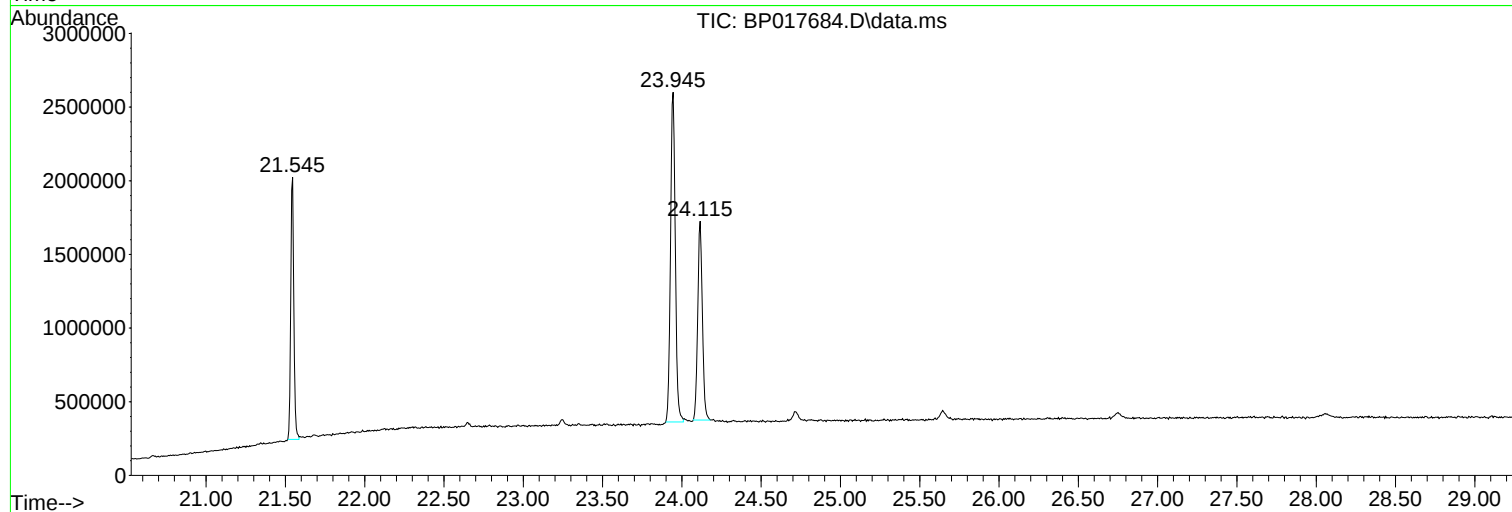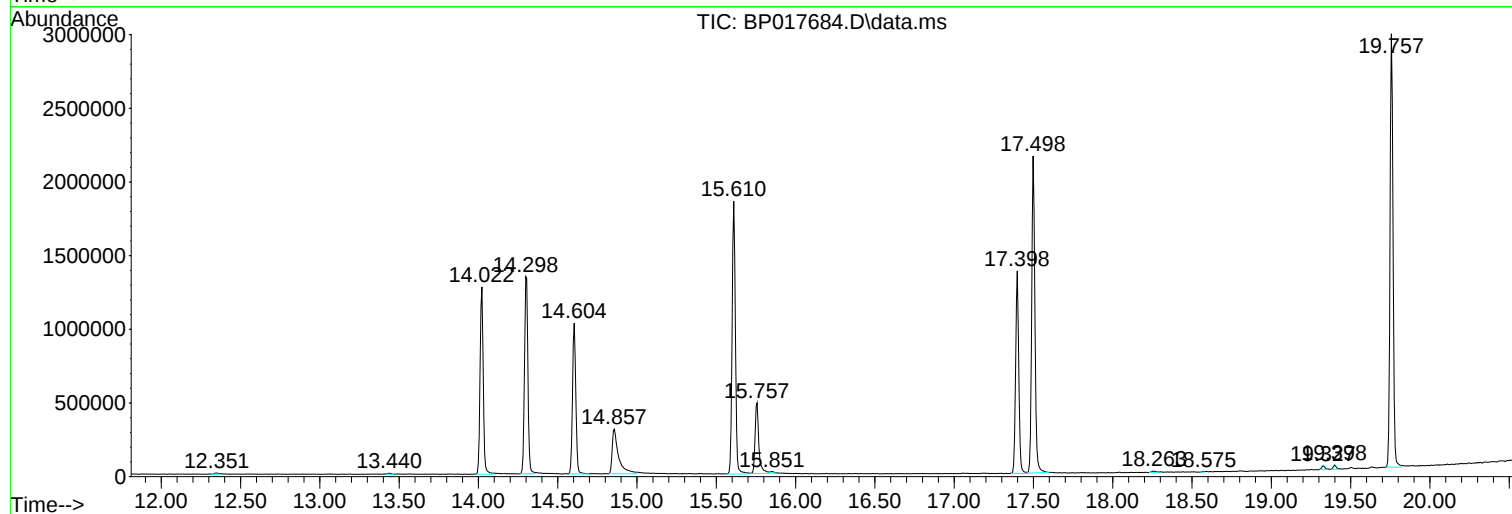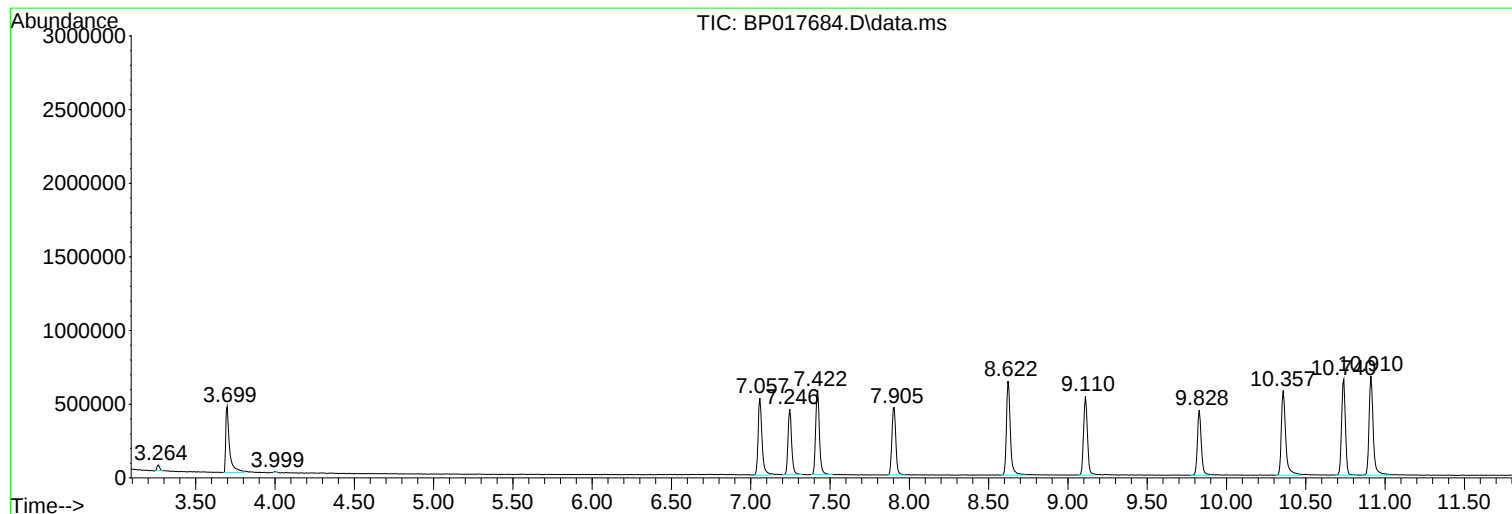

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017684.D
Acq On : 16 Oct 2023 16:13
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017684.D
Acq On : 16 Oct 2023 16:13
Operator : MA/JU
Sample : PB156296BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------