

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
 Data File : BP017685.D
 Acq On : 16 Oct 2023 16:47
 Operator : MA/JU
 Sample : PB156298BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK298

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rBV	42563	53012	1.30%	0.160%
2	3.693	100	103	117	rBV	441295	696900	17.05%	2.100%
3	3.999	152	155	161	rVB5	8372	10014	0.24%	0.030%
4	7.058	669	675	690	rBV	520088	843573	20.63%	2.542%
5	7.246	701	707	721	rVB	435763	677465	16.57%	2.041%
6	7.422	729	737	746	rBV	568694	902984	22.09%	2.721%
7	7.899	812	818	827	rBV	378142	617885	15.11%	1.862%
8	8.369	896	898	903	rVB6	2907	4122	0.10%	0.012%
9	8.622	934	941	959	rBV	610202	1040626	25.45%	3.136%
10	9.111	1014	1024	1036	rBV	507987	853956	20.89%	2.573%
11	9.828	1139	1146	1155	rBV	412632	682345	16.69%	2.056%
12	10.358	1229	1236	1257	rBV	542499	1043160	25.51%	3.143%
13	10.740	1291	1301	1311	rVV	493609	840267	20.55%	2.532%
14	10.910	1323	1330	1347	rBV	611313	1113017	27.22%	3.354%
15	11.134	1365	1368	1371	rBV5	3611	4213	0.10%	0.013%
16	12.340	1570	1573	1582	rBV6	8767	16936	0.41%	0.051%
17	13.440	1756	1760	1766	rVB9	6082	13932	0.34%	0.042%
18	14.022	1852	1859	1871	rBV	1111379	1574757	38.52%	4.745%
19	14.298	1898	1906	1915	rBV	1209990	1805804	44.17%	5.441%
20	14.604	1951	1958	1967	rBV	749737	1103601	26.99%	3.325%
21	14.798	1989	1991	1994	rBV4	4001	5346	0.13%	0.016%
22	14.857	1995	2001	2022	rVV	278581	719154	17.59%	2.167%
23	15.610	2122	2129	2142	rBV	1622749	2384692	58.33%	7.186%
24	15.757	2147	2154	2167	rVV	422394	676498	16.55%	2.038%
25	15.851	2167	2170	2175	rVB5	11527	21286	0.52%	0.064%
26	17.057	2373	2375	2378	rBV4	3723	5245	0.13%	0.016%
27	17.398	2426	2433	2443	rBV	984103	1407407	34.42%	4.241%
28	17.498	2443	2450	2465	rVV	1897463	2699189	66.02%	8.133%
29	18.257	2573	2579	2582	rVV7	9718	18594	0.45%	0.056%
30	18.798	2669	2671	2675	rVB5	4608	4474	0.11%	0.013%
31	19.328	2756	2761	2766	rBV6	23813	37360	0.91%	0.113%
32	19.398	2770	2773	2780	rVB2	25456	32871	0.80%	0.099%
33	19.498	2787	2790	2795	rBV7	10294	14255	0.35%	0.043%
34	19.757	2828	2834	2845	rBV	2675330	3399983	83.16%	10.245%
35	21.539	3132	3137	3145	rBV	1229064	1785361	43.67%	5.380%
36	23.945	3538	3546	3563	rBV2	1912608	4088513	100.00%	12.320%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017685.D
Acq On : 16 Oct 2023 16:47
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK298

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	24.116	3568	3575	3589	rVB	946001	1988329	48.63%	5.991%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 33187126

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017685.D
Acq On : 16 Oct 2023 16:47
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK298

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

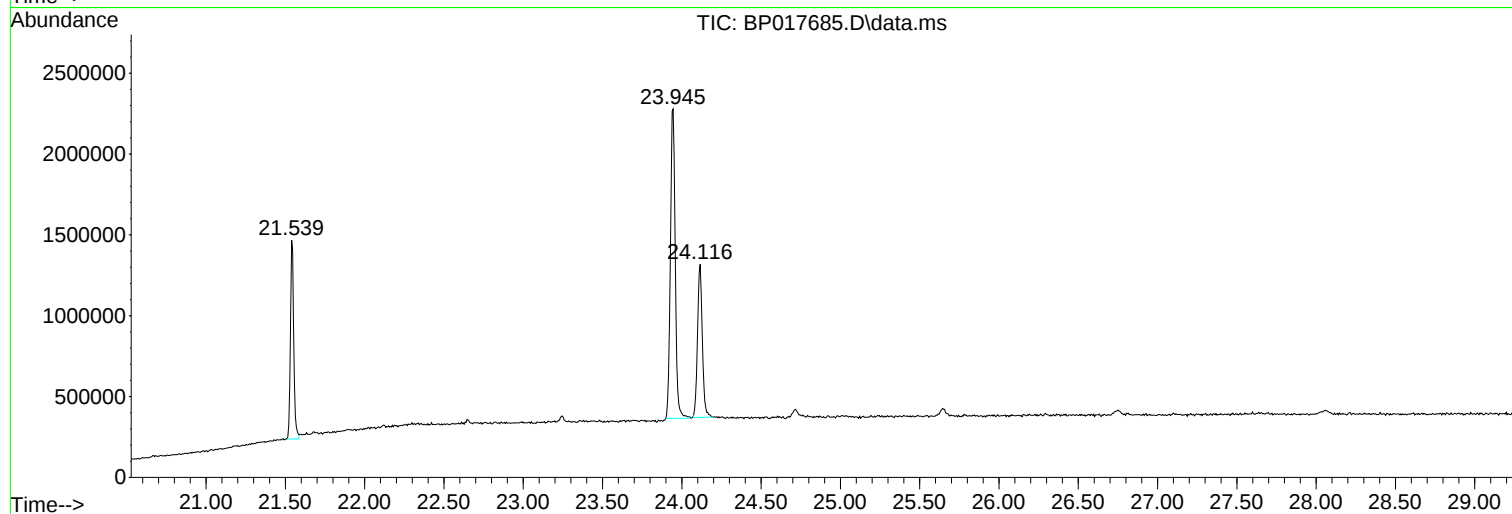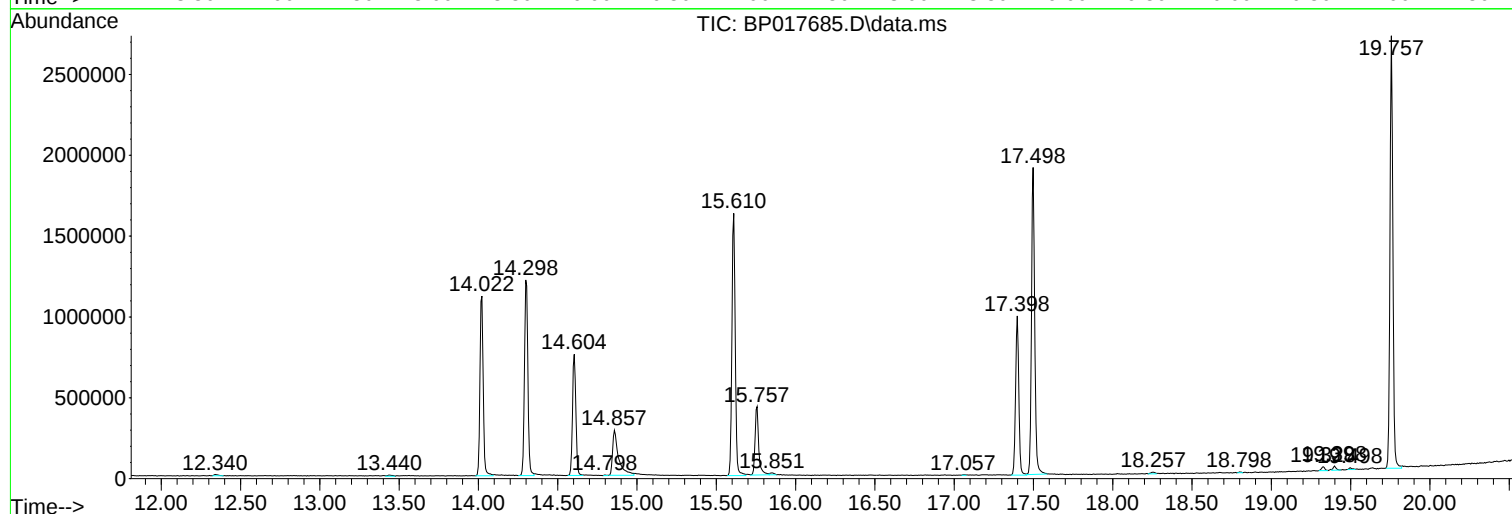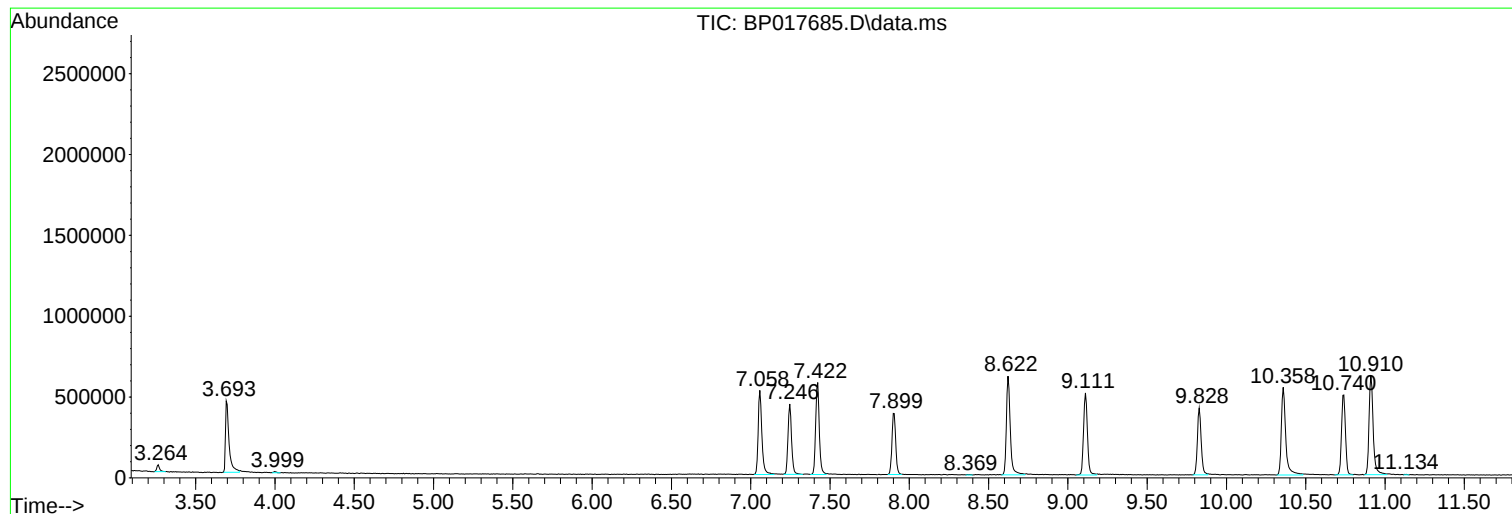

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017685.D
Acq On : 16 Oct 2023 16:47
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK298

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101623\
Data File : BP017685.D
Acq On : 16 Oct 2023 16:47
Operator : MA/JU
Sample : PB156298BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK298

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------