
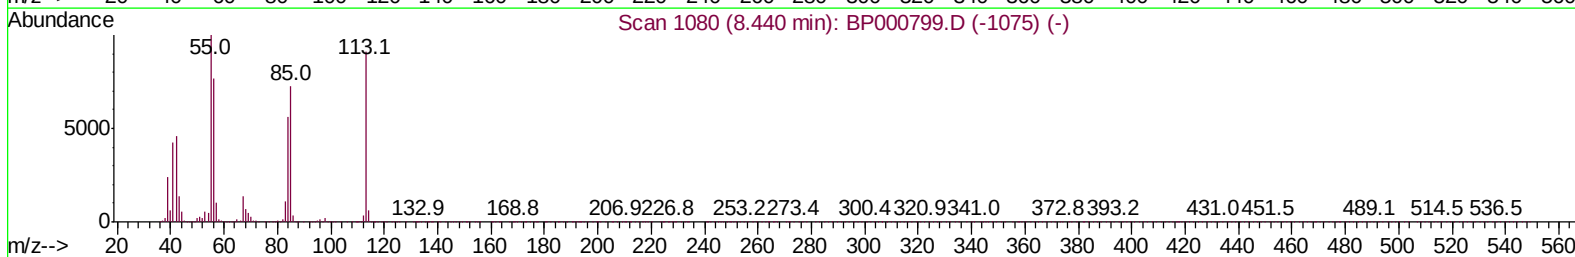
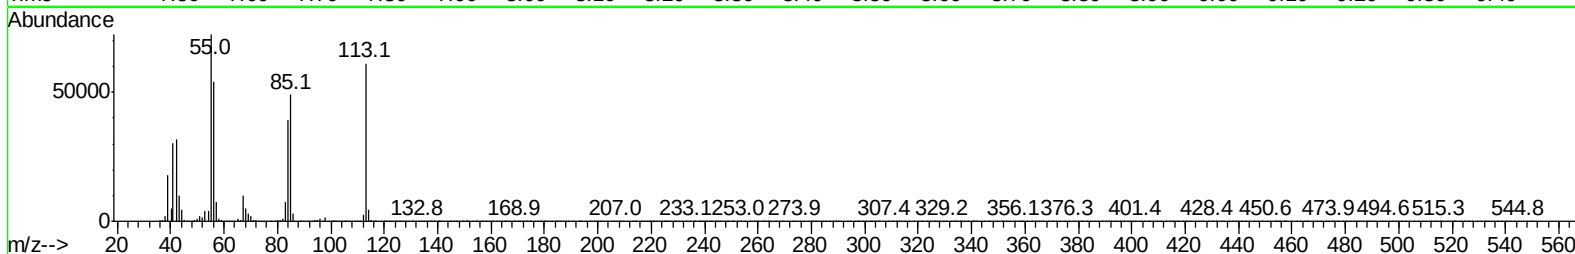


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101719\
Data File : BP000821.D
Acq On : 16 Oct 2019 19:23
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 17 08:04:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 07:55:39 2019
Response via : Initial Calibration

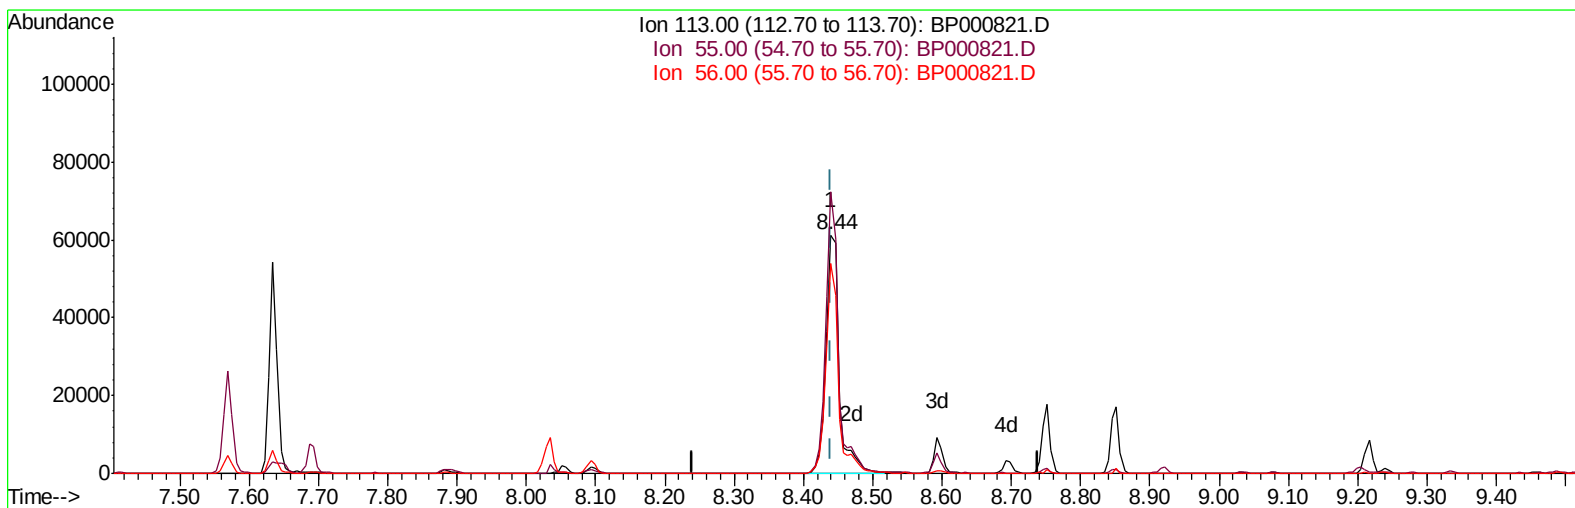

TIC: BP000821.D

(32) Caprolactam

8.440min (+0.000) 16.15ng/ul m

response 79561

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	118.26
56.00	86.80	88.19
0.00	0.00	0.00