

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
 Data File : BP000833.D
 Acq On : 17 Oct 2019 11:11
 Operator : JU
 Sample : K5378-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0044

Quant Time: Oct 17 14:57:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	176378	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	675644	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	380558	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.30	188	715001	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	618346	20.00	ng/ul	0.00
86) Perylene-d12	15.46	264	698699	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.36	96	19476	4.58	ng/uL	-0.03
5) Phenol-d5	6.39	99	76822	5.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	176357	25.93	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	255323	22.27	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	153613	14.78	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	148901	28.99	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	165661	30.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.89	165	283087	27.05	ng/ul	0.00
29) 4-Chloroaniline-d4	8.10	131	24569	2.11	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	828001	31.08	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	980901	29.93	ng/ul	0.00
52) 4-Nitrophenol-d4	9.93	143	19916	4.85	ng/ul	0.01
58) Fluorene-d10	10.32	176	687967	30.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	78224	22.97	ng/ul	0.00
71) Anthracene-d10	11.35	188	1009216	30.47	ng/ul	0.00
79) Pyrene-d10	12.74	212	1058572	30.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1056589	30.63	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	9.51	163	36667	1.381	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000833.D
Acq On : 17 Oct 2019 11:11
Operator : JU
Sample : K5378-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0044

Quant Time: Oct 17 14:57:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

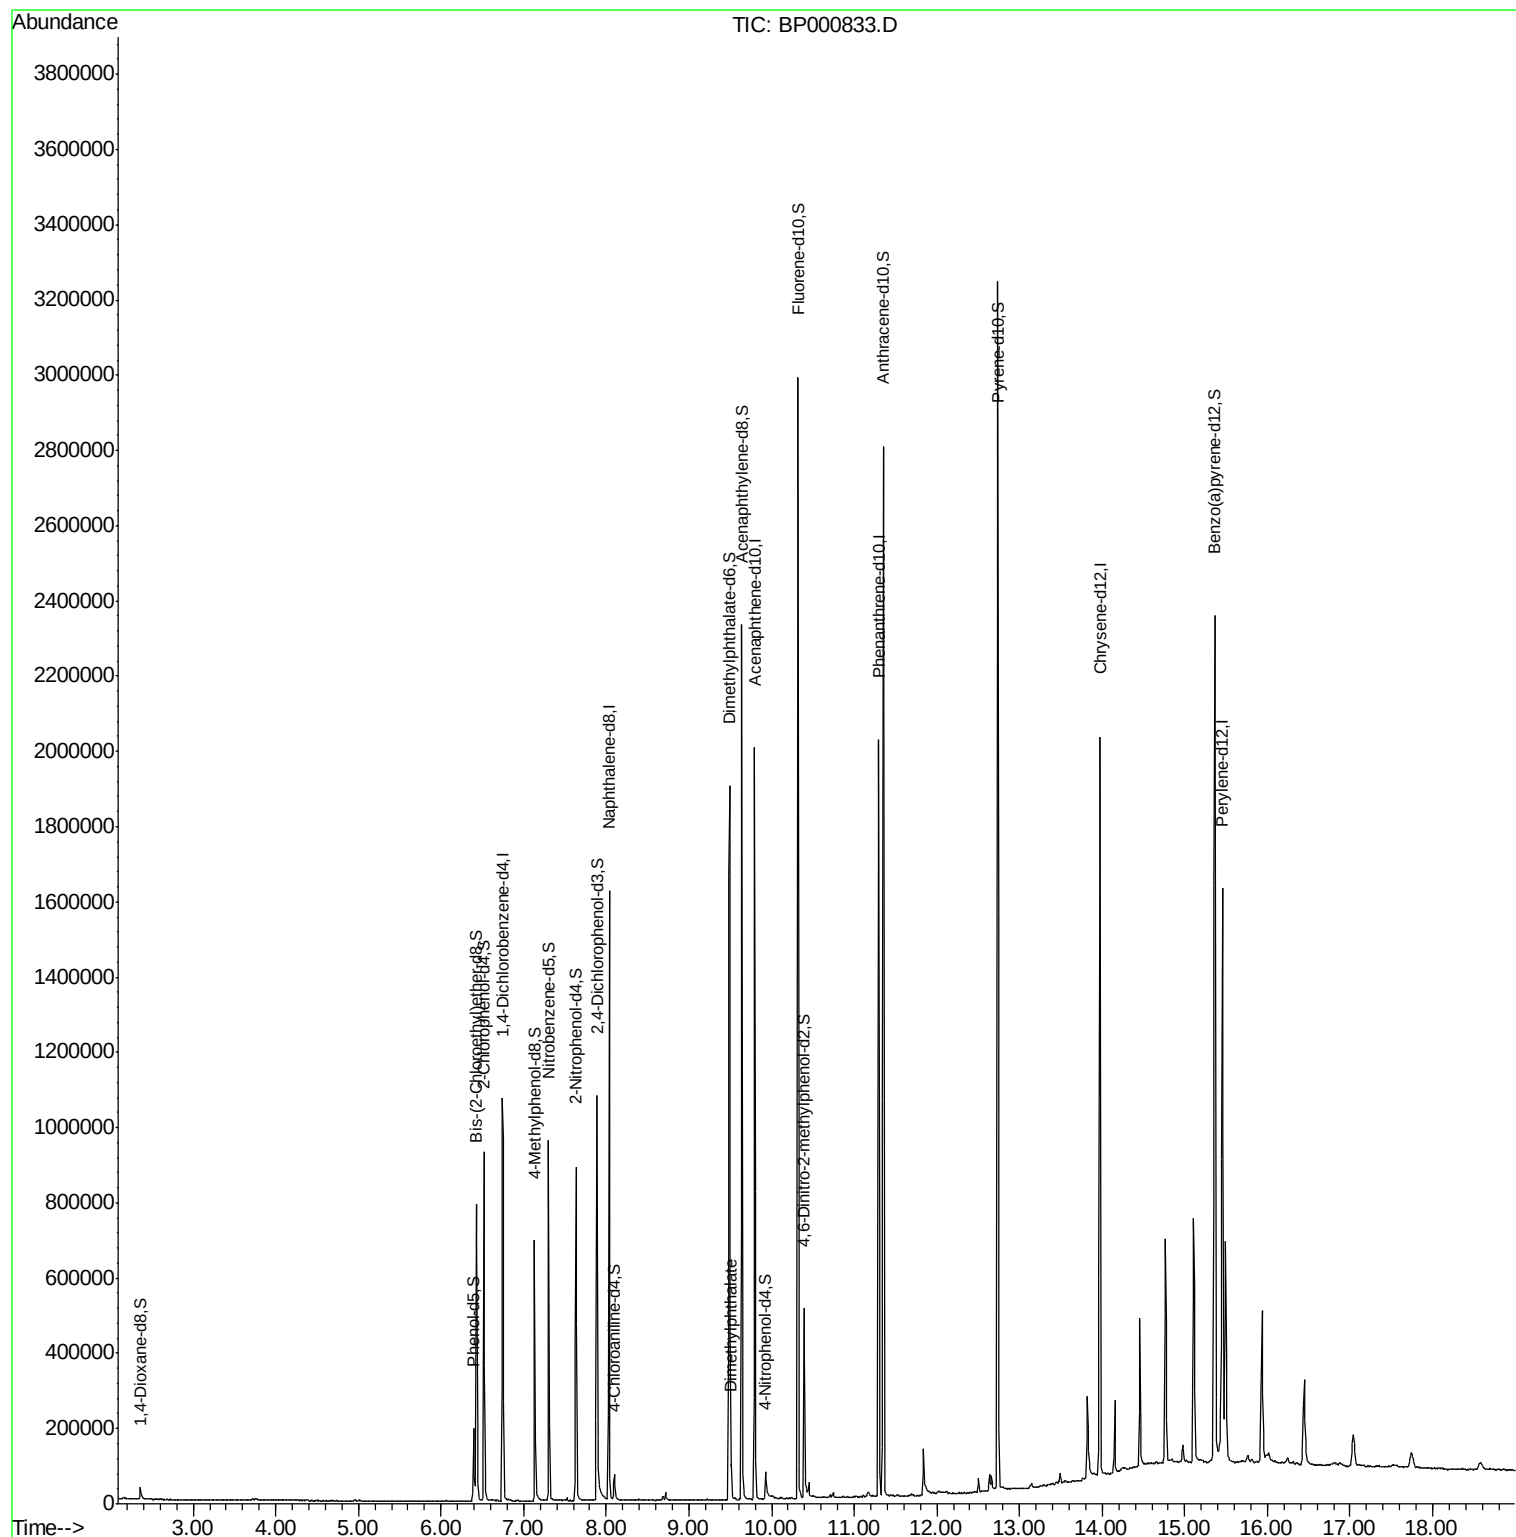

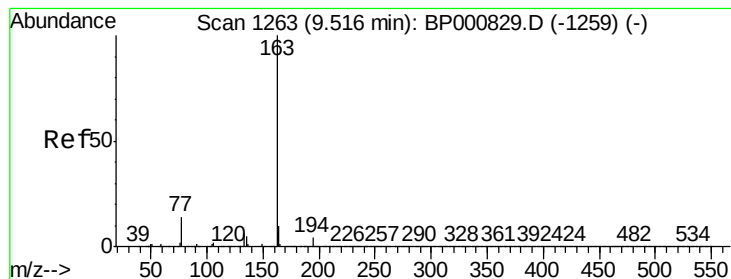

#45

Dimethylphthalate

Concen: 1.381 ng/ul

RT: 9.51 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BP000833.D

Acq: 17 Oct 2019 11:11

Instrument :

BNA_P

ClientSampleId :

C0044


Tot Ion:163 Resp: 36667

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 9.9 8.1 12.1

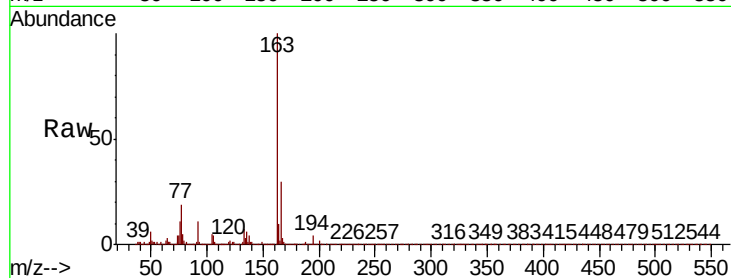

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

