

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000836.D
 Acq On : 17 Oct 2019 12:24
 Operator : JU
 Sample : K5346-12MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ET0N4MSD

Manual Integrations
 APPROVED

mohammad
 10/20/2019 8:11:25 PM

Quant Time: Oct 17 15:26:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 09:27:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	219515	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	809696	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	429027	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.30	188	759045	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	638159	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	688527	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.39	96	23290	4.40	ng/uL	0.00
5) Phenol-d5	6.39	99	96730	5.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	217680	25.71	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	310465	21.76	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	212673m	16.44	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	179303	29.13	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	197989	30.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	322252	25.69	ng/ul	0.00
29) 4-Chloroaniline-d4	8.10	131	41561	2.98	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	892118	29.70	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	1042553	28.22	ng/ul	0.00
52) 4-Nitrophenol-d4	9.92	143	25370	5.48	ng/ul	0.00
58) Fluorene-d10	10.32	176	731315	28.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	93162	25.77	ng/ul	0.00
71) Anthracene-d10	11.35	188	1108504	31.53	ng/ul	0.00
79) Pyrene-d10	12.74	212	1166379	32.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1092407	32.14	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	6.40	94	102244	5.990	ng/ul	97
10) 2-Chlorophenol	6.53	128	312037	20.996	ng/ul	99
15) N-Nitroso-di-n-propylamine	7.16	70	225302	26.186	ng/ul	98
33) 4-Chloro-3-methylphenol	8.59	107	264798	21.667	ng/ul	96
50) Acenaphthene	9.83	153	697263	26.424	ng/ul	98
53) 4-Nitrophenol	9.93	109	16495	5.222	ng/ul	96
55) 2,4-Dinitrotoluene	9.99	165	244715	29.845	ng/ul	99
69) Pentachlorophenol	11.11	266	108090	29.512	ng/ul	98
80) Pvrene	12.76	202	1391099	30.724	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000836.D
Acq On : 17 Oct 2019 12:24
Operator : JU
Sample : K5346-12MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
ETON4MSD

Quant Time: Oct 17 15:26:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 09:27:24 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
10/20/2019 8:11:25 PM

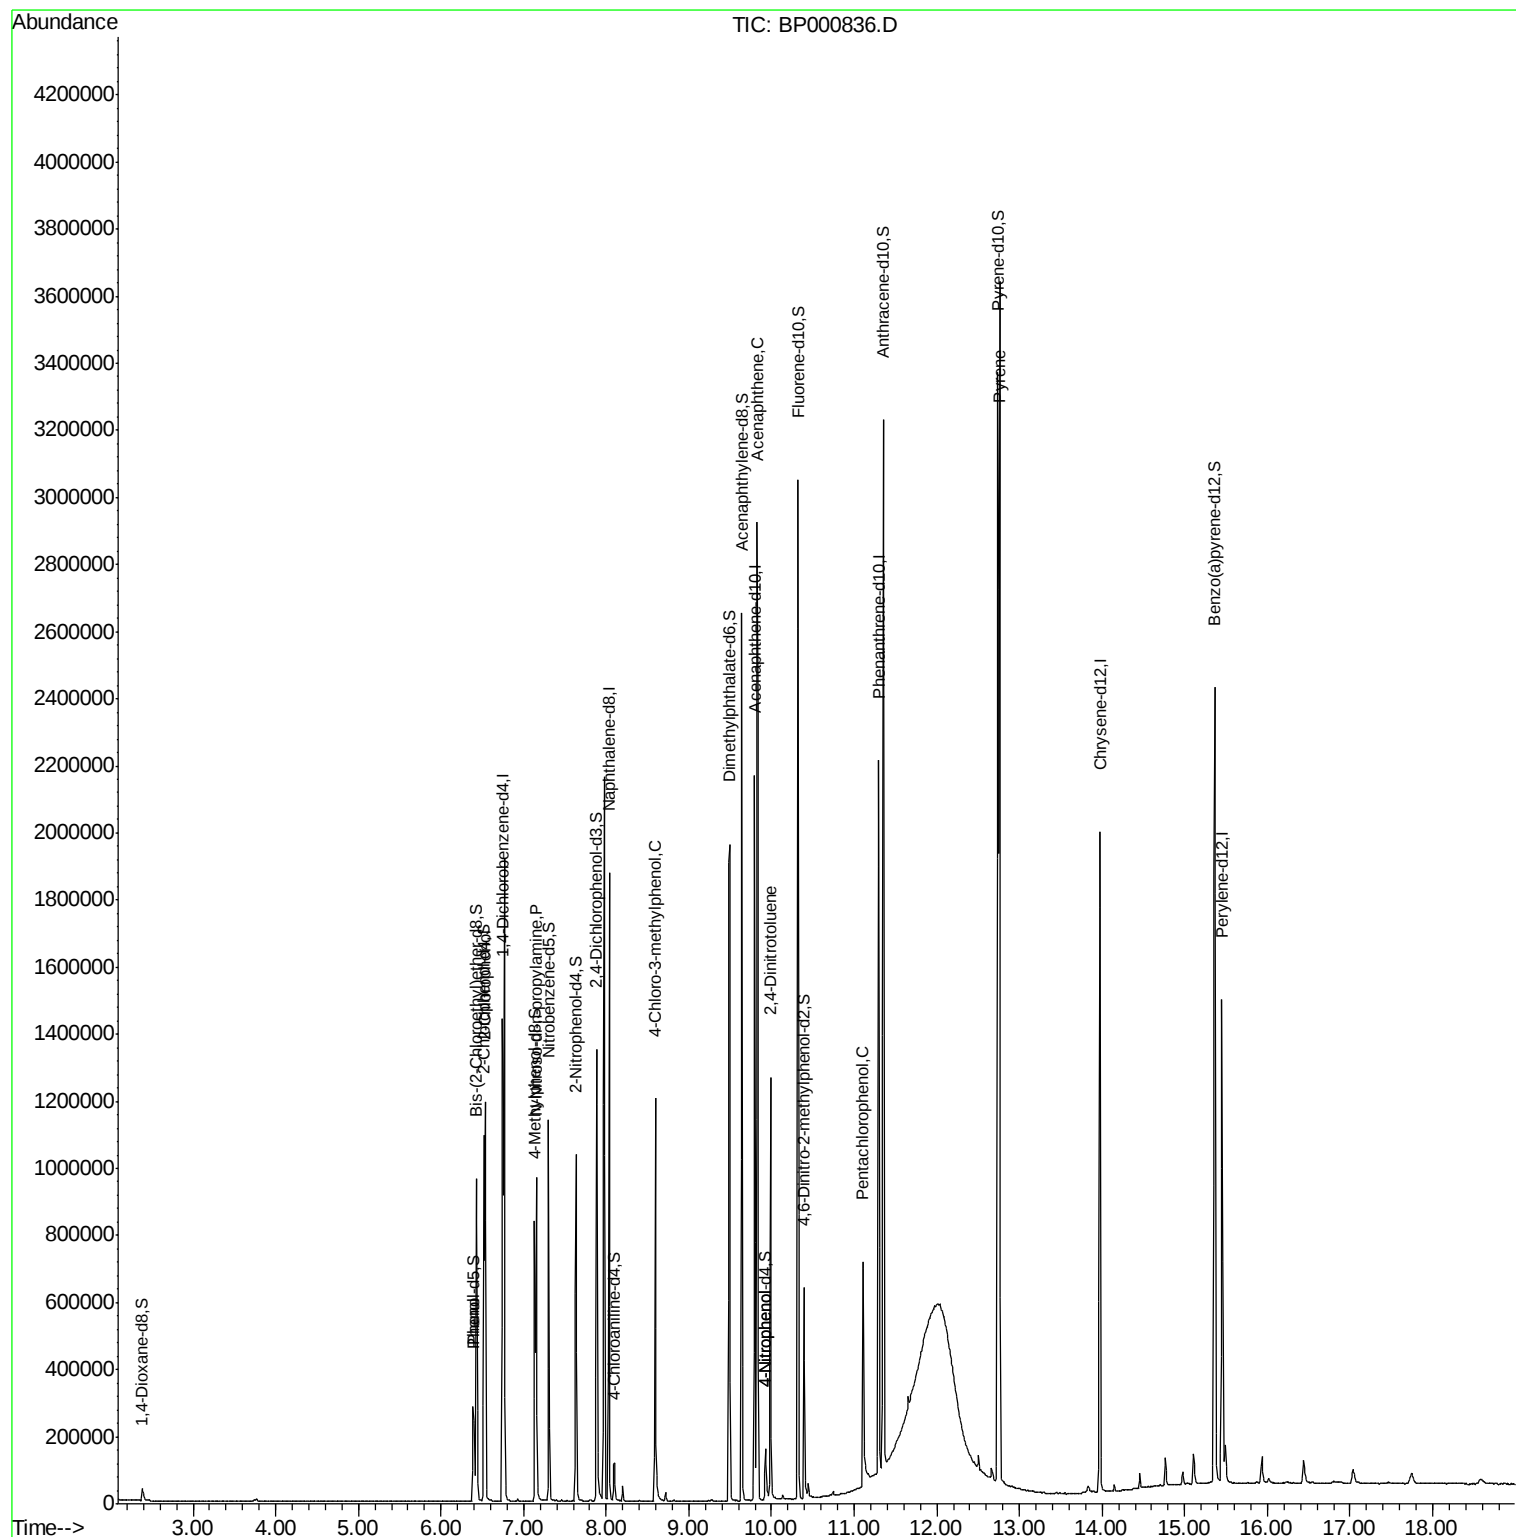

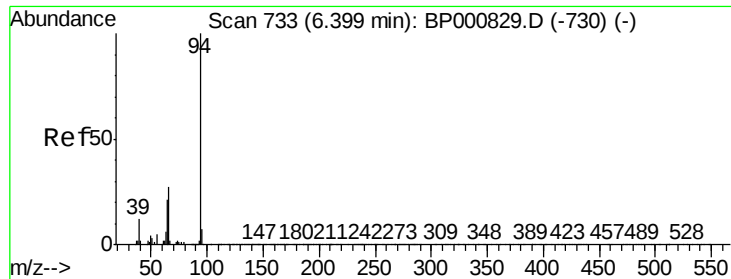

#6

Phenol

Concen: 5.990 ng/ul

RT: 6.40 min Scan# 734

Delta R.T. 0.01 min

Lab File: BP000836.D

Acq: 17 Oct 2019 12:24

Instrument :

BNA_P





ClientSampleId :

ETON4MSD

Tot Ion:	94	Resp:	102244
Ion Ratio	Lower	Upper	
94	100		
65	21.9	19.2	28.8
66	30.9	25.7	38.5

Manual Integrations
APPROVED

mohammad
10/20/2019 8:11:25 PM

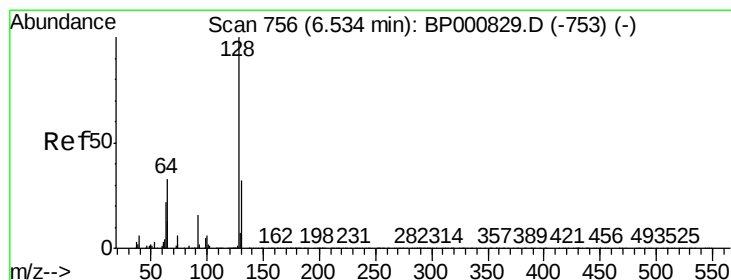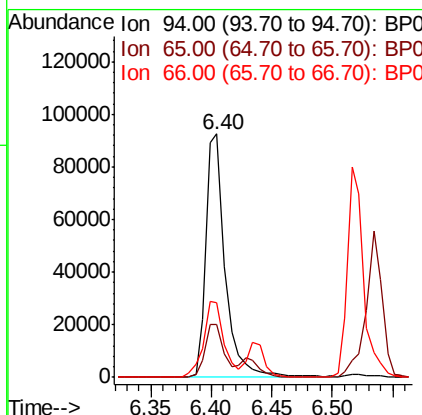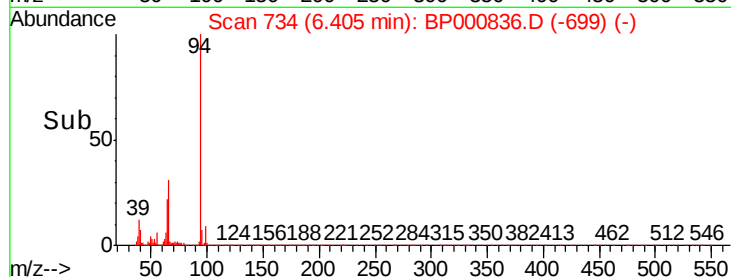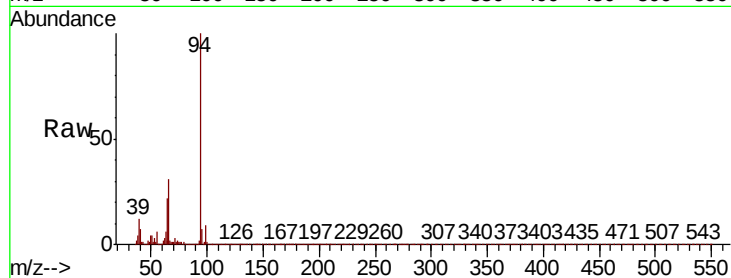

#10

2-Chlorophenol

Concen: 20.996 ng/ul




RT: 6.53 min Scan# 756


Delta R.T. 0.00 min

Lab File: BP000836.D

Acq: 17 Oct 2019 12:24

Tgt Ion:	128	Resp:	312037
Ion Ratio	Lower	Upper	
128	100		
64	36.7	29.3	43.9
130	31.9	26.0	39.0

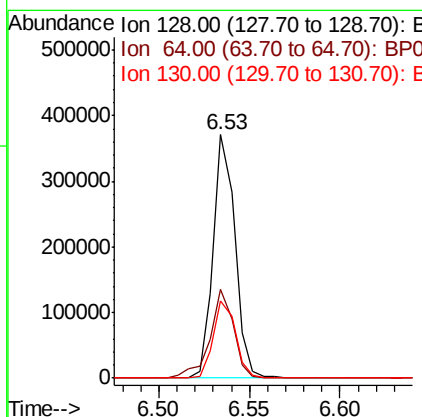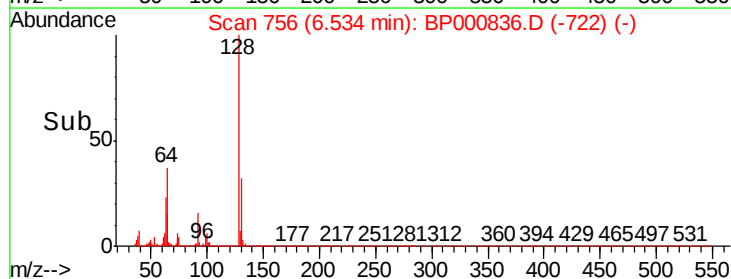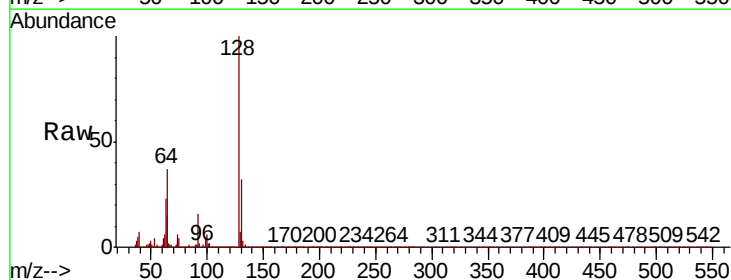

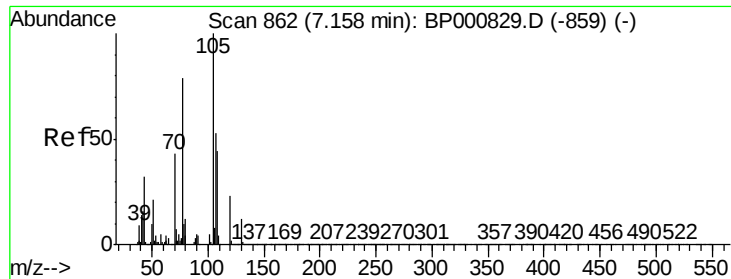





#15
N-Nitroso-di-n-propylamine
Concen: 26.186 ng/ul
RT: 7.16 min Scan# 862
Delta R.T. -0.00 min
Lab File: BP000836.D
Acq: 17 Oct 2019 12:24

Instrument :
BNA_P
ClientSampleId :
ETON4MSD

Tot Ion	Ratio	Lower	Upper
70	100		
42	39.1	33.5	50.3
101	11.8	9.6	14.4
130	27.4	21.8	32.8




Manual Integrations
APPROVED


mohammad
10/20/2019 8:11:25 PM

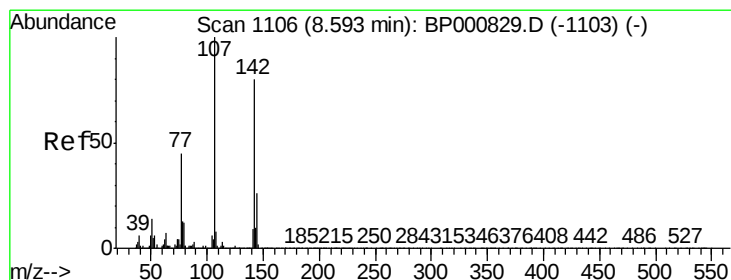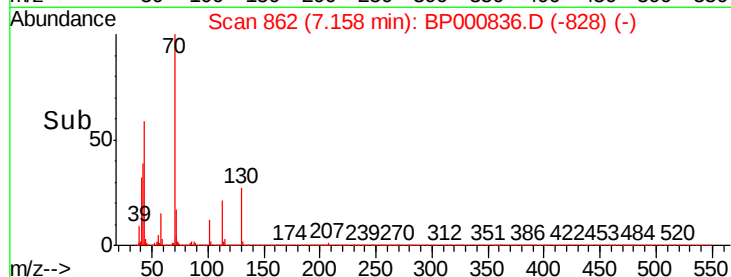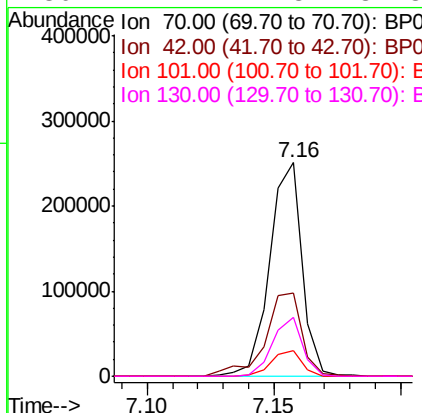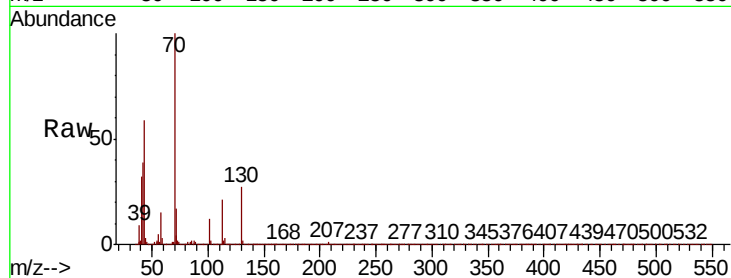

#33
4-Chloro-3-methylphenol
Concen: 21.667 ng/ul
RT: 8.59 min Scan# 1106
Delta R.T. -0.00 min
Lab File: BP000836.D
Acq: 17 Oct 2019 12:24

Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.4	20.6	30.8
142	84.5	64.6	96.8

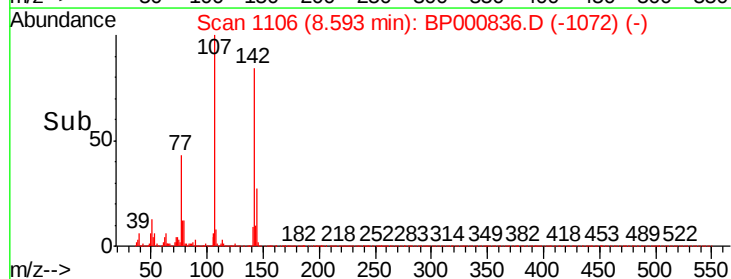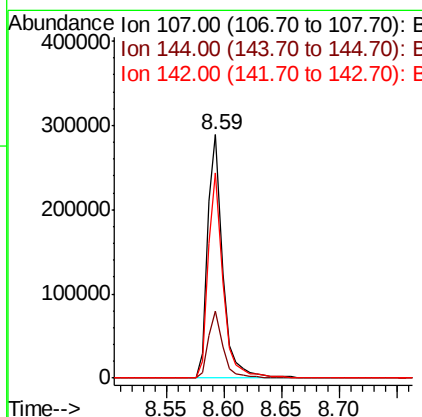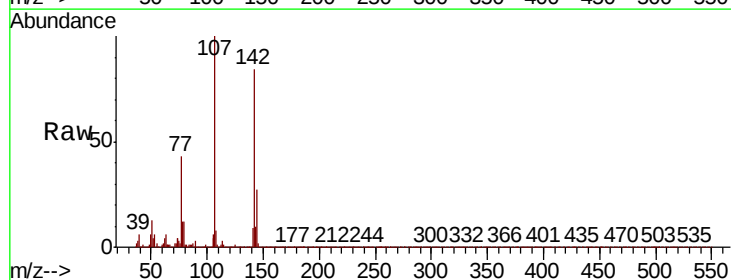

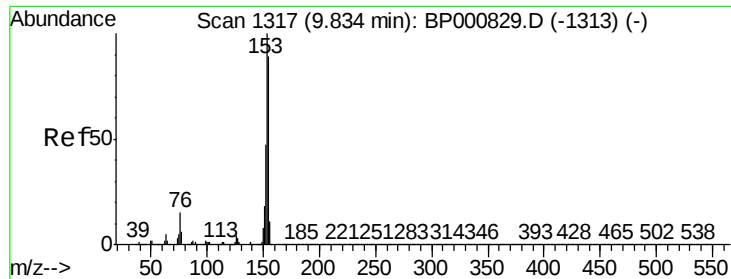





#50
Acenaphthene
Concen: 26.424 ng/ul
RT: 9.83 min Scan# 1316
Delta R.T. -0.00 min
Lab File: BP000836.D
Acq: 17 Oct 2019 12:24

Instrument :
BNA_P
ClientSampleId :
ETON4MSD

Tot Ion	Ratio	Lower	Upper
153	100		
152	47.2	38.6	57.8
154	88.2	71.9	107.9




Manual Integrations
APPROVED


mohammad
10/20/2019 8:11:25 PM

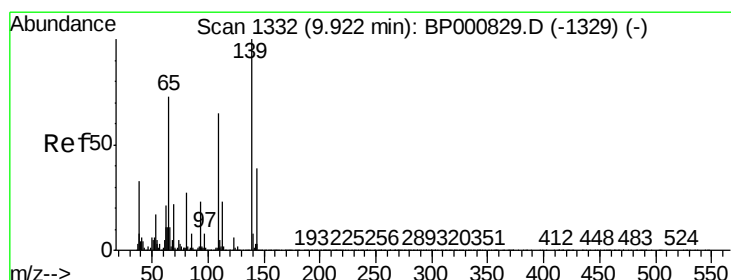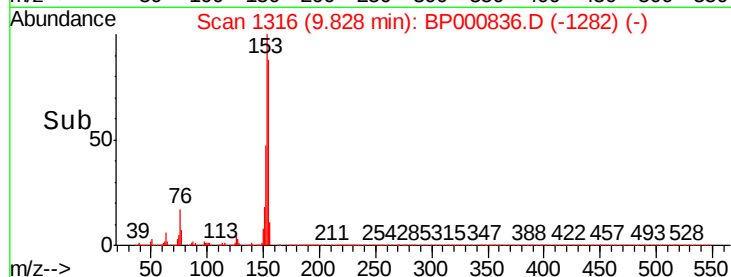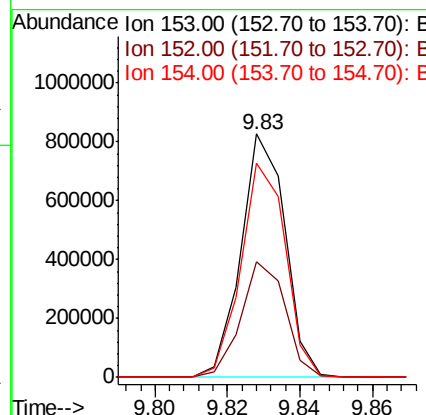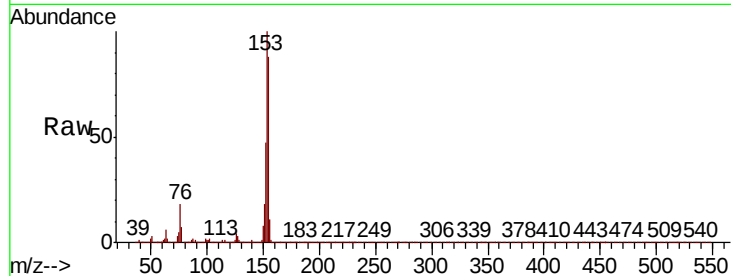

#53
4-Nitrophenol
Concen: 5.222 ng/ul
RT: 9.93 min Scan# 1333
Delta R.T. 0.01 min
Lab File: BP000836.D
Acq: 17 Oct 2019 12:24

Tgt Ion	Ratio	Lower	Upper
109	100		
139	148.2	115.1	172.7
65	118.0	97.9	146.9

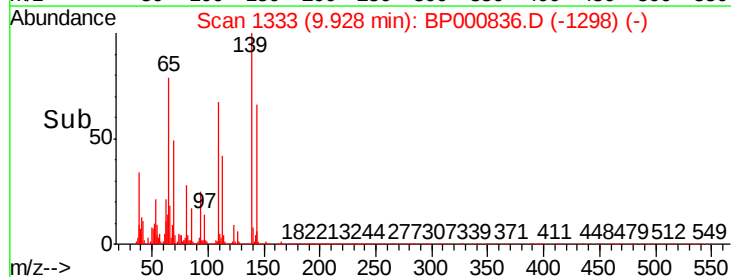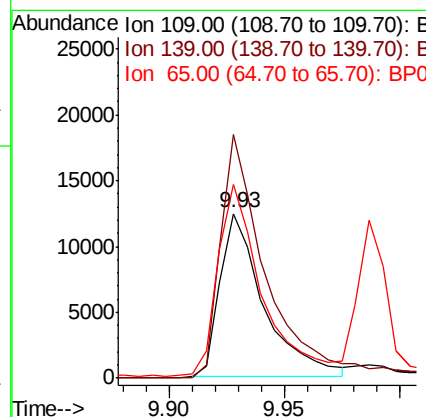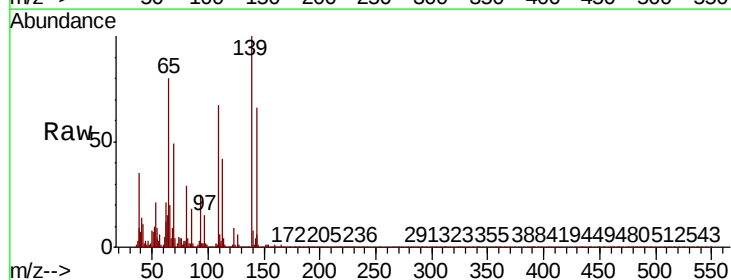

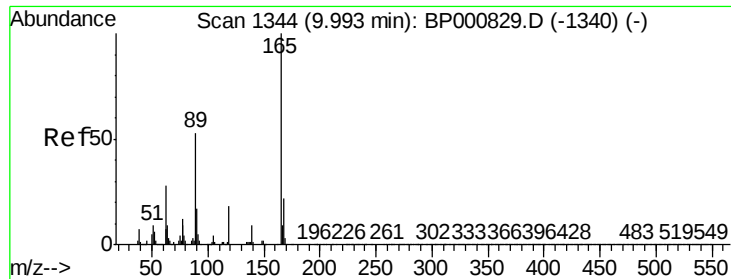





#55
2,4-Dinitrotoluene
Concen: 29.845 ng/ul
RT: 9.99 min Scan# 1343
Delta R.T. 0.00 min
Lab File: BP000836.D
Acq: 17 Oct 2019 12:24

Instrument :
BNA_P
ClientSampleId :
ETON4MSD

Tot Ion	Ratio	Resp Lower	Upper
165	100		
63	33.3	26.4	39.6
182	3.0	2.3	3.5




Manual Integrations
APPROVED


mohammad
10/20/2019 8:11:25 PM

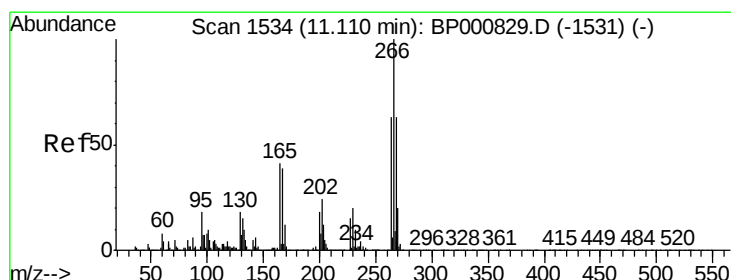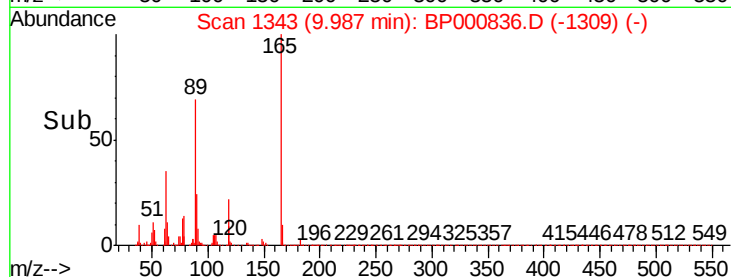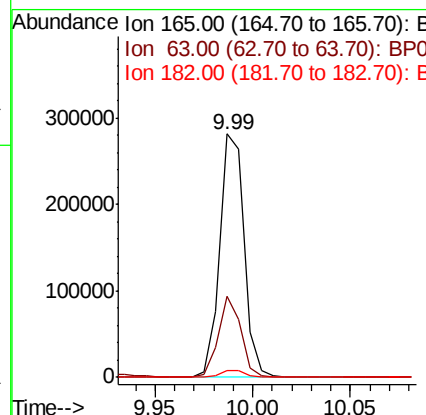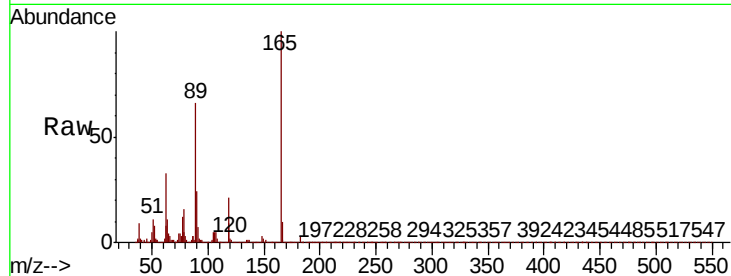

#69
Pentachlorophenol
Concen: 29.512 ng/ul
RT: 11.11 min Scan# 1534
Delta R.T. -0.00 min
Lab File: BP000836.D
Acq: 17 Oct 2019 12:24

Tgt Ion	Ratio	Resp Lower	Upper
266	100		
264	62.2	49.6	74.4
268	64.2	49.6	74.4

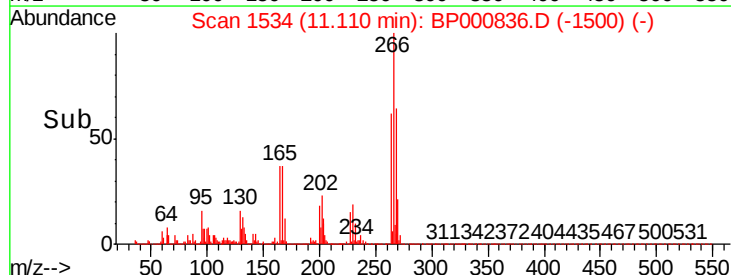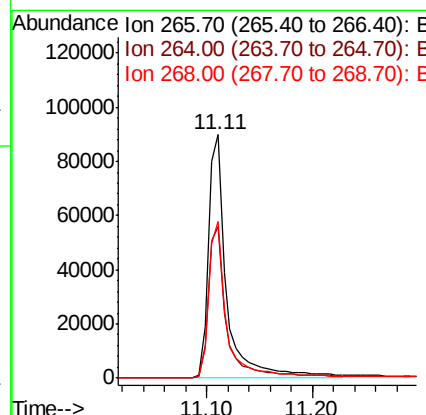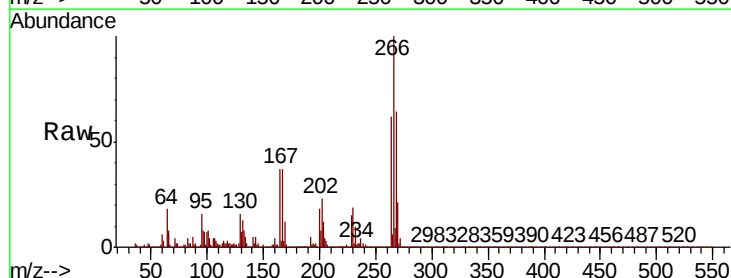

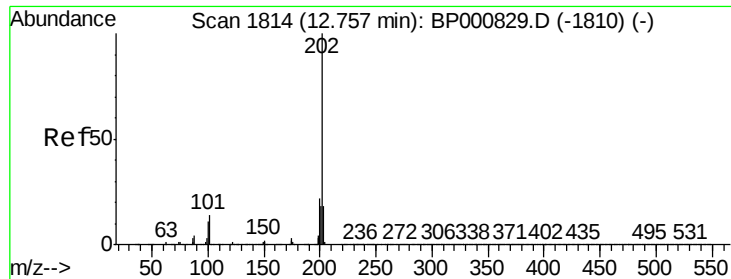

#80
 Pvrene
 Concen: 30.724 ng/ul
 RT: 12.76 min Scan# 1814
 Delta R.T. 0.00 min
 Lab File: BP000836.D
 Acq: 17 Oct 2019 12:24

Instrument :
 BNA_P
 ClientSampleId :
 ET0N4MSD

Tot Ion	Ratio	Lower	Upper
202	100		
101	14.9	9.7	14.5#
100	11.9	7.8	11.8#

Manual Integrations
 APPROVED

mohammad
 10/20/2019 8:11:25 PM

