

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000808.D
 Acq On : 16 Oct 2019 13:18
 Operator : JU
 Sample : K5223-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEPD8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	46	50	63	rVB	28124	42017	1.59%	0.124%
2	3.522	239	244	254	rBV2	14040	27012	1.02%	0.080%
3	3.675	260	270	275	rBV3	5145	12857	0.49%	0.038%
4	3.734	275	280	282	rVV	11251	17276	0.66%	0.051%
5	3.764	282	285	293	rVB	10350	16475	0.62%	0.049%
6	6.387	727	731	736	rBV	745024	800980	30.38%	2.360%
7	6.428	736	738	750	rVV	732112	647472	24.56%	1.908%
8	6.516	750	753	761	rVV	982395	825095	31.30%	2.432%
9	6.746	789	792	802	rBV	1296166	1100640	41.75%	3.244%
10	7.134	854	858	872	rBV	816130	761345	28.88%	2.244%
11	7.305	884	887	894	rBV	881421	702210	26.64%	2.069%
12	7.522	920	924	928	rBV	20538	17395	0.66%	0.051%
13	7.634	939	943	954	rBV	712941	578125	21.93%	1.704%
14	7.881	982	985	1007	rVV	1085462	979541	37.16%	2.887%
15	8.034	1007	1011	1014	rVV	1734230	1449614	54.99%	4.272%
16	8.093	1018	1021	1036	rVV	957703	797395	30.25%	2.350%
17	8.716	1124	1127	1131	rBV	15177	15427	0.59%	0.045%
18	9.116	1189	1195	1201	rVB	24230	26217	0.99%	0.077%
19	9.216	1206	1212	1214	rBV2	17249	19360	0.73%	0.057%
20	9.240	1214	1216	1219	rVB	12135	9792	0.37%	0.029%
21	9.451	1249	1252	1255	rVV2	16070	16216	0.62%	0.048%
22	9.487	1255	1258	1261	rVV	1559003	1371669	52.03%	4.042%
23	9.510	1261	1262	1271	rVV	588203	363883	13.80%	1.072%
24	9.640	1281	1284	1298	rVV	2061078	1725078	65.44%	5.084%
25	9.798	1307	1311	1314	rVV	2045379	1749760	66.37%	5.156%
26	9.828	1314	1316	1322	rVB	45342	37816	1.43%	0.111%
27	9.916	1327	1331	1339	rBV	247483	333004	12.63%	0.981%
28	9.981	1339	1342	1343	rVV	27910	28038	1.06%	0.083%
29	10.004	1343	1346	1351	rVB2	171129	161687	6.13%	0.476%
30	10.216	1377	1382	1384	rBV2	12439	14411	0.55%	0.042%
31	10.316	1396	1399	1402	rBV	2252691	2007029	76.13%	5.915%
32	10.346	1402	1404	1409	rVB2	113686	101580	3.85%	0.299%
33	10.393	1409	1412	1418	rBV	301010	270630	10.27%	0.798%
34	10.451	1418	1422	1426	rVV2	41143	60761	2.30%	0.179%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000808.D
 Acq On : 16 Oct 2019 13:18
 Operator : JU
 Sample : K5223-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEPD8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	10.504	1428	1431	1436	rVB	32473	31244	1.19%	0.092%
36	10.593	1442	1446	1450	rBV	17442	19265	0.73%	0.057%
37	10.716	1460	1467	1470	rBV5	10267	17640	0.67%	0.052%
38	10.834	1481	1487	1495	rVB	54912	56875	2.16%	0.168%
39	10.904	1496	1499	1503	rBV	78518	74440	2.82%	0.219%
40	11.034	1518	1521	1527	rVB3	22682	22621	0.86%	0.067%
41	11.110	1530	1534	1537	rVB2	8472	9942	0.38%	0.029%
42	11.169	1542	1544	1547	rBV2	9473	9981	0.38%	0.029%
43	11.298	1562	1566	1568	rVV	1984305	1835705	69.63%	5.410%
44	11.316	1568	1569	1572	rVV	187073	139454	5.29%	0.411%
45	11.351	1572	1575	1578	rVV	2394195	2038395	77.32%	6.007%
46	11.410	1582	1585	1589	rVB5	11659	13167	0.50%	0.039%
47	11.528	1600	1605	1608	rBV	45756	46884	1.78%	0.138%
48	11.657	1624	1627	1631	rVV	44323	35637	1.35%	0.105%
49	11.804	1648	1652	1654	rBV	21938	21148	0.80%	0.062%
50	11.834	1654	1657	1660	rVV	53859	57170	2.17%	0.168%
51	11.869	1660	1663	1668	rVV	73951	72908	2.77%	0.215%
52	11.916	1668	1671	1673	rVV	30258	28782	1.09%	0.085%
53	11.940	1673	1675	1680	rVB	16105	15370	0.58%	0.045%
54	12.016	1681	1688	1691	rBV5	13631	25662	0.97%	0.076%
55	12.104	1700	1703	1706	rBV2	18245	18790	0.71%	0.055%
56	12.363	1744	1747	1749	rVV	16509	17242	0.65%	0.051%
57	12.404	1752	1754	1756	rVV2	12162	13876	0.53%	0.041%
58	12.451	1758	1762	1766	rVB3	11486	15911	0.60%	0.047%
59	12.522	1771	1774	1778	rVV	349803	290447	11.02%	0.856%
60	12.569	1780	1782	1784	rVV2	9115	9053	0.34%	0.027%
61	12.622	1788	1791	1794	rVV	12655	14440	0.55%	0.043%
62	12.663	1795	1798	1806	rVV2	30395	43008	1.63%	0.127%
63	12.734	1806	1810	1817	rVV2	2418697	2636225	100.00%	7.769%
64	12.781	1817	1818	1820	rVV2	14111	11309	0.43%	0.033%
65	12.804	1820	1822	1828	rVB2	14936	21089	0.80%	0.062%
66	12.898	1835	1838	1845	rVB	330609	269447	10.22%	0.794%
67	12.975	1847	1851	1855	rBV3	16082	24521	0.93%	0.072%
68	13.040	1859	1862	1864	rBV2	13085	12894	0.49%	0.038%
69	13.063	1864	1866	1868	rVV3	11686	13251	0.50%	0.039%
70	13.087	1868	1870	1874	rVB	32964	29348	1.11%	0.086%
71	13.157	1874	1882	1884	rBV2	27408	49527	1.88%	0.146%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
 Data File : BP000808.D
 Acq On : 16 Oct 2019 13:18
 Operator : JU
 Sample : K5223-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEPD8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

72	13.192	1885	1888	1891	rVV3	26477	24658	0.94%	0.073%
73	13.287	1901	1904	1907	rBV	17721	14722	0.56%	0.043%
74	13.322	1907	1910	1914	rBV2	13880	14983	0.57%	0.044%
75	13.381	1918	1920	1924	rBV	81246	71786	2.72%	0.212%
76	13.457	1929	1933	1936	rBV	120070	106565	4.04%	0.314%
77	13.610	1956	1959	1963	rVB	13545	16216	0.62%	0.048%
78	13.745	1979	1982	1984	rBV	13605	13171	0.50%	0.039%
79	13.769	1984	1986	1987	rBV	17216	13939	0.53%	0.041%
80	13.822	1991	1995	2003	rVV	296937	494878	18.77%	1.458%
81	13.969	2015	2020	2023	rBV	2092600	2111779	80.11%	6.223%
82	13.992	2023	2024	2033	rVB	255157	214896	8.15%	0.633%
83	14.145	2048	2050	2056	rVB2	39936	40984	1.55%	0.121%
84	14.363	2085	2087	2090	rBV	23539	28247	1.07%	0.083%
85	14.457	2100	2103	2107	rVB2	70007	66712	2.53%	0.197%
86	14.575	2120	2123	2128	rVB	117939	106721	4.05%	0.315%
87	14.769	2152	2156	2159	rBV	87386	92335	3.50%	0.272%
88	14.839	2165	2168	2172	rVB	55290	56751	2.15%	0.167%
89	14.969	2188	2190	2195	rBV	27384	30222	1.15%	0.089%
90	15.016	2195	2198	2201	rBV	193700	234941	8.91%	0.692%
91	15.045	2201	2203	2208	rVB	165065	162065	6.15%	0.478%
92	15.104	2210	2213	2217	rBV	117237	146651	5.56%	0.432%
93	15.357	2252	2256	2260	rBV	1697454	1940537	73.61%	5.719%
94	15.386	2260	2261	2266	rVB	197365	139611	5.30%	0.411%
95	15.451	2267	2272	2276	rBV	1410066	1726162	65.48%	5.087%
96	15.486	2276	2278	2294	rVB2	108480	184823	7.01%	0.545%
97	15.928	2349	2353	2359	rBV	87877	126598	4.80%	0.373%
98	16.433	2435	2439	2455	rVB2	52795	119267	4.52%	0.351%
99	16.922	2517	2522	2534	rVB2	144849	323998	12.29%	0.955%
100	17.357	2591	2596	2605	rBV	76265	158849	6.03%	0.468%


Sum of corrected areas: 33933542

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000808.D
Acq On : 16 Oct 2019 13:18
Operator : JU
Sample : K5223-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
BEPD8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

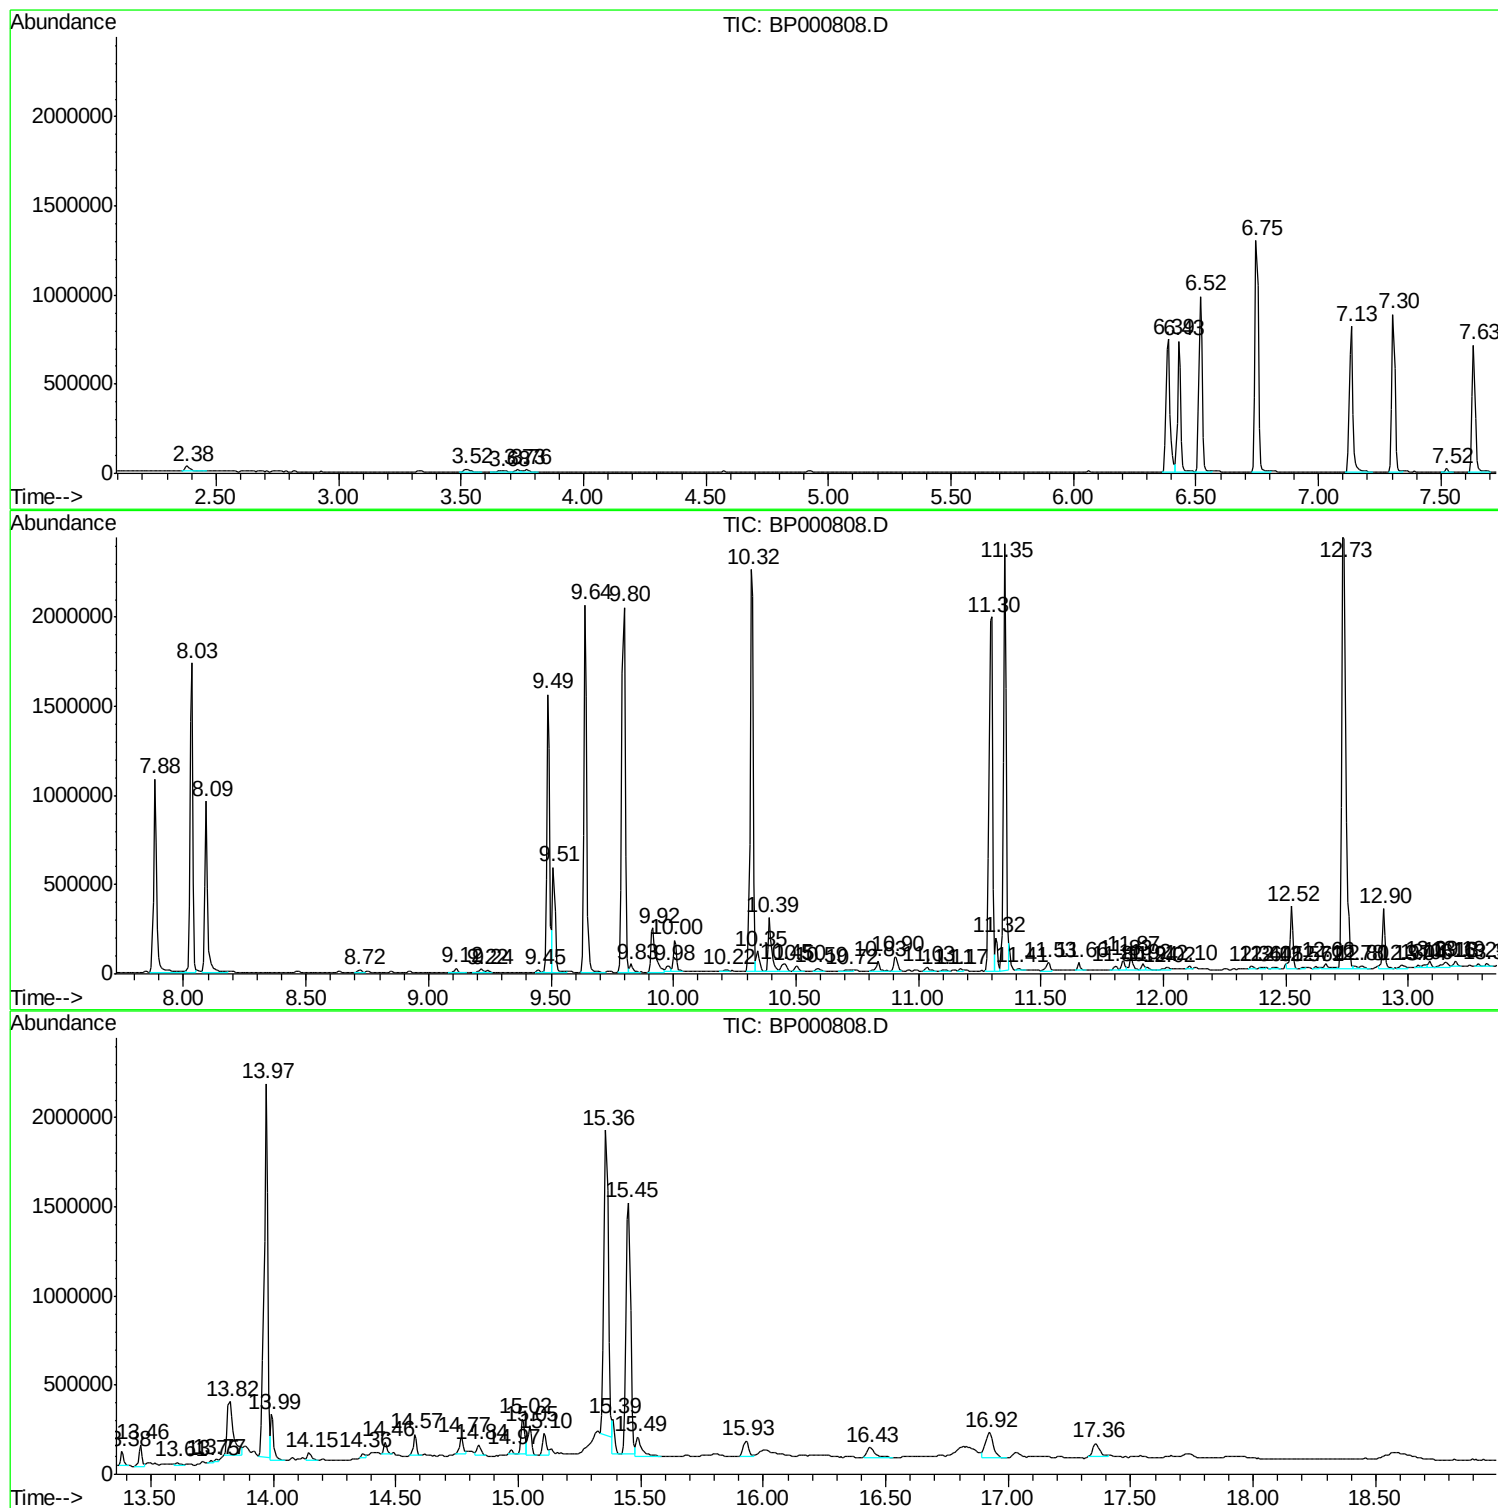

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000808.D
Acq On : 16 Oct 2019 13:18
Operator : JU
Sample : K5223-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BEPD8










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic13.82 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.82	4.69 ng/ul	494878	Chrysene-d12	13.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentadecane	210	C15H30	000295-48-7	94
2		2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	93
3		1-Triacontanol	438	C30H62O	000593-50-0	91
4		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	91
5		1-Nonadecanol	284	C19H40O	001454-84-8	90

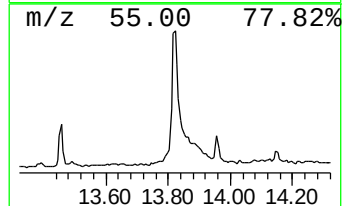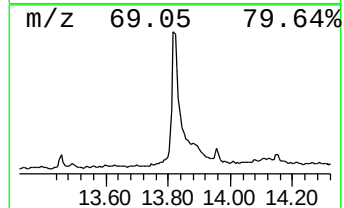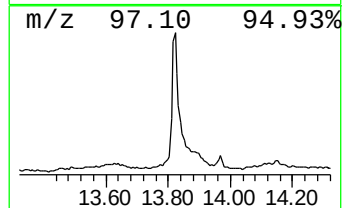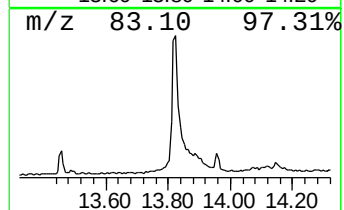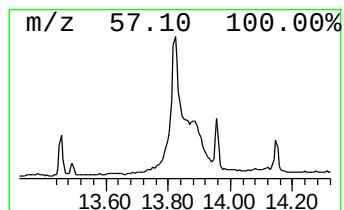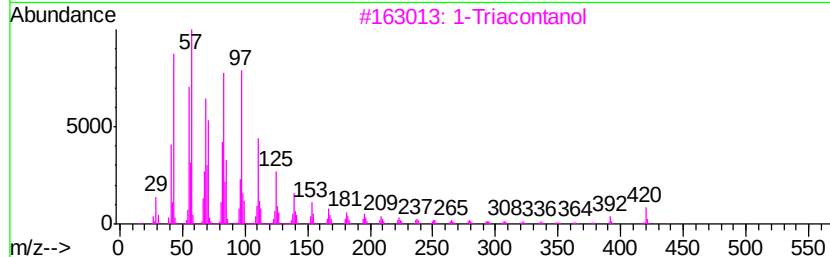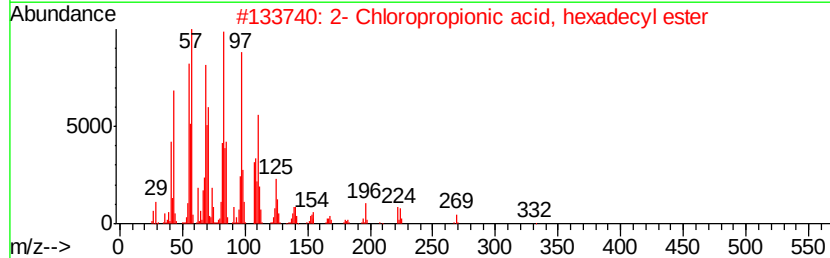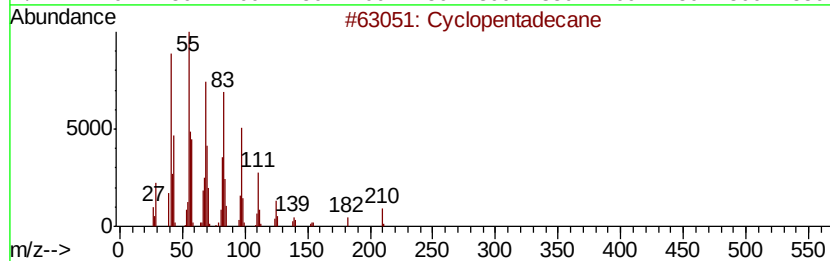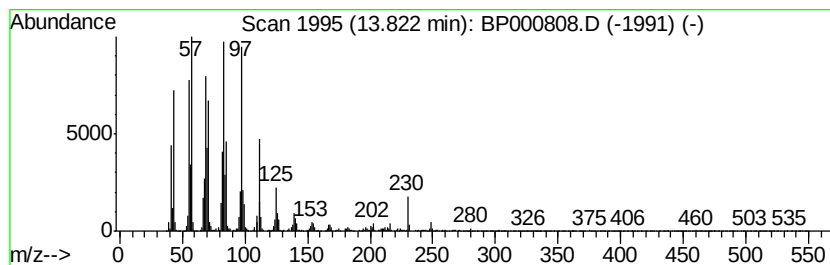

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
Data File : BP000808.D
Acq On : 16 Oct 2019 13:18
Operator : JU
Sample : K5223-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BEPD8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	13.82	4.7	ng/ul	494878	5	13.97	2111780	20.0