

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000820.D
 Acq On : 16 Oct 2019 18:10
 Operator : JU
 Sample : PB123786BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	48	50	67	rVB	55770	83136	2.62%	0.204%
2	3.770	279	286	293	rBV	12118	18652	0.59%	0.046%
3	4.622	424	431	436	rVB	2401	4145	0.13%	0.010%
4	5.005	492	496	505	rBV3	2108	3998	0.13%	0.010%
5	6.387	727	731	735	rBV	1452953	1338324	42.13%	3.282%
6	6.434	735	739	750	rVB	1168554	1126387	35.46%	2.762%
7	6.517	750	753	757	rBV	1755030	1503019	47.32%	3.686%
8	6.746	789	792	808	rVB	1593292	1329843	41.87%	3.261%
9	7.134	854	858	873	rBV	2007762	1725850	54.33%	4.232%
10	7.305	884	887	891	rBV	1446698	1225947	38.60%	3.007%
11	7.634	939	943	954	rBV	1266706	1016813	32.01%	2.494%
12	7.881	982	985	1007	rBV	2062972	1712369	53.91%	4.199%
13	8.034	1007	1011	1014	rBV	1994137	1708235	53.78%	4.189%
14	8.093	1017	1021	1024	rBV	2048833	1611721	50.74%	3.953%
15	8.716	1124	1127	1138	rBV	27701	28427	0.89%	0.070%
16	8.816	1141	1144	1149	rVB2	3388	3706	0.12%	0.009%
17	9.487	1255	1258	1262	rBV	2264038	2016738	63.49%	4.946%
18	9.552	1267	1269	1274	rVB4	3444	3969	0.12%	0.010%
19	9.640	1280	1284	1288	rBV	3117036	2693296	84.79%	6.605%
20	9.799	1307	1311	1314	rBV	2351622	2004847	63.12%	4.917%
21	9.910	1327	1330	1344	rBV	612912	696500	21.93%	1.708%
22	10.010	1344	1347	1360	rVB2	18085	29220	0.92%	0.072%
23	10.210	1378	1381	1385	rVB	6928	6262	0.20%	0.015%
24	10.322	1396	1400	1403	rBV	3298090	3021319	95.12%	7.409%
25	10.393	1409	1412	1419	rBV	518011	461480	14.53%	1.132%
26	10.446	1419	1421	1431	rVB	52422	53001	1.67%	0.130%
27	10.746	1469	1472	1476	rVB	15296	12753	0.40%	0.031%
28	11.110	1529	1534	1538	rBV2	7587	6696	0.21%	0.016%
29	11.175	1541	1545	1550	rBV	7577	9138	0.29%	0.022%
30	11.293	1562	1565	1569	rBV	2236935	1965459	61.88%	4.820%
31	11.352	1571	1575	1579	rBV	3445044	2975030	93.66%	7.296%
32	11.516	1601	1603	1608	rVB	3178	3681	0.12%	0.009%
33	12.022	1684	1689	1695	rBV9	2145	5537	0.17%	0.014%
34	12.504	1767	1771	1779	rBV	35749	32437	1.02%	0.080%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000820.D
Acq On : 16 Oct 2019 18:10
Operator : JU
Sample : PB123786BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK86

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

35	12.663	1794	1798	1802	rBV	31790	27442	0.86%	0.067%
36	12.740	1807	1811	1814	rBV	3570779	3176403	100.00%	7.790%
37	13.393	1919	1922	1927	rBV3	6375	7872	0.25%	0.019%
38	13.828	1993	1996	2000	rBV2	7222	7561	0.24%	0.019%
39	13.969	2016	2020	2031	rVB	2000494	1890112	59.50%	4.635%
40	14.146	2048	2050	2053	rBV2	5301	5159	0.16%	0.013%
41	14.457	2100	2103	2107	rBV	14297	14715	0.46%	0.036%
42	14.769	2153	2156	2160	rBV	25148	23285	0.73%	0.057%
43	14.975	2187	2191	2195	rBV	34661	38959	1.23%	0.096%
44	15.110	2210	2214	2220	rBV2	32018	45875	1.44%	0.113%
45	15.363	2251	2257	2266	rBV	2481820	2970427	93.52%	7.285%
46	15.451	2267	2272	2277	rVV	1612349	1918264	60.39%	4.704%
47	15.493	2277	2279	2294	rVB	49135	69884	2.20%	0.171%
48	15.934	2350	2354	2360	rVB	31338	44934	1.41%	0.110%
49	16.016	2365	2368	2373	rVB3	13533	19623	0.62%	0.048%
50	16.440	2436	2440	2450	rVB4	23599	45169	1.42%	0.111%
51	17.039	2537	2542	2549	rVB4	14852	32683	1.03%	0.080%


Sum of corrected areas: 40776302

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000820.D
Acq On : 16 Oct 2019 18:10
Operator : JU
Sample : PB123786BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK86

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

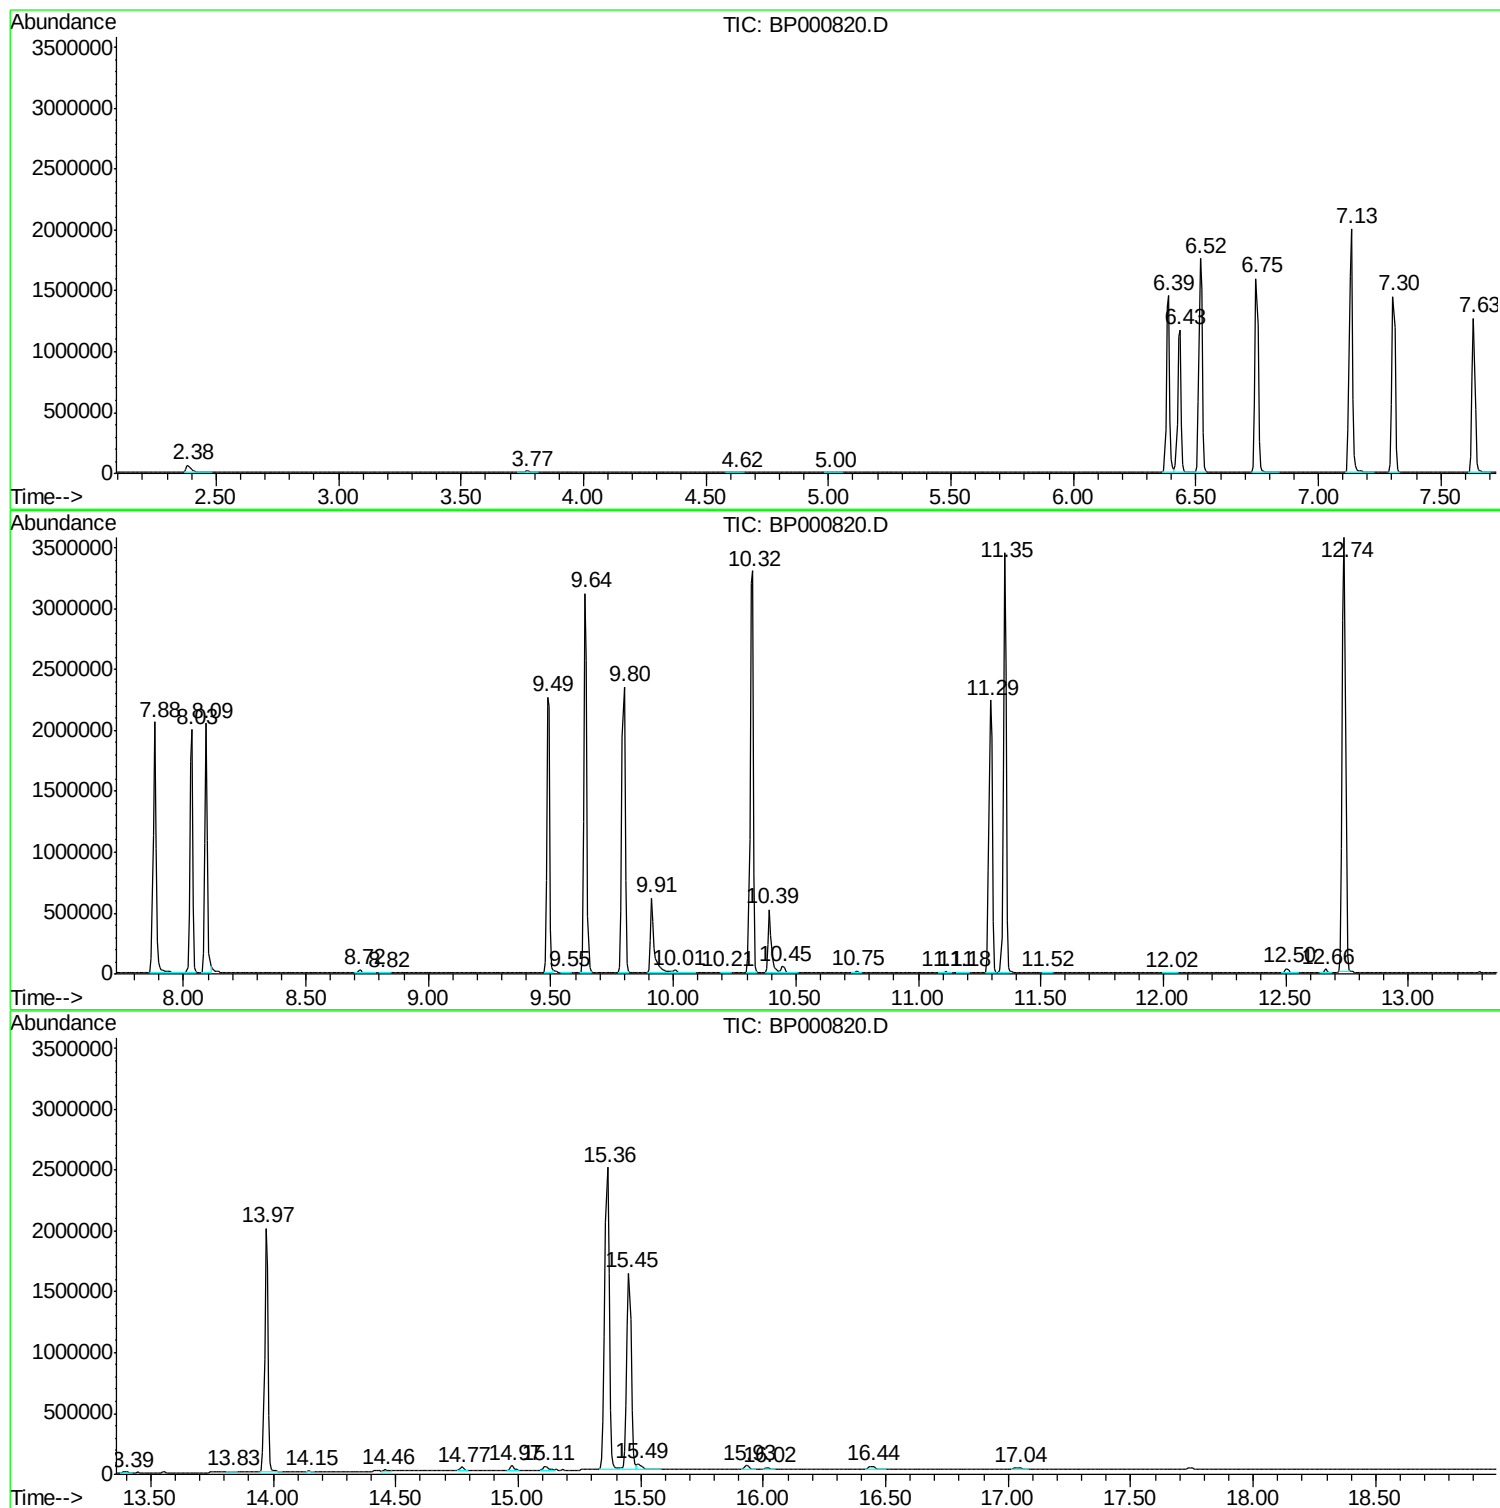

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
Data File : BP000820.D
Acq On : 16 Oct 2019 18:10
Operator : JU
Sample : PB123786BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK86

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
Data File : BP000820.D
Acq On : 16 Oct 2019 18:10
Operator : JU
Sample : PB123786BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK86

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc