

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000841.D
 Acq On : 17 Oct 2019 15:11
 Operator : JU
 Sample : PB124015TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB29

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	48	50	60	rVB	9063	13541	0.46%	0.040%
2	3.675	265	270	274	rBV	2499	4046	0.14%	0.012%
3	3.728	274	279	280	rVV	6473	7657	0.26%	0.023%
4	3.763	280	285	298	rVB	93947	142128	4.85%	0.421%
5	6.063	668	676	682	rBV3	4972	8912	0.30%	0.026%
6	6.387	728	731	735	rBV2	260300	284701	9.71%	0.844%
7	6.428	735	738	750	rVV	956441	843503	28.76%	2.500%
8	6.522	750	754	764	rVV	979716	920565	31.38%	2.728%
9	6.745	789	792	802	rBV	1338784	1121778	38.24%	3.324%
10	6.816	802	804	811	rVB2	6103	6678	0.23%	0.020%
11	7.134	855	858	874	rBV	874954	774680	26.41%	2.296%
12	7.304	884	887	894	rBV	1095612	938076	31.98%	2.780%
13	7.457	908	913	917	rBV7	2933	3442	0.12%	0.010%
14	7.522	921	924	927	rBV	16462	13233	0.45%	0.039%
15	7.575	927	933	935	rBV4	3781	5672	0.19%	0.017%
16	7.634	940	943	959	rVB	971164	773764	26.38%	2.293%
17	7.822	972	975	982	rBV	8628	10567	0.36%	0.031%
18	7.881	982	985	1004	rVV	1234526	1274805	43.46%	3.778%
19	8.034	1007	1011	1014	rVV	1783166	1496565	51.02%	4.435%
20	8.098	1018	1022	1031	rVB	85673	97315	3.32%	0.288%
21	8.722	1124	1128	1136	rBV	20359	22897	0.78%	0.068%
22	9.204	1206	1210	1212	rBV2	8127	8507	0.29%	0.025%
23	9.287	1218	1224	1230	rBV5	2439	4866	0.17%	0.014%
24	9.492	1255	1259	1261	rBV	2014324	1756107	59.87%	5.204%
25	9.510	1261	1262	1273	rVB	230729	156005	5.32%	0.462%
26	9.639	1281	1284	1288	rBV	2582285	2265829	77.25%	6.714%
27	9.734	1297	1300	1304	rVB	5256	5417	0.18%	0.016%
28	9.798	1307	1311	1314	rBV	2195914	1824252	62.19%	5.406%
29	9.892	1324	1327	1330	rBV2	4984	4236	0.14%	0.013%
30	9.928	1330	1333	1345	rVV	68684	114952	3.92%	0.341%
31	10.010	1345	1347	1352	rVB5	6918	8143	0.28%	0.024%
32	10.210	1379	1381	1383	rBV	3678	4200	0.14%	0.012%
33	10.239	1383	1386	1389	rVB	22688	16727	0.57%	0.050%
34	10.322	1396	1400	1403	rBV	2998955	2661083	90.72%	7.885%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000841.D
 Acq On : 17 Oct 2019 15:11
 Operator : JU
 Sample : PB124015TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB29

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	10.392	1409	1412	1419	rBV	474426	441918	15.07%	1.310%
36	10.445	1419	1421	1430	rVB	41254	49098	1.67%	0.145%
37	10.633	1450	1453	1455	rBV3	3560	3777	0.13%	0.011%
38	10.692	1460	1463	1465	rVV3	4915	5211	0.18%	0.015%
39	10.716	1465	1467	1469	rVV2	9215	8208	0.28%	0.024%
40	10.745	1469	1472	1476	rVB3	13920	14743	0.50%	0.044%
41	10.869	1490	1493	1496	rVB	4097	3482	0.12%	0.010%
42	11.110	1531	1534	1537	rBV	6506	5071	0.17%	0.015%
43	11.169	1541	1544	1552	rBV2	26873	25922	0.88%	0.077%
44	11.251	1555	1558	1562	rBV5	3597	3911	0.13%	0.012%
45	11.292	1562	1565	1569	rBV	2063992	1878947	64.06%	5.568%
46	11.351	1571	1575	1579	rBV	3010357	2693021	91.81%	7.980%
47	11.598	1615	1617	1623	rVB	5670	5868	0.20%	0.017%
48	11.669	1627	1629	1637	rVB	9886	11148	0.38%	0.033%
49	11.833	1655	1657	1660	rBV2	12314	12742	0.43%	0.038%
50	11.869	1660	1663	1666	rVB	42418	34812	1.19%	0.103%
51	11.963	1677	1679	1682	rVB2	3390	3277	0.11%	0.010%
52	12.016	1684	1688	1692	rBV3	18740	18780	0.64%	0.056%
53	12.380	1747	1750	1752	rBV	7478	7189	0.25%	0.021%
54	12.410	1752	1755	1760	rVB	20140	18293	0.62%	0.054%
55	12.504	1768	1771	1773	rBV	35527	31964	1.09%	0.095%
56	12.522	1773	1774	1777	rVB	15137	11180	0.38%	0.033%
57	12.663	1795	1798	1802	rVB	30135	25918	0.88%	0.077%
58	12.739	1807	1811	1814	rVV	3314746	2933242	100.00%	8.692%
59	12.786	1816	1819	1821	rVV	27949	28834	0.98%	0.085%
60	12.804	1821	1822	1826	rVB3	12949	10096	0.34%	0.030%
61	13.145	1877	1880	1889	rBV	37029	33766	1.15%	0.100%
62	13.369	1914	1918	1922	rBV6	4331	8668	0.30%	0.026%
63	13.492	1936	1939	1942	rBV	68643	54837	1.87%	0.162%
64	13.557	1947	1950	1953	rVB4	2640	3660	0.12%	0.011%
65	13.704	1973	1975	1978	rVB3	5091	4201	0.14%	0.012%
66	13.827	1992	1996	2005	rBV2	118785	132413	4.51%	0.392%
67	13.974	2016	2021	2024	rBV	1834961	1802428	61.45%	5.341%
68	14.063	2034	2036	2044	rVB5	6336	8107	0.28%	0.024%
69	14.151	2047	2051	2055	rBV	120182	117217	4.00%	0.347%
70	14.345	2082	2084	2087	rVB2	6261	4440	0.15%	0.013%
71	14.374	2087	2089	2093	rVB2	5682	6279	0.21%	0.019%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000841.D
Acq On : 17 Oct 2019 15:11
Operator : JU
Sample : PB124015TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB29

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

72	14.457	2100	2103	2113	rBV	152597	145386	4.96%	0.431%
73	14.769	2152	2156	2163	rBV	159796	163316	5.57%	0.484%
74	14.839	2165	2168	2174	rVB	32794	36848	1.26%	0.109%
75	14.974	2188	2191	2196	rBV	33625	35991	1.23%	0.107%
76	15.021	2197	2199	2202	rVB2	8870	7675	0.26%	0.023%
77	15.110	2210	2214	2224	rBV	141380	170542	5.81%	0.505%
78	15.363	2251	2257	2264	rBV	2258550	2721542	92.78%	8.065%
79	15.451	2267	2272	2277	rVV	1479903	1951973	66.55%	5.784%
80	15.492	2277	2279	2293	rVB	140248	184111	6.28%	0.546%
81	15.933	2349	2354	2363	rBV	82852	131592	4.49%	0.390%
82	16.439	2435	2440	2450	rBV	48160	97526	3.32%	0.289%
83	17.039	2538	2542	2553	rVB3	19829	42797	1.46%	0.127%


Sum of corrected areas: 33746816

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000841.D
Acq On : 17 Oct 2019 15:11
Operator : JU
Sample : PB124015TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB29

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

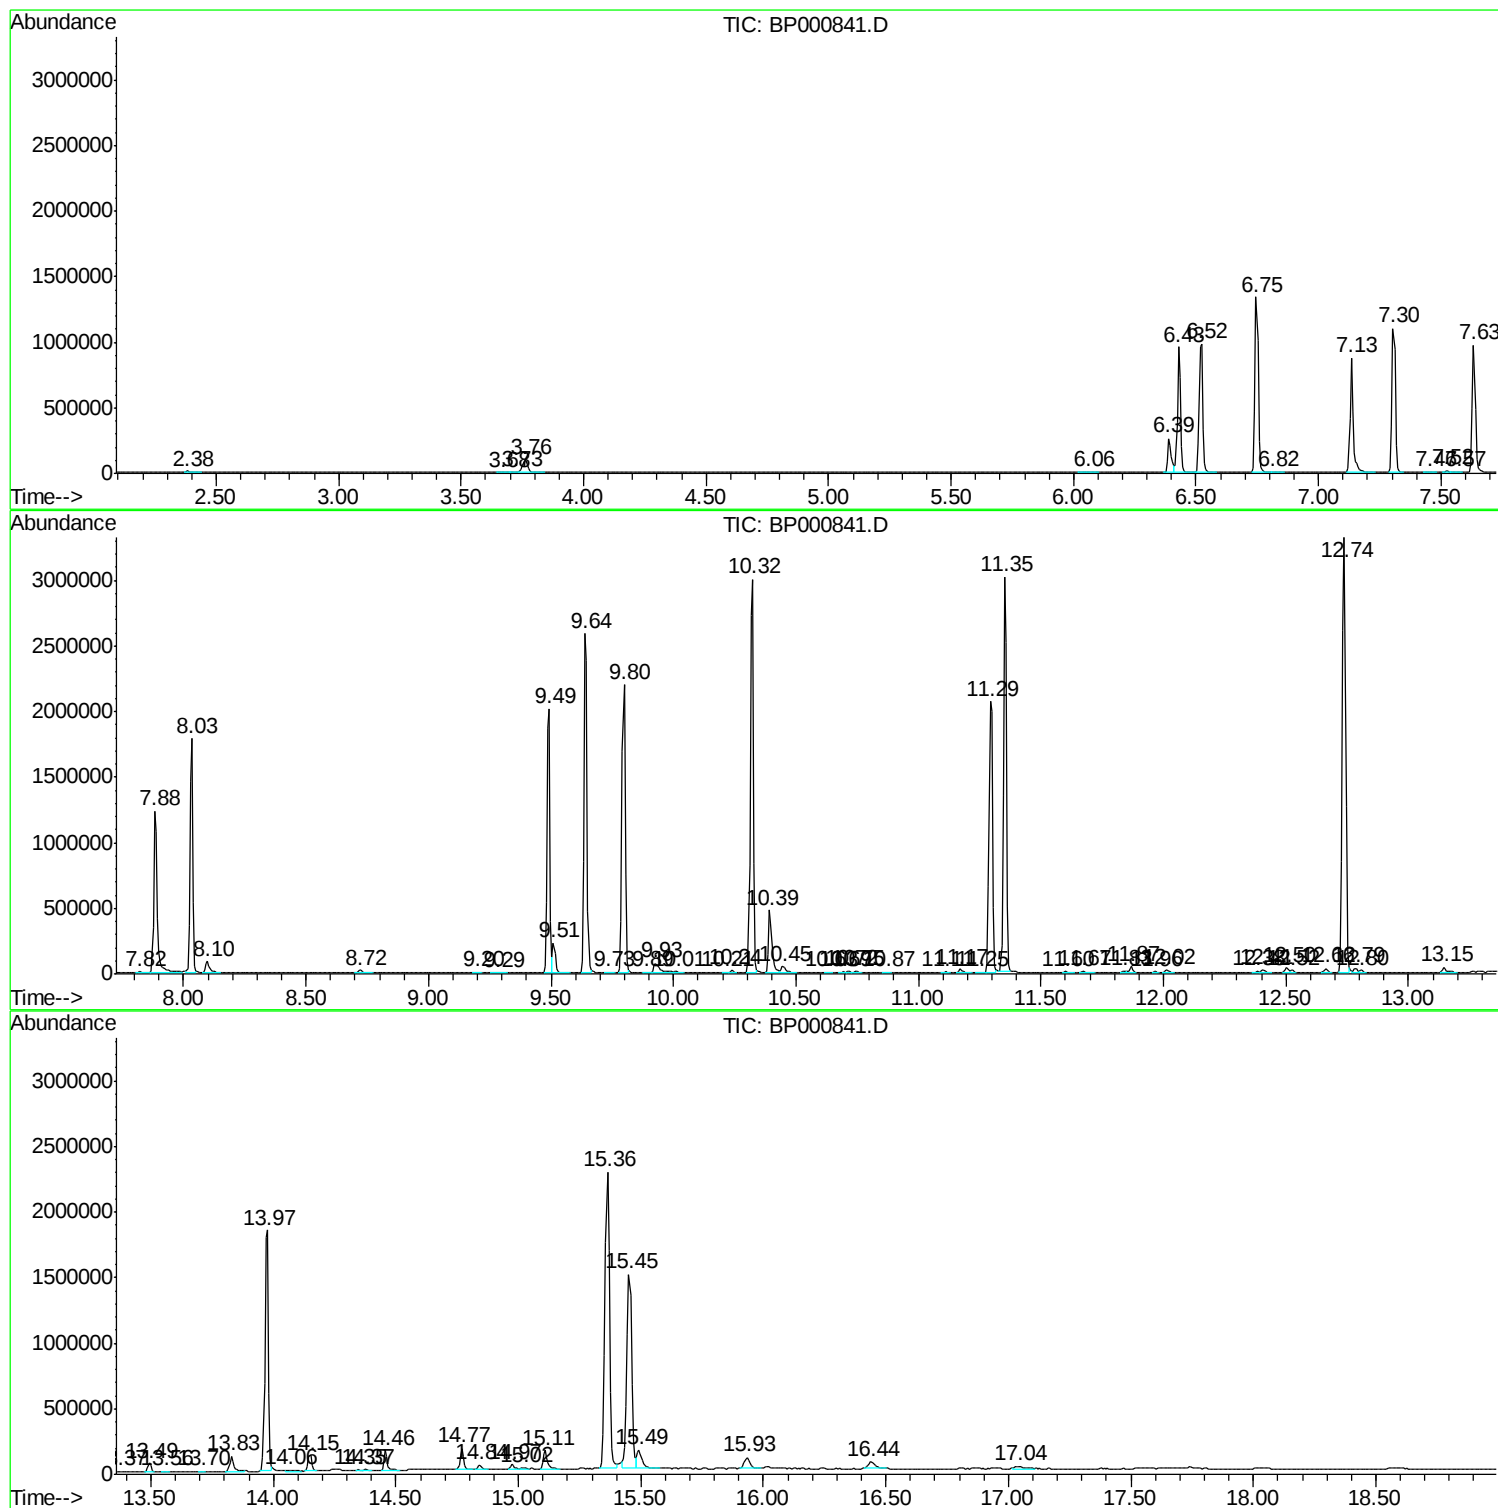

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
Data_File : BP000841.D
Acq_On : 17 Oct 2019 15:111
Operator : JUJ
Sample : PB124015TBB
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
SLEB29

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.MM
Quant_Title : SVOA CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
