

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
 Data File : BP000843.D
 Acq On : 17 Oct 2019 15:59
 Operator : JU
 Sample : PB124015BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.358	43	46	59	rBV	42766	64445	2.16%	0.184%
2	3.752	279	283	292	rVB	6203	9889	0.33%	0.028%
3	6.387	728	731	735	rBV	1211102	1016211	34.04%	2.895%
4	6.428	735	738	750	rVV	904526	887714	29.73%	2.529%
5	6.522	750	754	764	rVB	1307168	1170591	39.21%	3.335%
6	6.746	789	792	812	rVB	1103511	965060	32.32%	2.750%
7	7.134	855	858	873	rBV	1677917	1345381	45.06%	3.833%
8	7.305	884	887	891	rBV	1101060	953844	31.95%	2.718%
9	7.634	940	943	961	rVB	1008922	787367	26.37%	2.243%
10	7.881	982	985	1007	rBV	1450827	1368744	45.85%	3.900%
11	8.034	1007	1011	1014	rVV	1609496	1289250	43.18%	3.673%
12	8.093	1018	1021	1038	rVB	1641621	1329314	44.53%	3.788%
13	8.722	1124	1128	1136	rBV	20003	22406	0.75%	0.064%
14	9.281	1218	1223	1228	rVB4	2746	3569	0.12%	0.010%
15	9.487	1255	1258	1262	rBV	2037526	1723218	57.72%	4.910%
16	9.640	1281	1284	1288	rBV	2733012	2271945	76.10%	6.473%
17	9.799	1307	1311	1314	rBV	1914704	1629583	54.58%	4.643%
18	9.916	1327	1331	1344	rBV	454861	588489	19.71%	1.677%
19	10.010	1344	1347	1352	rVB2	10939	14339	0.48%	0.041%
20	10.322	1396	1400	1403	rBV	2957578	2667394	89.34%	7.600%
21	10.393	1409	1412	1419	rBV	506383	444732	14.90%	1.267%
22	10.446	1419	1421	1431	rVB	44666	45261	1.52%	0.129%
23	10.746	1469	1472	1481	rVB2	13043	12136	0.41%	0.035%
24	11.110	1531	1534	1539	rVB2	6130	5596	0.19%	0.016%
25	11.175	1541	1545	1551	rBV2	6375	7096	0.24%	0.020%
26	11.293	1562	1565	1569	rBV	2020294	1753250	58.72%	4.995%
27	11.351	1571	1575	1579	rBV	3135814	2681621	89.82%	7.641%
28	12.045	1685	1693	1697	rBV9	3617	8856	0.30%	0.025%
29	12.504	1768	1771	1781	rBV	33794	30548	1.02%	0.087%
30	12.663	1793	1798	1802	rBV	29399	25548	0.86%	0.073%
31	12.740	1807	1811	1814	rBV	3402764	2985533	100.00%	8.506%
32	12.804	1820	1822	1825	rVB2	5971	5536	0.19%	0.016%
33	13.292	1902	1905	1908	rBV2	2911	3606	0.12%	0.010%
34	13.445	1928	1931	1935	rVB2	13650	11857	0.40%	0.034%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000843.D
Acq On : 17 Oct 2019 15:59
Operator : JU
Sample : PB124015BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK15

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

35	13.828	1993	1996	2004	rVB2	8380	12732	0.43%	0.036%
36	13.969	2016	2020	2037	rBV	1852756	1763375	59.06%	5.024%
37	14.145	2047	2050	2056	rBV	10510	12117	0.41%	0.035%
38	14.457	2100	2103	2108	rBV2	18513	18559	0.62%	0.053%
39	14.769	2153	2156	2161	rVB	38212	38724	1.30%	0.110%
40	14.975	2188	2191	2195	rBV	29941	30761	1.03%	0.088%
41	15.110	2210	2214	2223	rVB2	44327	64355	2.16%	0.183%
42	15.363	2251	2257	2266	rBV	2471373	2883660	96.59%	8.216%
43	15.451	2267	2272	2277	rVV2	1462463	1833231	61.40%	5.223%
44	15.492	2277	2279	2292	rVB	70413	95516	3.20%	0.272%
45	15.928	2349	2353	2363	rBV	41801	69922	2.34%	0.199%
46	16.016	2365	2368	2373	rVB4	12564	16862	0.56%	0.048%
47	16.439	2435	2440	2451	rVB	39220	78445	2.63%	0.224%
48	17.033	2536	2541	2549	rBV3	22138	49115	1.65%	0.140%


Sum of corrected areas: 35097303

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101719\
Data File : BP000843.D
Acq On : 17 Oct 2019 15:59
Operator : JU
Sample : PB124015BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

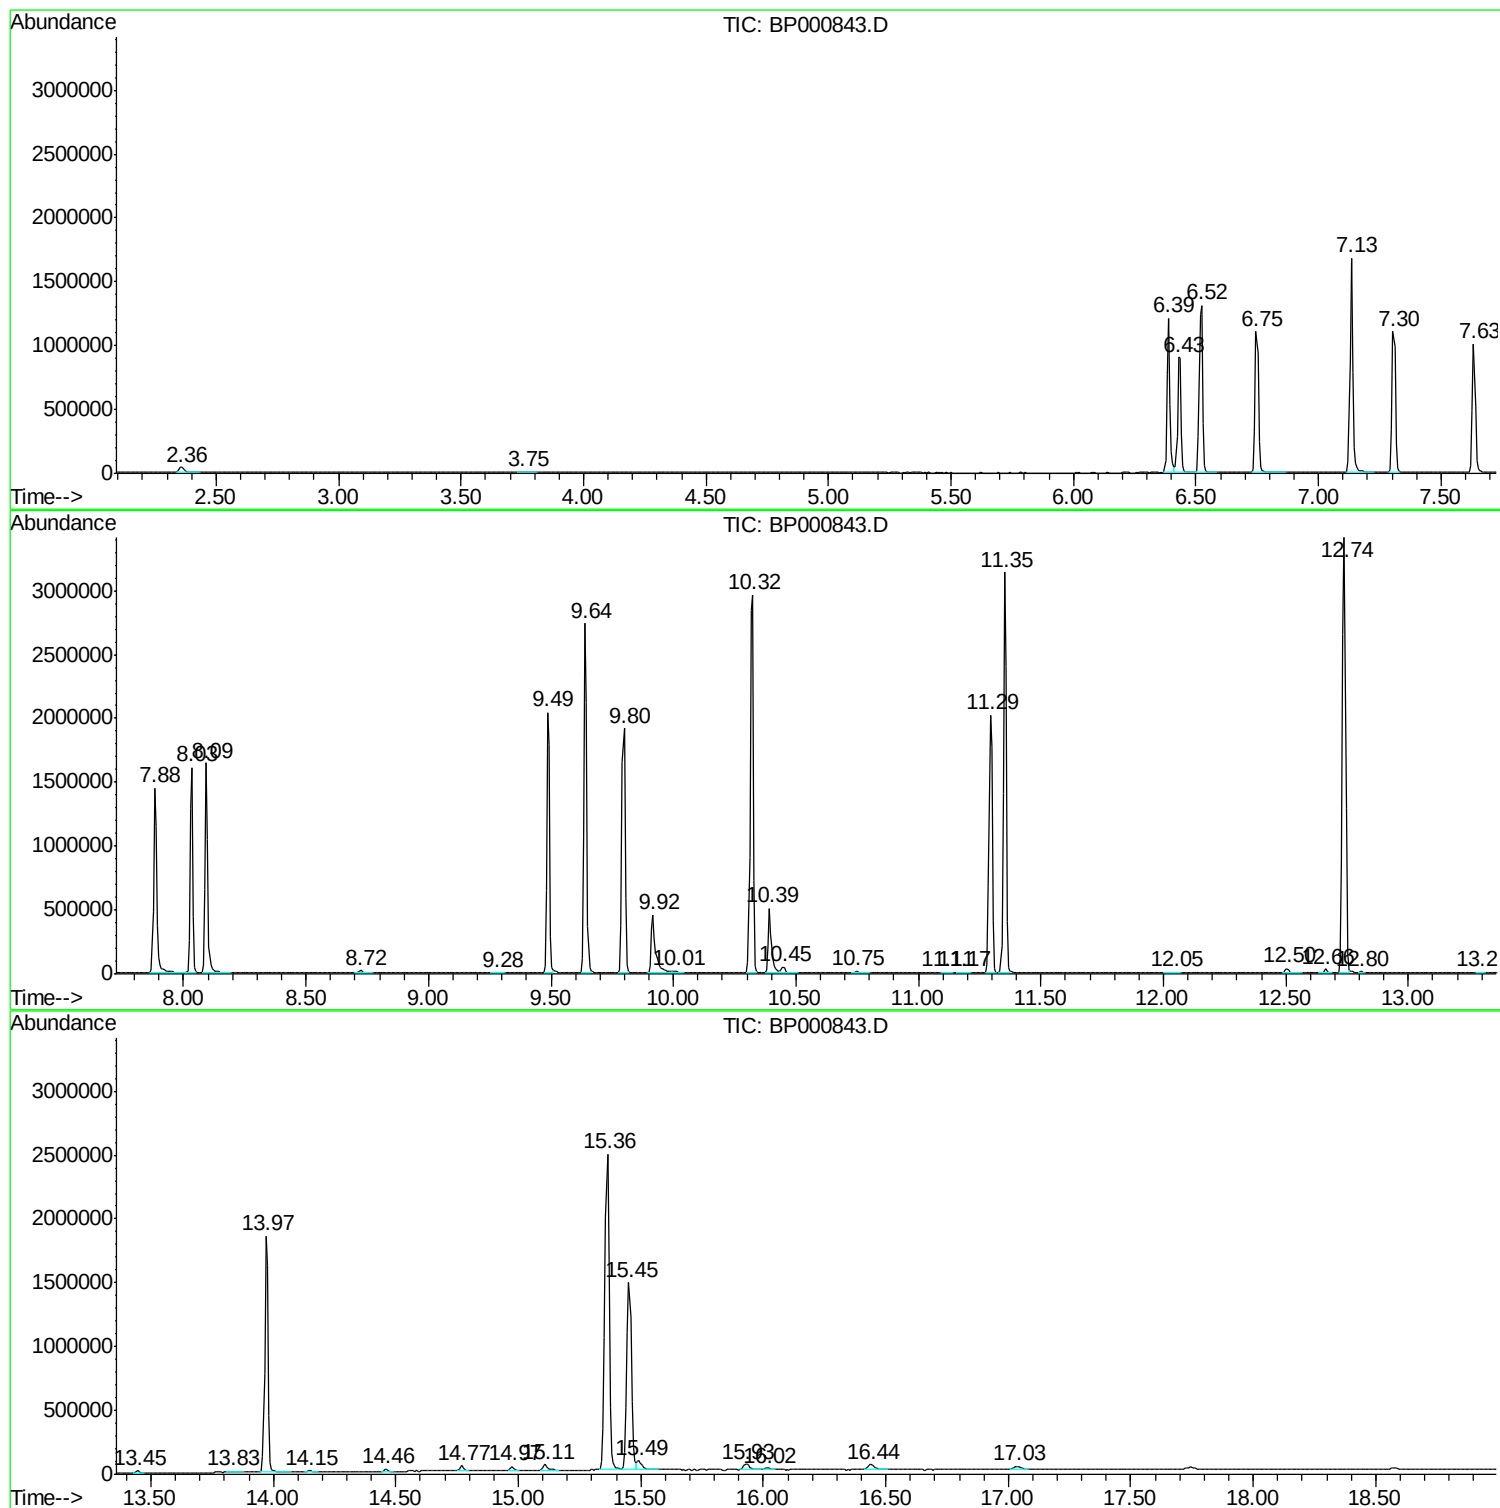

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
Data File : BP000843.D
Acq On : 17 Oct 2019 15:59
Operator : JU
Sample : PB124015BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101719\
Data File : BP000843.D
Acq On : 17 Oct 2019 15:59
Operator : JU
Sample : PB124015BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK15

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc