

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017709.D
 Acq On : 17 Oct 2023 21:32
 Operator : MA/JU
 Sample : 04864-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJV5

Quant Time: Oct 18 00:45:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 12 16:14:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	108590	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	434481	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	280242	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	646760	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	714211	20.000	ng/ul	-0.01
88) Perylene-d12	24.098	264	826224	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	18059	6.131	ng/uL	0.00
4) Pyridine-d5	3.699	84	169543	20.824	ng/ul	0.00
7) Phenol-d5	7.057	99	154380	15.270	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	219270	35.764	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.416	132	254084	32.469	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	216392	26.798	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	136134	37.303	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.822	143	147596	35.964	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.351	165	281413	36.484	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131	342437	30.973	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	965181	39.767	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	1008005	38.567	ng/ul	0.00
54) 4-Nitrophenol-d4	14.863	143	51278	12.633	ng/ul	0.01
60) Fluorene-d10	15.604	176	836041	40.495	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	126719	27.720	ng/ul	0.00
73) Anthracene-d10	17.492	188	1377955	41.271	ng/ul	0.00
81) Pyrene-d10	19.751	212	1742995	40.548	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	1926500	41.534	ng/ul	-0.01
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.151	77	35938	3.834	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017709.D
Acq On : 17 Oct 2023 21:32
Operator : MA/JU
Sample : 04864-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCJV5

Quant Time: Oct 18 00:45:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 12 16:14:36 2023
Response via : Initial Calibration

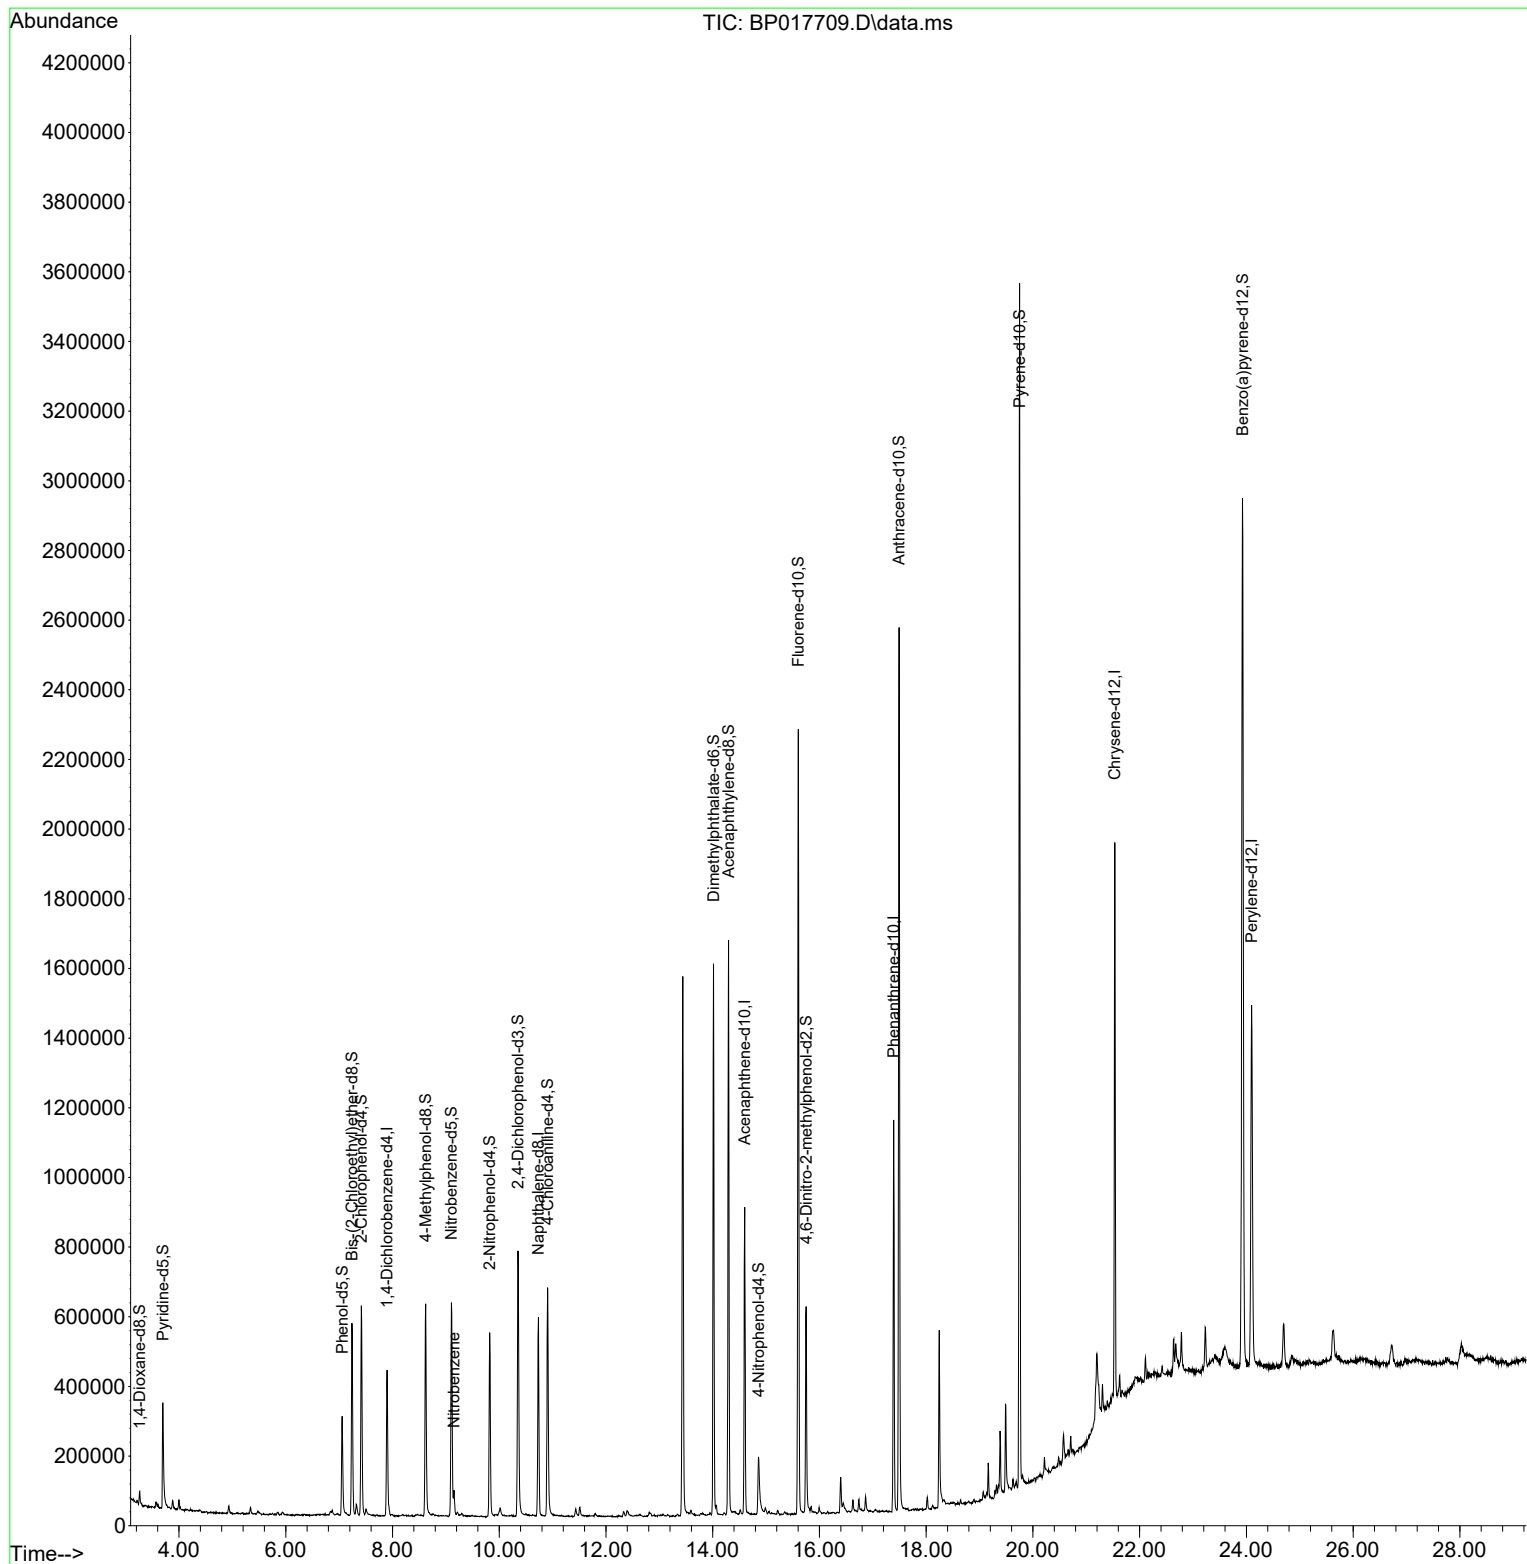

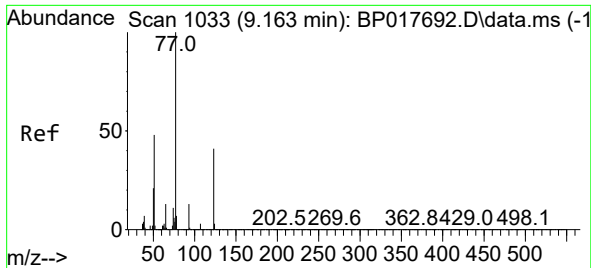

#22
 Nitrobenzene
 Concen: 3.834 ng/ul
 RT: 9.151 min Scan# 10
 Delta R.T. -0.006 min
 Lab File: BP017709.D
 Acq: 17 Oct 2023 21:32

Instrument :
 BNA_P
 ClientSampleId :
 DCJV5

Tgt Ion:	77	Resp:	35938
Ion	Ratio	Lower	Upper
77	100		
123	40.9	33.8	50.6
65	14.1	10.6	16.0

