




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017707.D
 Acq On : 17 Oct 2023 20:24
 Operator : MA/JU
 Sample : 04852-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJV3

Manual IntegrationsAPPROVED

Quant Time: Oct 18 00:45:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 12 16:14:36 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2023
 Supervised By :mohammad ahmed 10/19/2023

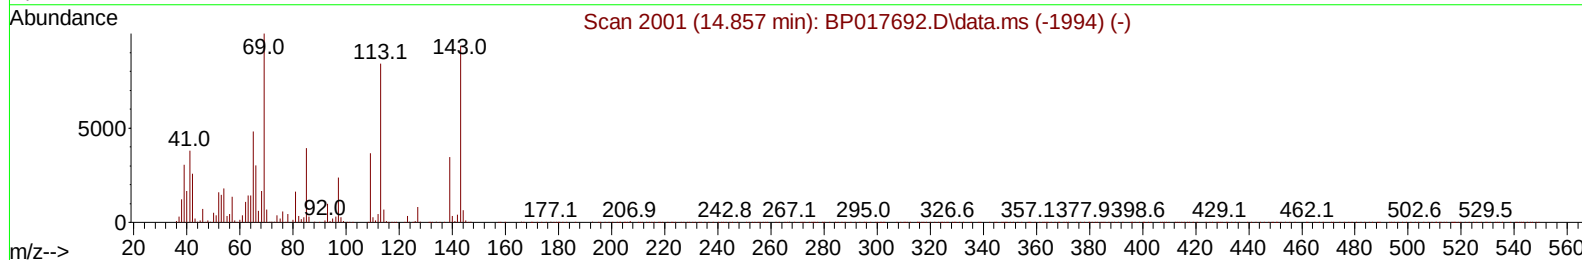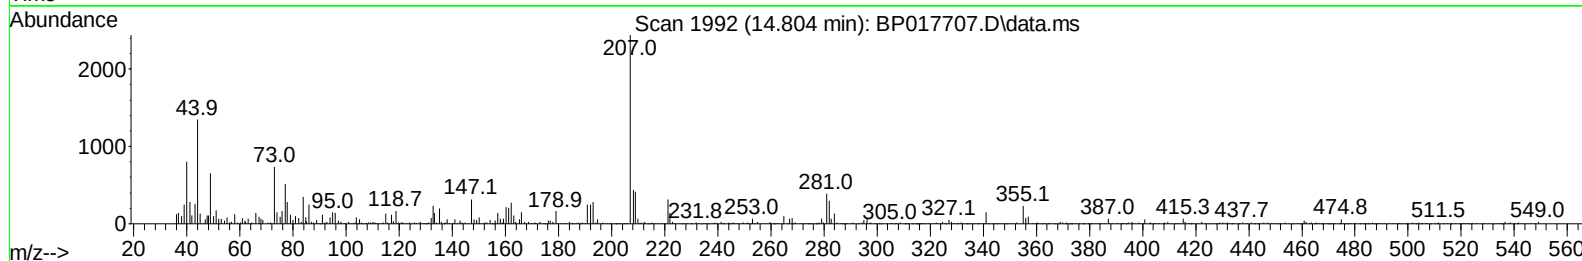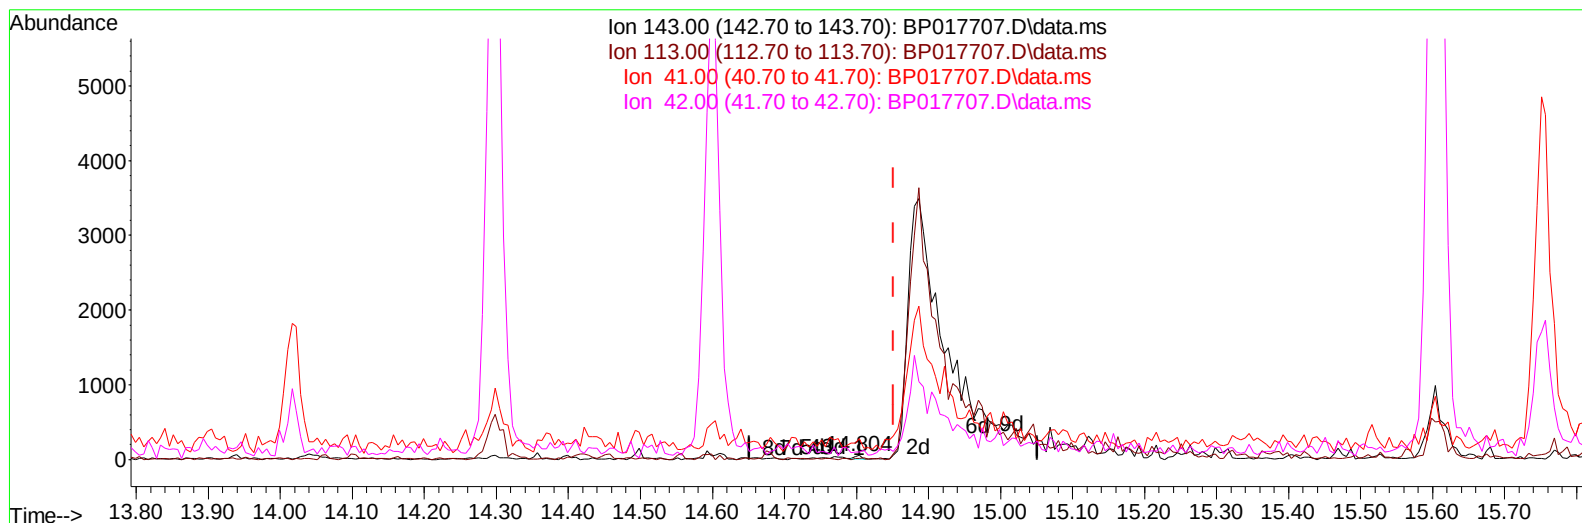

TIC: BP017707.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (-0.047) 0.01 ng/u1

response 32

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	82.30	19.64#
41.00	41.10	498.21#
42.00	27.50	185.71#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017707.D
 Acq On : 17 Oct 2023 20:24
 Operator : MA/JU
 Sample : 04852-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJV3

Manual IntegrationsAPPROVED

Quant Time: Oct 18 00:45:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 12 16:14:36 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2023
 Supervised By :mohammad ahmed 10/19/2023

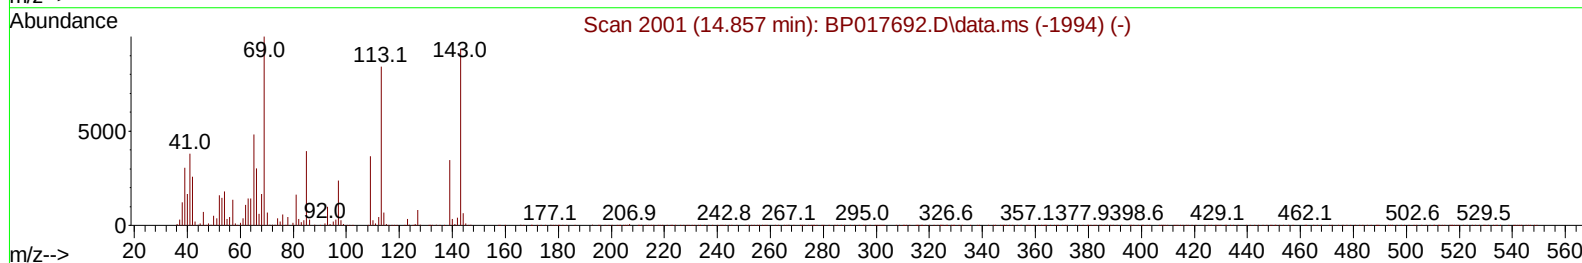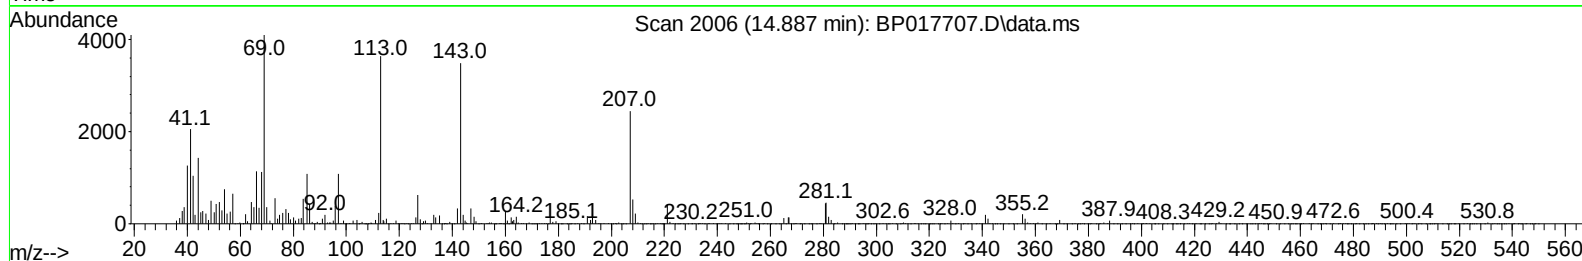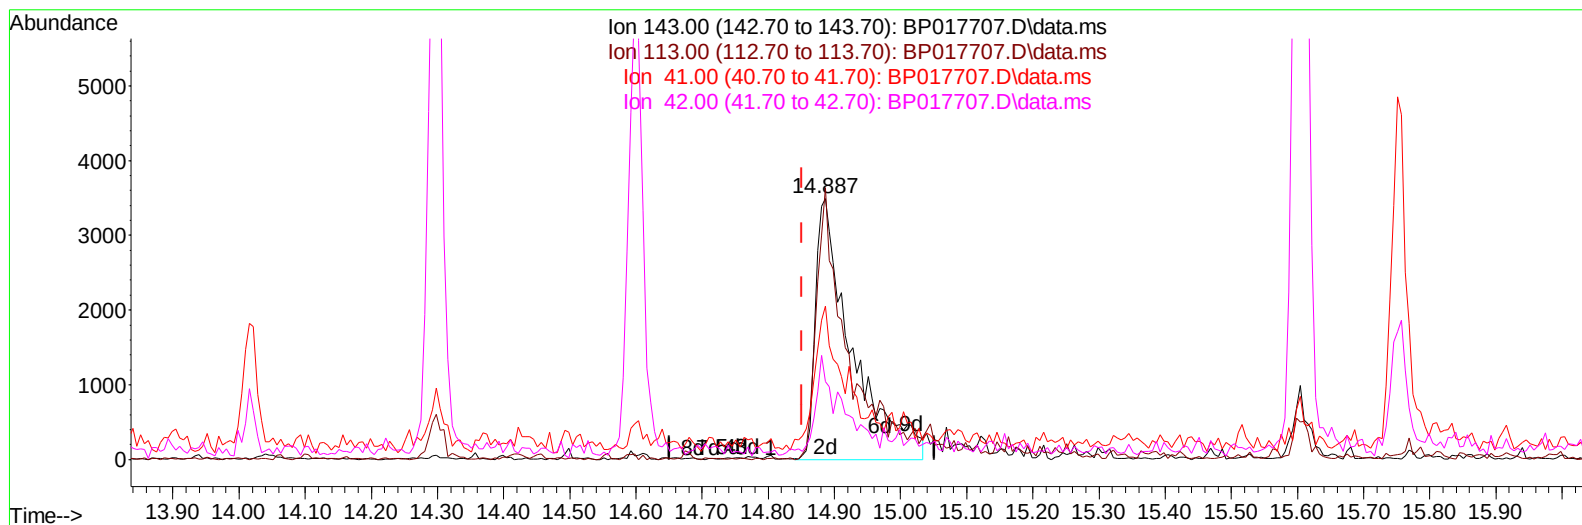

TIC: BP017707.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.887min (+ 0.035) 4.13 ng/ul m

response 13309

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	82.30	104.01#
41.00	41.10	58.79#
42.00	27.50	29.74

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017707.D
 Acq On : 17 Oct 2023 20:24
 Operator : MA/JU
 Sample : 04852-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJV3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2023
 Supervised By :mohammad ahmed 10/19/2023

Quant Time: Oct 18 01:07:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 12 16:14:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	87924	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	355185	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	222498	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	524175	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	574172	20.000	ng/ul	-0.01
88) Perylene-d12	24.098	264	686012	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	6770	2.839	ng/uL	0.00
4) Pyridine-d5	3.705	84	76523	11.608	ng/ul	0.00
7) Phenol-d5	7.064	99	49974	6.105	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	187834	37.838	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.422	132	173586	27.396	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	99505	15.219	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	113739	38.125	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	113920	33.955	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	190369	30.191	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	266698	29.508	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	742803	38.547	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	797021	38.409	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	13309m	4.130	ng/ul	0.04
60) Fluorene-d10	15.604	176	671841	40.987	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	91512	24.700	ng/ul	0.00
73) Anthracene-d10	17.492	188	1119712	41.379	ng/ul	0.00
81) Pyrene-d10	19.751	212	1415936	40.973	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	1579769	41.020	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017707.D
Acq On : 17 Oct 2023 20:24
Operator : MA/JU
Sample : 04852-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCJV3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2023
Supervised By :mohammad ahmed 10/19/2023

Quant Time: Oct 18 01:07:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 12 16:14:36 2023
Response via : Initial Calibration

