

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017693.D
 Acq On : 17 Oct 2023 10:24
 Operator : MA/JU
 Sample : PB156333BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK333

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB	42448	53347	1.33%	0.153%
2	3.699	100	104	119	rBV	463259	711371	17.76%	2.039%
3	7.064	670	676	693	rVV	521398	857732	21.41%	2.459%
4	7.252	702	708	718	rBV	443527	683721	17.07%	1.960%
5	7.428	731	738	753	rBV	574244	923571	23.06%	2.647%
6	7.905	813	819	830	rBV	467743	771684	19.27%	2.212%
7	8.546	924	928	932	rBV7	2413	4759	0.12%	0.014%
8	8.628	934	942	959	rBV2	597038	1050966	26.24%	3.013%
9	9.116	1015	1025	1039	rBV	495722	854513	21.33%	2.450%
10	9.310	1053	1058	1062	rVB7	2565	5163	0.13%	0.015%
11	9.834	1140	1147	1162	rBV	411585	705932	17.62%	2.024%
12	10.269	1218	1221	1227	rBV7	2681	4764	0.12%	0.014%
13	10.363	1229	1237	1254	rBV	529641	1032778	25.78%	2.961%
14	10.746	1293	1302	1312	rBV	631009	1050223	26.22%	3.011%
15	10.916	1324	1331	1345	rBV	614439	1117873	27.91%	3.204%
16	12.357	1571	1576	1582	rBV5	9028	18447	0.46%	0.053%
17	13.446	1756	1761	1765	rBV8	6510	10935	0.27%	0.031%
18	14.022	1853	1859	1873	rBV	1078166	1610488	40.21%	4.617%
19	14.134	1877	1878	1882	rVB4	4193	4528	0.11%	0.013%
20	14.304	1899	1907	1924	rBV	1273590	1844284	46.04%	5.287%
21	14.416	1924	1926	1930	rVV5	5373	6502	0.16%	0.019%
22	14.445	1930	1931	1938	rVB6	3771	5352	0.13%	0.015%
23	14.610	1951	1959	1974	rBV	903156	1381629	34.49%	3.961%
24	14.863	1996	2002	2024	rBV	240469	692994	17.30%	1.987%
25	15.398	2089	2093	2095	rVB5	3686	4935	0.12%	0.014%
26	15.616	2120	2130	2148	rBV	1598519	2458179	61.37%	7.047%
27	15.763	2148	2155	2165	rBV	377961	616981	15.40%	1.769%
28	16.392	2259	2262	2267	rBV7	2561	4376	0.11%	0.013%
29	17.063	2373	2376	2382	rVB8	3587	6061	0.15%	0.017%
30	17.187	2395	2397	2403	rBV7	3762	5563	0.14%	0.016%
31	17.398	2427	2433	2444	rBV	1164552	1742193	43.49%	4.994%
32	17.504	2444	2451	2465	rVV	1808568	2691170	67.19%	7.714%
33	18.257	2574	2579	2581	rBV6	8493	13598	0.34%	0.039%
34	19.333	2758	2762	2766	rBV4	23989	30417	0.76%	0.087%
35	19.404	2770	2774	2779	rVB3	23943	36751	0.92%	0.105%
36	19.757	2829	2834	2846	rBV	2643017	3439814	85.88%	9.860%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017693.D
Acq On : 17 Oct 2023 10:24
Operator : MA/JU
Sample : PB156333BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	21.545	3133	3138	3149	rBV	1547388	2135328	53.31%	6.121%
38	23.939	3538	3545	3556	rBV	1917463	4005588	100.00%	11.482%
39	24.110	3568	3574	3587	rVB	1076390	2290442	57.18%	6.566%




Sum of corrected areas: 34884952

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017693.D
Acq On : 17 Oct 2023 10:24
Operator : MA/JU
Sample : PB156333BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

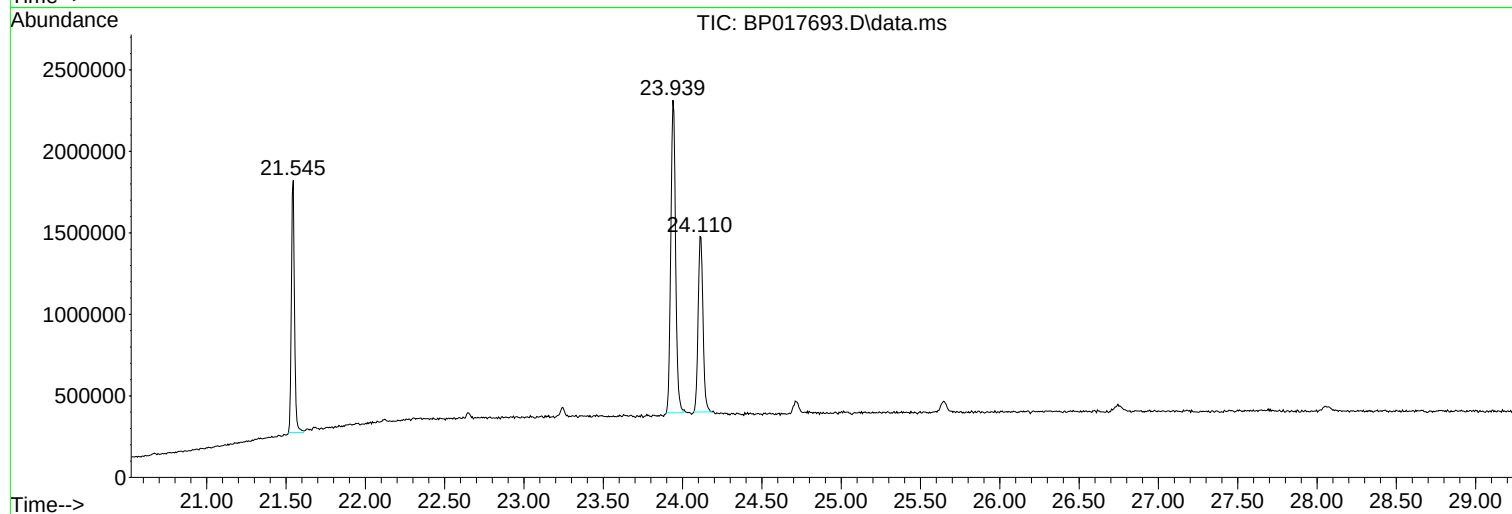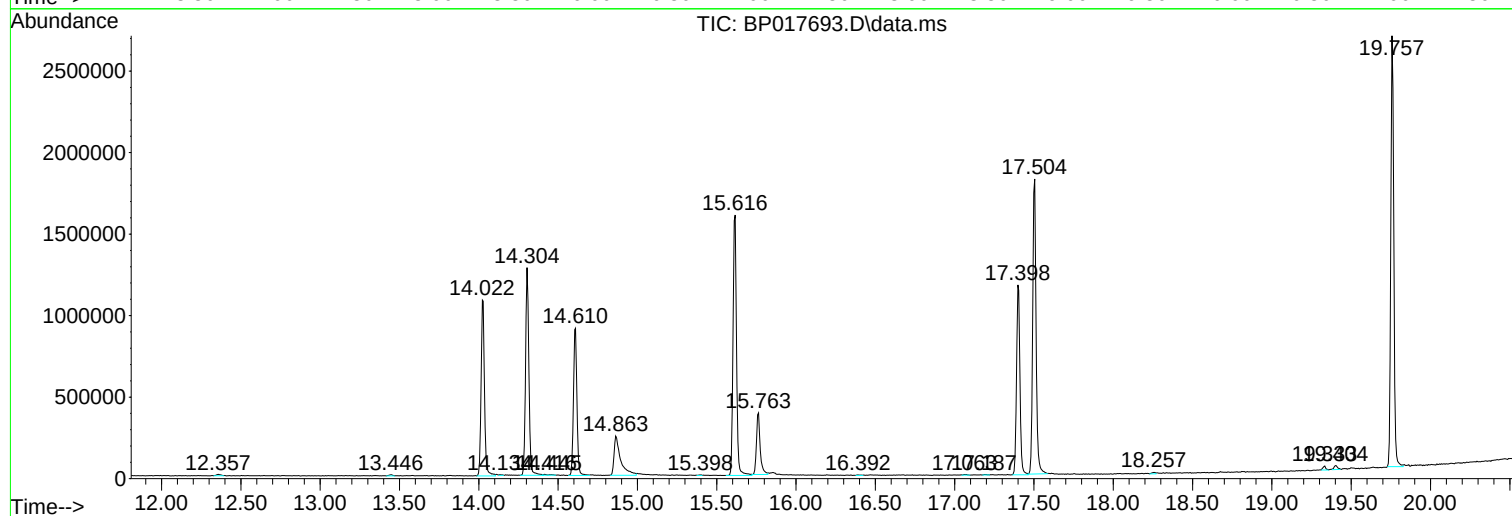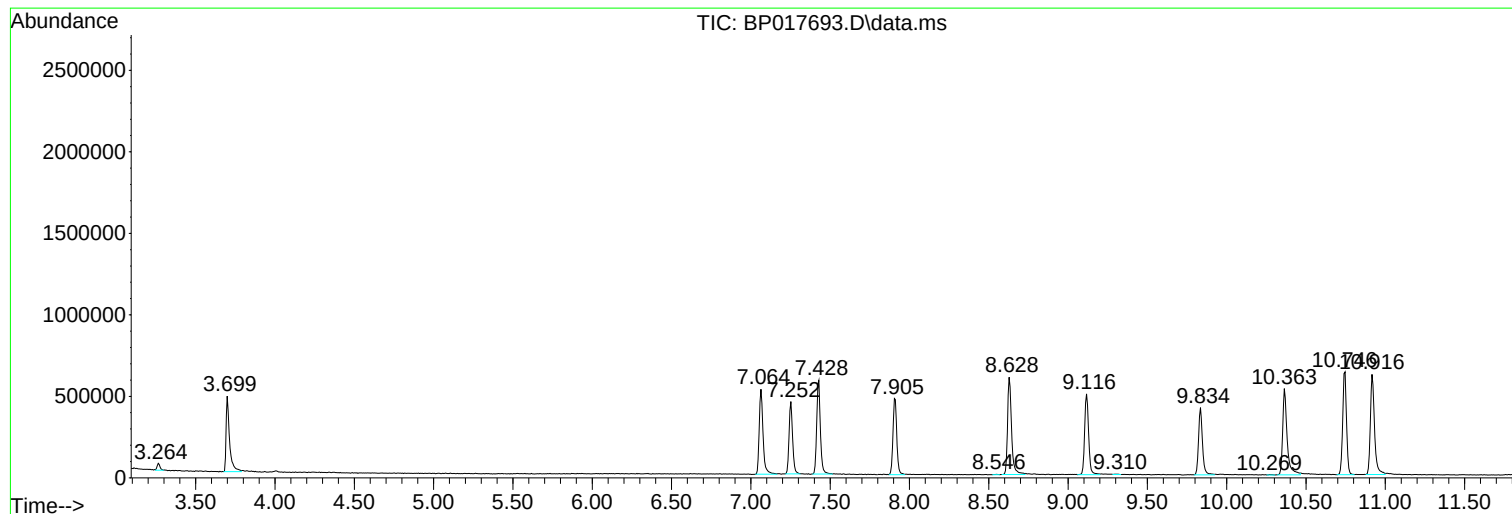

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017693.D
Acq On : 17 Oct 2023 10:24
Operator : MA/JU
Sample : PB156333BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017693.D
Acq On : 17 Oct 2023 10:24
Operator : MA/JU
Sample : PB156333BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------