

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017697.D
 Acq On : 17 Oct 2023 14:38
 Operator : MA/JU
 Sample : PB156335BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB	49434	62878	1.37%	0.156%
2	3.699	101	104	120	rBV	535609	839762	18.29%	2.083%
3	4.005	154	156	161	rVB3	10138	13008	0.28%	0.032%
4	5.234	361	365	368	rVB6	3434	5165	0.11%	0.013%
5	7.069	670	677	690	rBV	645660	1085045	23.63%	2.691%
6	7.258	701	709	721	rBV	536342	844102	18.38%	2.094%
7	7.428	731	738	751	rBV	715481	1110781	24.19%	2.755%
8	7.910	812	820	830	rBV	492808	791317	17.23%	1.963%
9	8.634	932	943	955	rBV	771046	1295440	28.21%	3.213%
10	9.122	1018	1026	1036	rBV	618903	1047123	22.81%	2.597%
11	9.840	1139	1148	1157	rBV	527006	886943	19.32%	2.200%
12	10.369	1231	1238	1253	rBV	679022	1297123	28.25%	3.217%
13	10.746	1295	1302	1316	rBV	642048	1076773	23.45%	2.671%
14	10.922	1325	1332	1346	rBV	731834	1295940	28.22%	3.214%
15	11.099	1359	1362	1364	rBV4	3789	5156	0.11%	0.013%
16	12.351	1569	1575	1581	rBV4	9682	21781	0.47%	0.054%
17	13.263	1726	1730	1734	rBV6	2475	4754	0.10%	0.012%
18	13.451	1758	1762	1770	rVB8	12575	21971	0.48%	0.054%
19	13.816	1819	1824	1830	rVB9	3788	7231	0.16%	0.018%
20	14.028	1852	1860	1876	rBV	1410479	1955814	42.60%	4.851%
21	14.310	1901	1908	1924	rBV2	1509356	2221238	48.38%	5.509%
22	14.451	1930	1932	1938	rVB6	3234	5000	0.11%	0.012%
23	14.616	1951	1960	1969	rBV	935281	1411354	30.74%	3.500%
24	14.863	1996	2002	2027	rBV	334297	895214	19.50%	2.220%
25	15.404	2091	2094	2098	rBV5	5297	7638	0.17%	0.019%
26	15.616	2124	2130	2142	rBV	1984633	2925407	63.71%	7.256%
27	15.763	2149	2155	2169	rBV	521761	815801	17.77%	2.023%
28	15.863	2169	2172	2179	rVV6	14653	28302	0.62%	0.070%
29	15.922	2179	2182	2188	rVB8	3889	7615	0.17%	0.019%
30	16.204	2227	2230	2234	rBV6	3984	4973	0.11%	0.012%
31	16.675	2307	2310	2314	rBV6	4246	6331	0.14%	0.016%
32	17.404	2428	2434	2445	rBV	1212542	1769843	38.55%	4.390%
33	17.510	2445	2452	2468	rVV	2187133	3243748	70.65%	8.045%
34	18.263	2576	2580	2585	rBV8	14472	21620	0.47%	0.054%
35	19.333	2758	2762	2767	rBV3	30985	40036	0.87%	0.099%
36	19.410	2771	2775	2778	rVB	26595	36283	0.79%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017697.D
Acq On : 17 Oct 2023 14:38
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK335

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	19.763	2829	2835	2845	rBV	2979536	4034974	87.88%	10.008%
38	21.551	3134	3139	3151	rBV	1538363	2172696	47.32%	5.389%
39	23.951	3540	3547	3562	rBV2	2213699	4591467	100.00%	11.388%
40	24.121	3570	3576	3590	rVB	1139750	2411737	52.53%	5.982%




Sum of corrected areas: 40319384

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017697.D
Acq On : 17 Oct 2023 14:38
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

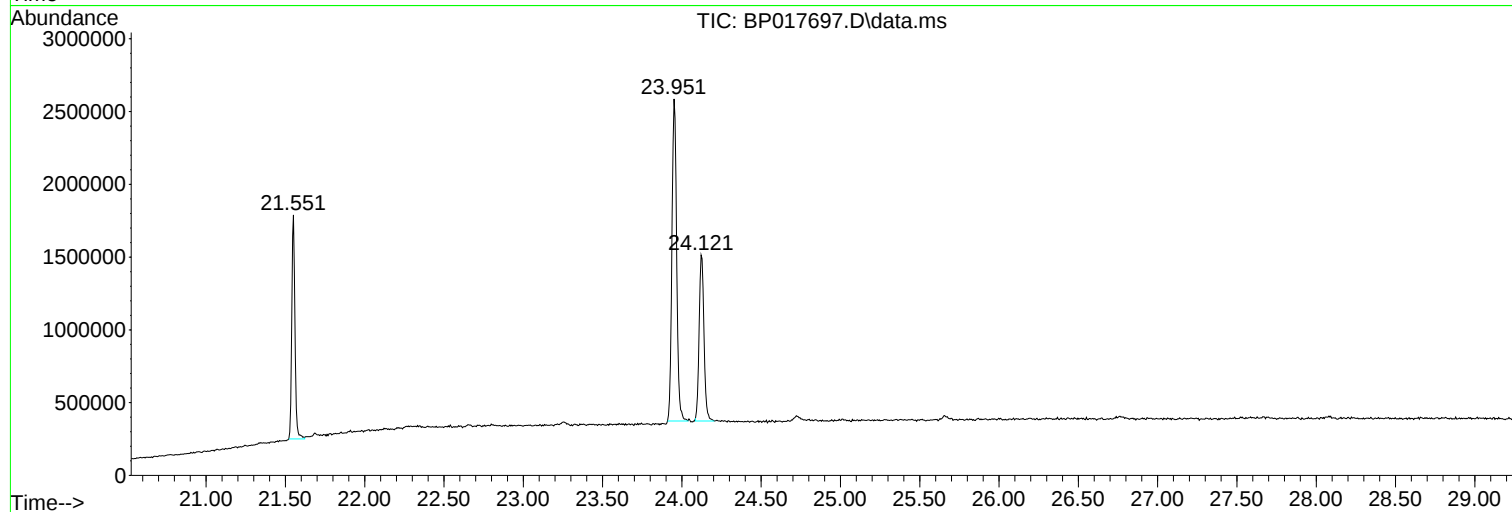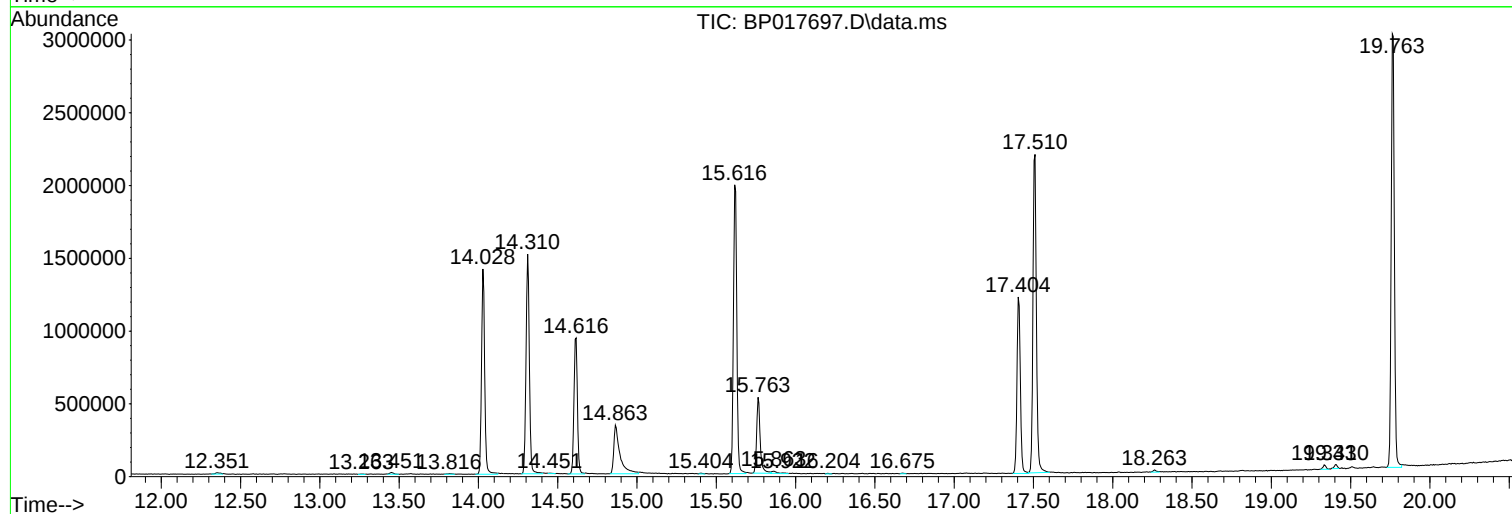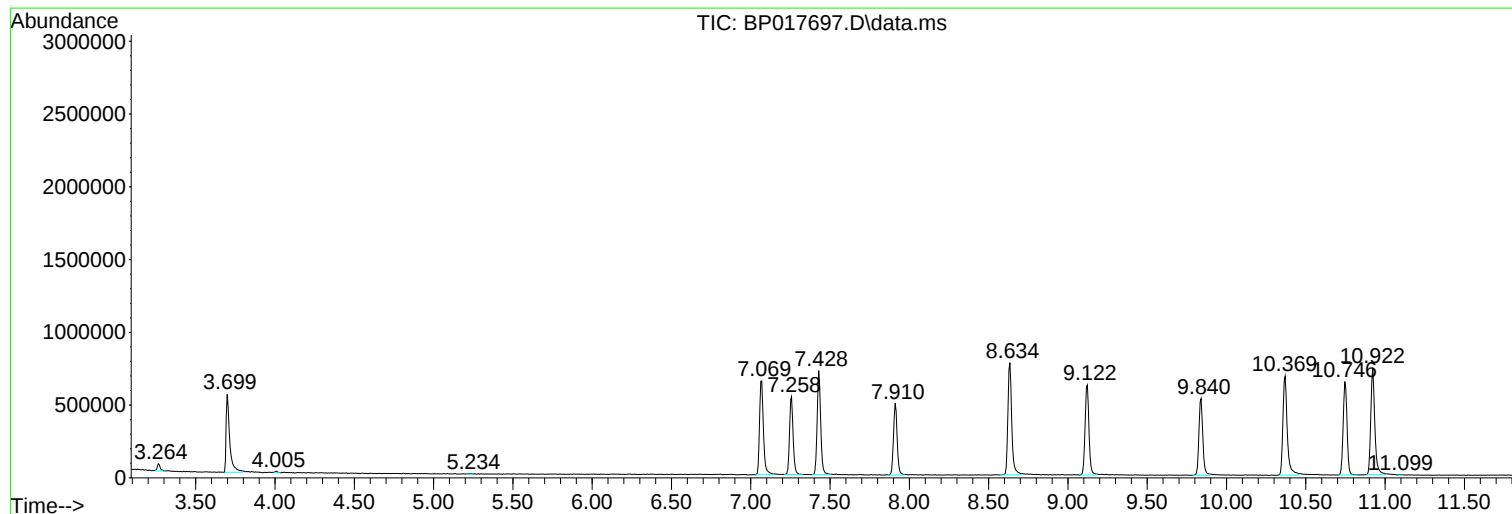

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017697.D
Acq On : 17 Oct 2023 14:38
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017697.D
Acq On : 17 Oct 2023 14:38
Operator : MA/JU
Sample : PB156335BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc