

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017698.D
 Acq On : 17 Oct 2023 15:12
 Operator : MA/JU
 Sample : 04889-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.587	253	255	259	rBV5	2814	4064	0.24%	0.056%
2	4.993	322	324	330	rVB7	2310	3014	0.18%	0.042%
3	5.552	417	419	427	rVB9	2562	4938	0.29%	0.068%
4	5.617	428	430	432	rVB3	2549	2180	0.13%	0.030%
5	5.664	436	438	440	rBV2	2174	1983	0.12%	0.027%
6	5.946	483	486	488	rBV4	2931	3648	0.22%	0.051%
7	6.058	502	505	506	rBV3	2623	2595	0.15%	0.036%
8	6.169	520	524	526	rBV5	1800	2428	0.14%	0.034%
9	6.228	531	534	535	rBV3	2142	2286	0.14%	0.032%
10	6.299	542	546	547	rBV4	2196	2467	0.15%	0.034%
11	6.669	607	609	612	rBV4	2551	3259	0.19%	0.045%
12	6.875	641	644	649	rVB7	3070	4057	0.24%	0.056%
13	7.558	755	760	761	rVV5	1687	2843	0.17%	0.039%
14	7.764	793	795	797	rBV3	1638	1831	0.11%	0.025%
15	7.852	806	810	812	rBV5	2584	4068	0.24%	0.056%
16	7.899	812	818	829	rVV	363085	608010	35.96%	8.431%
17	7.993	832	834	838	rVB5	3602	4564	0.27%	0.063%
18	8.463	913	914	919	rBV5	2511	3155	0.19%	0.044%
19	8.569	928	932	934	rBV5	2838	3888	0.23%	0.054%
20	8.599	934	937	938	rBV3	1955	2327	0.14%	0.032%
21	8.922	989	992	994	rVB4	2086	2050	0.12%	0.028%
22	8.946	994	996	999	rBV4	1794	2283	0.14%	0.032%
23	9.005	1005	1006	1009	rVB3	2702	2204	0.13%	0.031%
24	9.134	1026	1028	1031	rBV4	3313	3007	0.18%	0.042%
25	9.222	1041	1043	1047	rBV5	1327	1835	0.11%	0.025%
26	9.258	1047	1049	1052	rVV4	1866	1906	0.11%	0.026%
27	9.393	1069	1072	1075	rVB5	2380	3028	0.18%	0.042%
28	9.428	1075	1078	1081	rBV5	2125	3462	0.20%	0.048%
29	9.658	1115	1117	1119	rBV3	2101	2017	0.12%	0.028%
30	9.675	1119	1120	1125	rBV5	1209	1978	0.12%	0.027%
31	9.763	1131	1135	1137	rVV5	1722	1862	0.11%	0.026%
32	9.993	1171	1174	1176	rBV4	2663	2797	0.17%	0.039%
33	10.316	1227	1229	1232	rBV4	2350	2316	0.14%	0.032%
34	10.734	1293	1300	1316	rBV	424385	786049	46.49%	10.899%
35	10.887	1325	1326	1331	rVB5	2365	2894	0.17%	0.040%
36	10.928	1331	1333	1336	rVB4	1933	2206	0.13%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017698.D
 Acq On : 17 Oct 2023 15:12
 Operator : MA/JU
 Sample : 04889-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

37	10.957	1336	1338	1341	rBV4	2450	2405	0.14%	0.033%
38	11.175	1372	1375	1380	rVB7	2032	3519	0.21%	0.049%
39	11.340	1400	1403	1406	rVB5	1703	2344	0.14%	0.033%
40	11.404	1412	1414	1417	rVV3	2263	2683	0.16%	0.037%

41	11.452	1421	1422	1426	rVV4	2135	2013	0.12%	0.028%
42	11.581	1442	1444	1449	rBV6	2166	2675	0.16%	0.037%
43	11.916	1497	1501	1502	rVB4	2194	2439	0.14%	0.034%
44	12.134	1534	1538	1540	rVB5	2104	2278	0.13%	0.032%
45	12.163	1540	1543	1546	rBV5	1964	2768	0.16%	0.038%

46	12.310	1563	1568	1571	rBV7	1568	2322	0.14%	0.032%
47	12.357	1573	1576	1579	rBV5	1906	2278	0.13%	0.032%
48	12.546	1605	1608	1611	rVB5	2193	2354	0.14%	0.033%
49	12.634	1617	1623	1624	rBV6	1619	2634	0.16%	0.037%
50	12.828	1654	1656	1659	rVB4	2455	2261	0.13%	0.031%

51	13.110	1700	1704	1706	rBV5	1928	2401	0.14%	0.033%
52	13.281	1728	1733	1736	rVB7	2639	3501	0.21%	0.049%
53	13.528	1772	1775	1776	rVB3	1968	1900	0.11%	0.026%
54	13.634	1790	1793	1796	rVB5	1404	1836	0.11%	0.025%
55	13.663	1796	1798	1800	rBV3	1603	1881	0.11%	0.026%

56	13.857	1829	1831	1833	rBV2	2447	1941	0.11%	0.027%
57	14.128	1871	1877	1878	rVB6	1402	2289	0.14%	0.032%
58	14.228	1890	1894	1897	rVB6	2091	2537	0.15%	0.035%
59	14.298	1903	1906	1908	rBV4	1471	2075	0.12%	0.029%
60	14.398	1922	1923	1929	rVB6	1659	1887	0.11%	0.026%

61	14.463	1929	1934	1937	rBV6	2161	3825	0.23%	0.053%
62	14.604	1949	1958	1972	rBV	613223	989786	58.53%	13.724%
63	14.793	1988	1990	1994	rVB5	2781	2408	0.14%	0.033%
64	14.893	2004	2007	2009	rVB4	2403	2809	0.17%	0.039%
65	14.928	2009	2013	2016	rBV6	2181	3599	0.21%	0.050%

66	15.081	2037	2039	2042	rVB4	2722	3055	0.18%	0.042%
67	15.110	2042	2044	2045	rBV2	2604	2241	0.13%	0.031%
68	15.169	2051	2054	2056	rVB4	2097	2018	0.12%	0.028%
69	15.322	2077	2080	2083	rBV5	2052	2009	0.12%	0.028%
70	15.393	2090	2092	2097	rVV6	2256	2909	0.17%	0.040%

71	15.451	2099	2102	2104	rBV4	1608	2102	0.12%	0.029%
72	15.634	2129	2133	2134	rBV4	1815	1965	0.12%	0.027%
73	15.698	2141	2144	2147	rBV4	1711	2207	0.13%	0.031%
74	15.751	2151	2153	2156	rVB4	2114	2385	0.14%	0.033%
75	15.792	2156	2160	2163	rBV6	1651	2935	0.17%	0.041%

76	15.869	2170	2173	2175	rBV4	2288	2410	0.14%	0.033%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017698.D
 Acq On : 17 Oct 2023 15:12
 Operator : MA/JU
 Sample : 04889-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

77	15.998	2193	2195	2202	rVB8	2533	4108	0.24%	0.057%
78	16.469	2272	2275	2278	rVB5	3181	3967	0.23%	0.055%
79	16.504	2278	2281	2282	rBV3	2767	2989	0.18%	0.041%
80	16.822	2331	2335	2337	rBV5	2033	3542	0.21%	0.049%
81	16.957	2356	2358	2361	rVV4	1727	1860	0.11%	0.026%
82	17.128	2384	2387	2390	rBV5	2688	3505	0.21%	0.049%
83	17.316	2417	2419	2424	rVB6	1440	2105	0.12%	0.029%
84	17.398	2427	2433	2448	rBV	750155	1267800	74.98%	17.579%
85	17.604	2466	2468	2471	rVB4	2173	2462	0.15%	0.034%
86	17.634	2471	2473	2475	rBV3	1896	1999	0.12%	0.028%
87	17.681	2475	2481	2482	rBV6	3334	3565	0.21%	0.049%
88	17.745	2489	2492	2494	rBV4	2406	2604	0.15%	0.036%
89	17.798	2499	2501	2504	rBV4	2243	3063	0.18%	0.042%
90	17.945	2522	2526	2527	rBV4	1967	2328	0.14%	0.032%
91	17.969	2527	2530	2531	rBV3	2203	2811	0.17%	0.039%
92	18.057	2543	2545	2547	rBV3	2448	2199	0.13%	0.030%
93	18.098	2550	2552	2555	rBV4	2346	2711	0.16%	0.038%
94	18.339	2592	2593	2596	rBV3	2876	3508	0.21%	0.049%
95	18.492	2616	2619	2622	rBV5	3606	4525	0.27%	0.063%
96	18.522	2622	2624	2626	rBV3	3533	2550	0.15%	0.035%
97	18.645	2643	2645	2646	rBV2	3305	2347	0.14%	0.033%
98	19.633	2811	2813	2815	rBV2	6944	5303	0.31%	0.074%
99	21.539	3132	3137	3151	rBV	1128333	1613749	95.44%	22.376%
100	24.110	3567	3574	3591	rVB	754565	1690937	100.00%	23.446%




Sum of corrected areas: 7211920

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP017698\
Data File : BP017698.D
Acq On : 17 Oct 2023 15:12
Operator : MA/JU
Sample : 04889-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

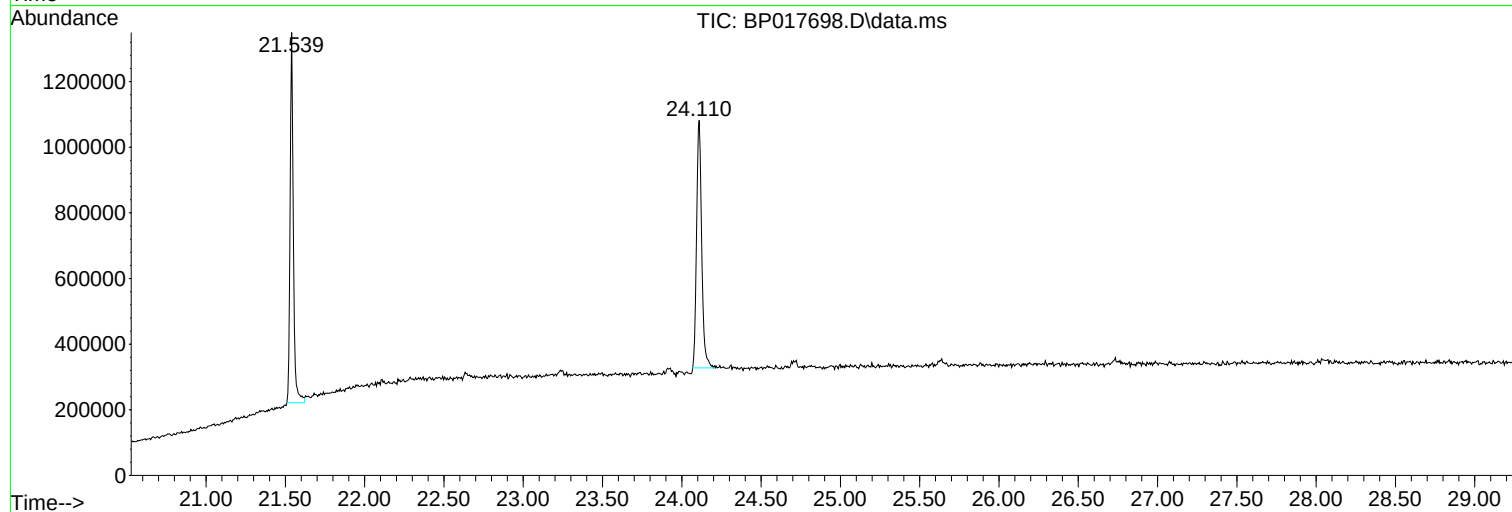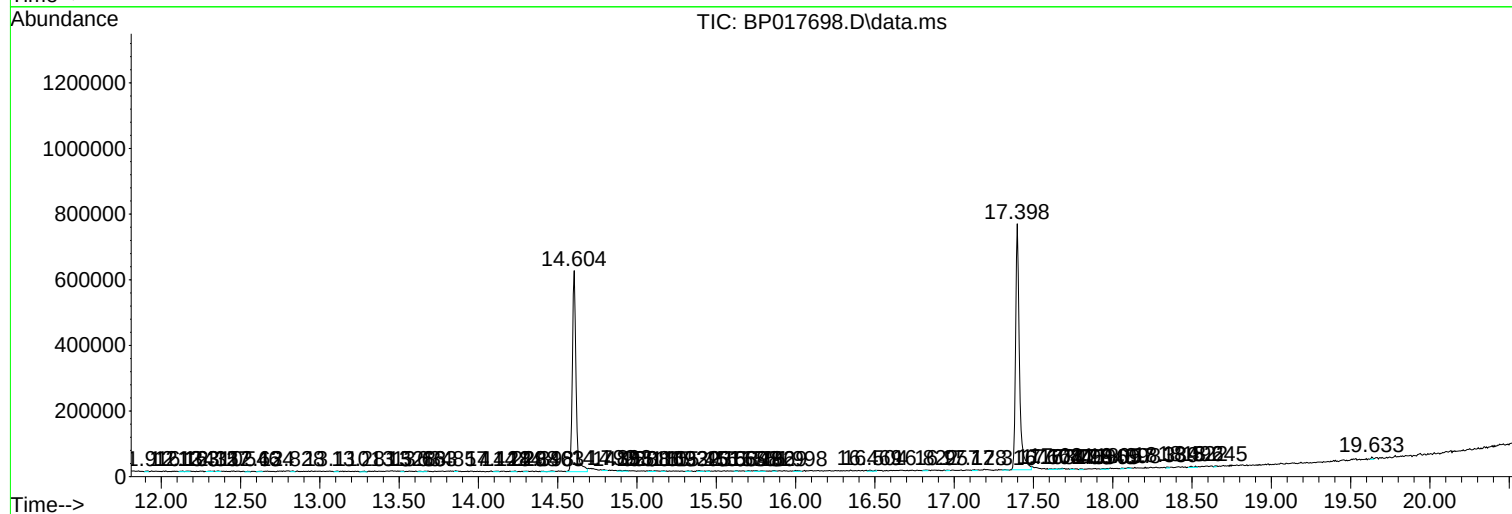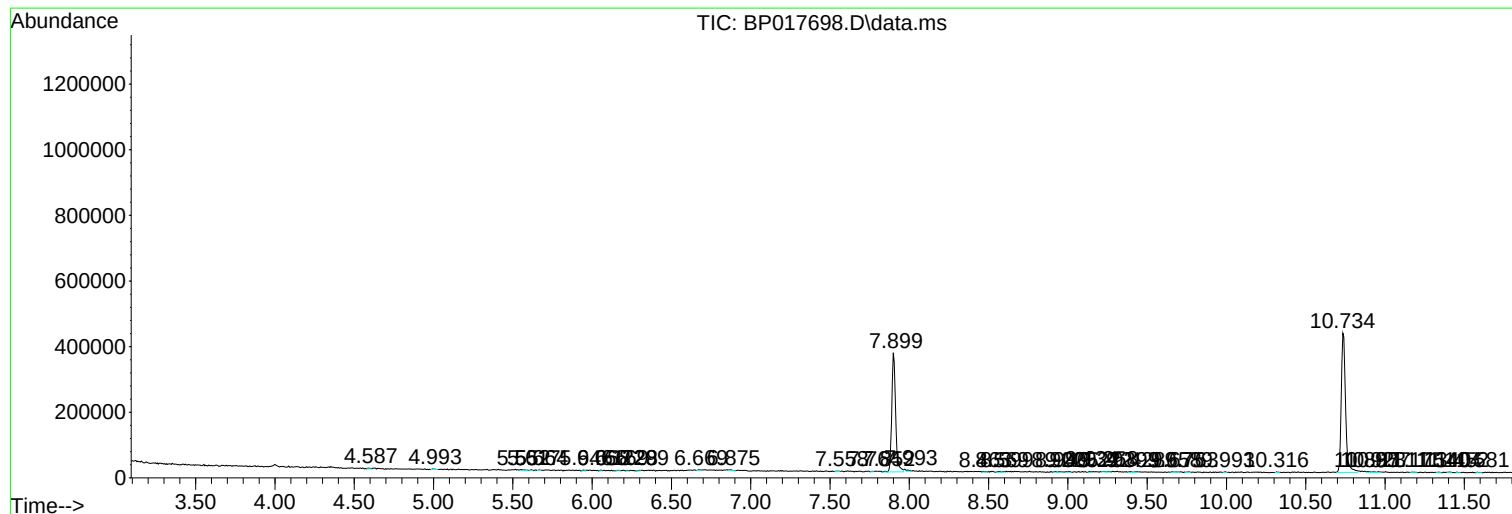

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017698.D
Acq On : 17 Oct 2023 15:12
Operator : MA/JU
Sample : 04889-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017698.D
Acq On : 17 Oct 2023 15:12
Operator : MA/JU
Sample : 04889-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc