

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017700.D
 Acq On : 17 Oct 2023 16:21
 Operator : MA/JU
 Sample : 04889-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.999	153	155	160	rBV6	5548	7490	0.45%	0.103%
2	4.187	186	187	192	rBV4	4976	4947	0.29%	0.068%
3	4.358	214	216	217	rVB2	3720	2049	0.12%	0.028%
4	4.464	233	234	236	rBV2	3768	3306	0.20%	0.045%
5	4.593	254	256	259	rBV4	2553	3477	0.21%	0.048%
6	4.658	266	267	268	rBV	3929	2635	0.16%	0.036%
7	5.305	375	377	378	rBV2	3042	2673	0.16%	0.037%
8	5.564	420	421	423	rBV2	3626	1991	0.12%	0.027%
9	5.664	436	438	441	rBV4	2495	2867	0.17%	0.039%
10	5.899	476	478	482	rBV5	2246	2762	0.16%	0.038%
11	5.934	482	484	488	rVB5	2213	2256	0.13%	0.031%
12	6.146	518	520	525	rVB6	2563	4638	0.28%	0.064%
13	6.846	638	639	643	rBV4	2497	2424	0.14%	0.033%
14	7.134	685	688	689	rBV3	2121	2006	0.12%	0.027%
15	7.210	697	701	702	rBV4	2729	1955	0.12%	0.027%
16	7.563	757	761	763	rBV5	1809	2484	0.15%	0.034%
17	7.599	765	767	768	rBV2	2565	2277	0.14%	0.031%
18	7.687	779	782	784	rBV3	2467	2724	0.16%	0.037%
19	7.728	787	789	793	rVB5	2294	2853	0.17%	0.039%
20	7.769	793	796	797	rBV3	1849	2165	0.13%	0.030%
21	7.899	811	818	835	rBV	351208	598364	35.57%	8.195%
22	8.287	881	884	888	rBV5	2318	2783	0.17%	0.038%
23	8.469	913	915	918	rBV4	1857	2399	0.14%	0.033%
24	8.581	932	934	937	rVB4	2730	2604	0.15%	0.036%
25	8.616	937	940	943	rVB5	1718	2257	0.13%	0.031%
26	8.728	958	959	962	rBV3	2152	2649	0.16%	0.036%
27	8.799	968	971	972	rBV3	2005	2048	0.12%	0.028%
28	8.934	992	994	997	rVB4	1802	1967	0.12%	0.027%
29	9.099	1019	1022	1023	rBV2	1886	2257	0.13%	0.031%
30	9.128	1026	1027	1034	rVV7	2390	4103	0.24%	0.056%
31	9.199	1037	1039	1042	rVB4	2492	2282	0.14%	0.031%
32	9.234	1042	1045	1046	rBV3	2825	2627	0.16%	0.036%
33	9.652	1114	1116	1121	rVB6	1395	2108	0.13%	0.029%
34	9.787	1136	1139	1143	rBV6	1494	1998	0.12%	0.027%
35	9.999	1170	1175	1177	rBV6	2010	2479	0.15%	0.034%
36	10.110	1193	1194	1197	rBV3	2517	2183	0.13%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017700.D
 Acq On : 17 Oct 2023 16:21
 Operator : MA/JU
 Sample : 04889-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

37	10.469	1252	1255	1258	rBV5	2230	2292	0.14%	0.031%
38	10.516	1261	1263	1264	rBV2	2342	2227	0.13%	0.031%
39	10.587	1274	1275	1278	rVB3	2882	2528	0.15%	0.035%
40	10.734	1292	1300	1314	rBV	415784	775000	46.07%	10.614%

41	11.081	1356	1359	1363	rBV6	1334	2153	0.13%	0.029%
42	11.169	1370	1374	1375	rVB4	2418	2745	0.16%	0.038%
43	11.210	1375	1381	1385	rVB9	2688	4430	0.26%	0.061%
44	11.251	1385	1388	1390	rBV4	2852	2548	0.15%	0.035%
45	11.334	1400	1402	1404	rVB3	2884	2264	0.13%	0.031%

46	11.540	1435	1437	1440	rVB4	2677	2315	0.14%	0.032%
47	11.575	1440	1443	1445	rBV4	1941	2555	0.15%	0.035%
48	11.669	1457	1459	1461	rVB3	2228	1943	0.12%	0.027%
49	11.775	1474	1477	1479	rBV4	2102	2414	0.14%	0.033%
50	12.016	1514	1518	1521	rVB6	1758	2236	0.13%	0.031%

51	12.069	1526	1527	1532	rVV5	2113	2422	0.14%	0.033%
52	12.204	1548	1550	1555	rVB6	1838	2909	0.17%	0.040%
53	12.240	1555	1556	1560	rBV4	1571	2006	0.12%	0.027%
54	12.416	1582	1586	1587	rBV4	3170	4451	0.26%	0.061%
55	12.581	1610	1614	1615	rBV4	1863	2102	0.12%	0.029%

56	12.869	1660	1663	1664	rBV3	2267	2264	0.13%	0.031%
57	12.963	1677	1679	1682	rVB4	1628	2013	0.12%	0.028%
58	13.122	1703	1706	1707	rBV3	1812	1981	0.12%	0.027%
59	13.445	1757	1761	1763	rBV5	4457	6692	0.40%	0.092%
60	13.487	1766	1768	1773	rVB6	3011	4490	0.27%	0.061%

61	13.728	1807	1809	1813	rVB5	2555	2731	0.16%	0.037%
62	13.898	1835	1838	1842	rBV6	1552	1949	0.12%	0.027%
63	14.204	1884	1890	1892	rBV7	1441	2762	0.16%	0.038%
64	14.257	1897	1899	1903	rVB4	1952	2432	0.14%	0.033%
65	14.504	1939	1941	1944	rBV4	3026	4260	0.25%	0.058%

66	14.604	1951	1958	1971	rBV	584656	987434	58.70%	13.524%
67	14.898	2007	2008	2011	rBV3	1900	2069	0.12%	0.028%
68	14.928	2011	2013	2018	rVB6	2994	4109	0.24%	0.056%
69	14.992	2020	2024	2026	rVB5	2536	3316	0.20%	0.045%
70	15.187	2054	2057	2059	rBV4	2002	2249	0.13%	0.031%

71	15.398	2085	2093	2098	rBV4	3660	7445	0.44%	0.102%
72	15.434	2098	2099	2102	rVB3	2119	1935	0.12%	0.027%
73	15.469	2102	2105	2107	rBV4	2004	2124	0.13%	0.029%
74	15.534	2112	2116	2117	rBV4	1970	2366	0.14%	0.032%
75	15.557	2117	2120	2122	rVB4	2618	2735	0.16%	0.037%

76	15.581	2122	2124	2127	rBV4	2953	3171	0.19%	0.043%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017700.D
 Acq On : 17 Oct 2023 16:21
 Operator : MA/JU
 Sample : 04889-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

77	15.628	2129	2132	2134	rBV4	1889	2620	0.16%	0.036%
78	15.939	2183	2185	2191	rVB6	1456	2093	0.12%	0.029%
79	16.363	2254	2257	2262	rVB7	1470	2223	0.13%	0.030%
80	16.651	2304	2306	2310	rVB5	2467	2822	0.17%	0.039%
81	16.686	2310	2312	2314	rBV3	1881	1993	0.12%	0.027%
82	16.922	2349	2352	2356	rBV6	3399	4750	0.28%	0.065%
83	17.016	2367	2368	2370	rBV2	3174	1967	0.12%	0.027%
84	17.104	2380	2383	2384	rBV3	2957	2228	0.13%	0.031%
85	17.181	2394	2396	2398	rBV3	2814	3132	0.19%	0.043%
86	17.286	2411	2414	2416	rBV4	2267	2480	0.15%	0.034%
87	17.398	2426	2433	2451	rBV	756735	1326120	78.83%	18.162%
88	17.681	2479	2481	2484	rBV4	3177	3331	0.20%	0.046%
89	17.733	2488	2490	2492	rBV3	2439	2086	0.12%	0.029%
90	17.986	2530	2533	2534	rBV2	3311	3847	0.23%	0.053%
91	18.033	2539	2541	2543	rVV3	2201	1929	0.11%	0.026%
92	18.075	2546	2548	2549	rBV2	2358	1955	0.12%	0.027%
93	18.128	2555	2557	2559	rBV3	2609	2672	0.16%	0.037%
94	18.245	2575	2577	2578	rVV2	3423	2398	0.14%	0.033%
95	18.263	2578	2580	2583	rVB3	4973	4946	0.29%	0.068%
96	18.433	2608	2609	2612	rVB3	4132	3243	0.19%	0.044%
97	18.663	2646	2648	2651	rBV4	3804	4777	0.28%	0.065%
98	18.880	2683	2685	2687	rVB3	3432	2168	0.13%	0.030%
99	21.539	3132	3137	3145	rBV	1186219	1666299	99.05%	22.821%
100	24.104	3567	3573	3586	rBV	762649	1682310	100.00%	23.040%




Sum of corrected areas: 7301543

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017700.D
Acq On : 17 Oct 2023 16:21
Operator : MA/JU
Sample : 04889-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

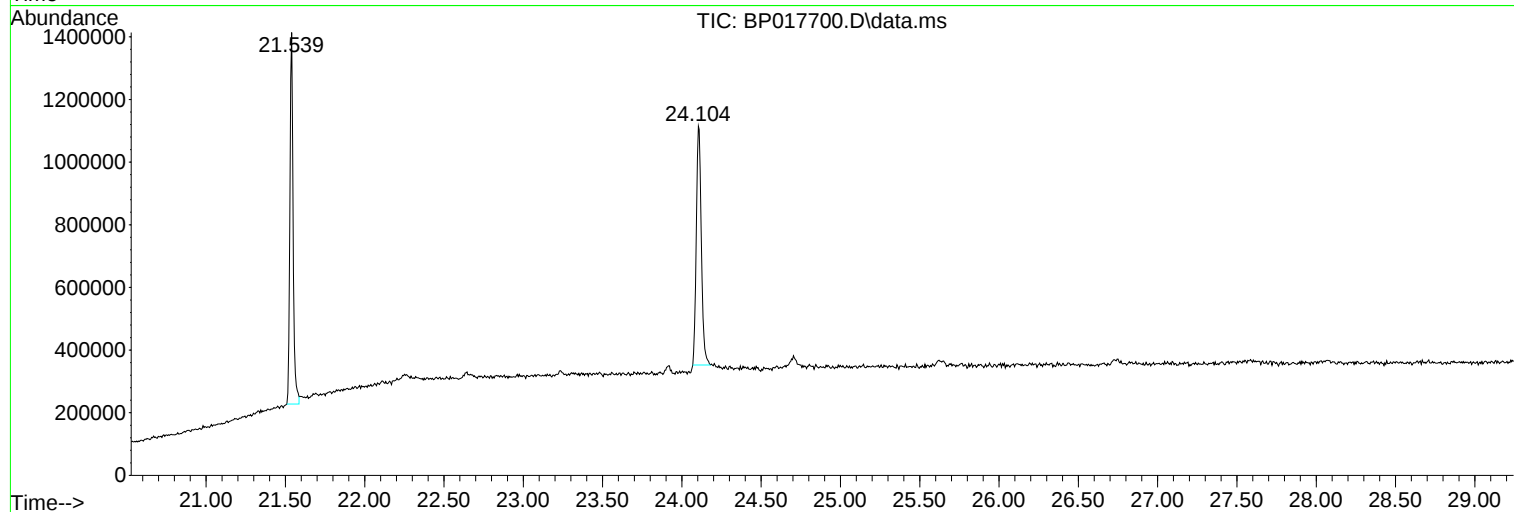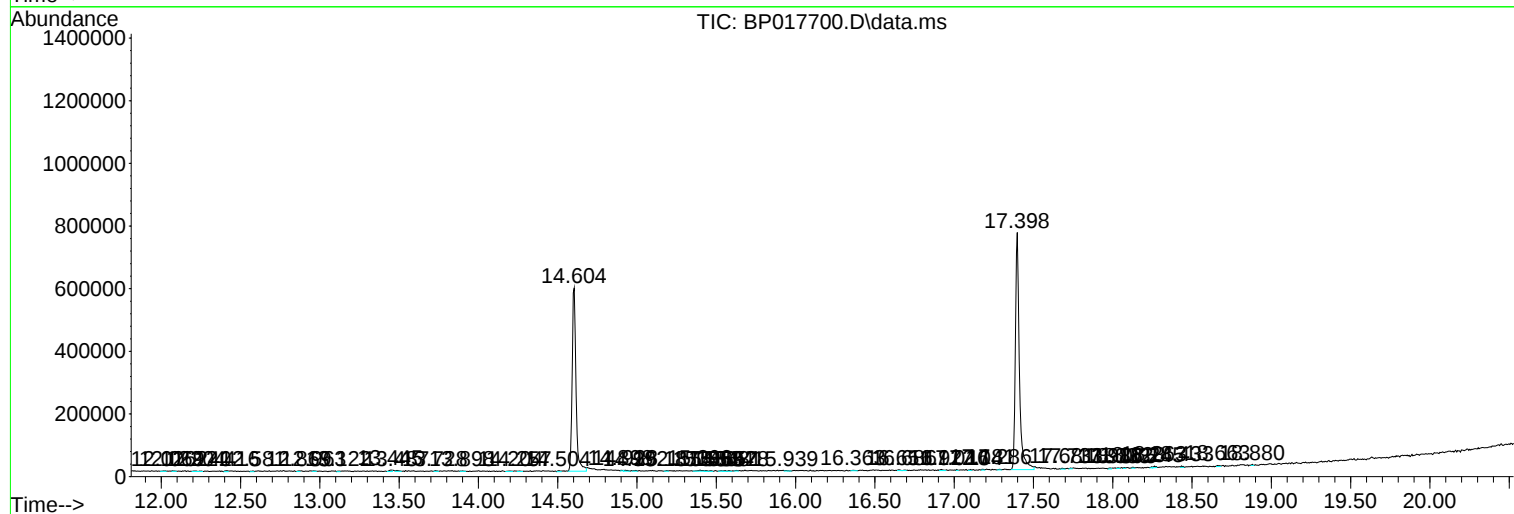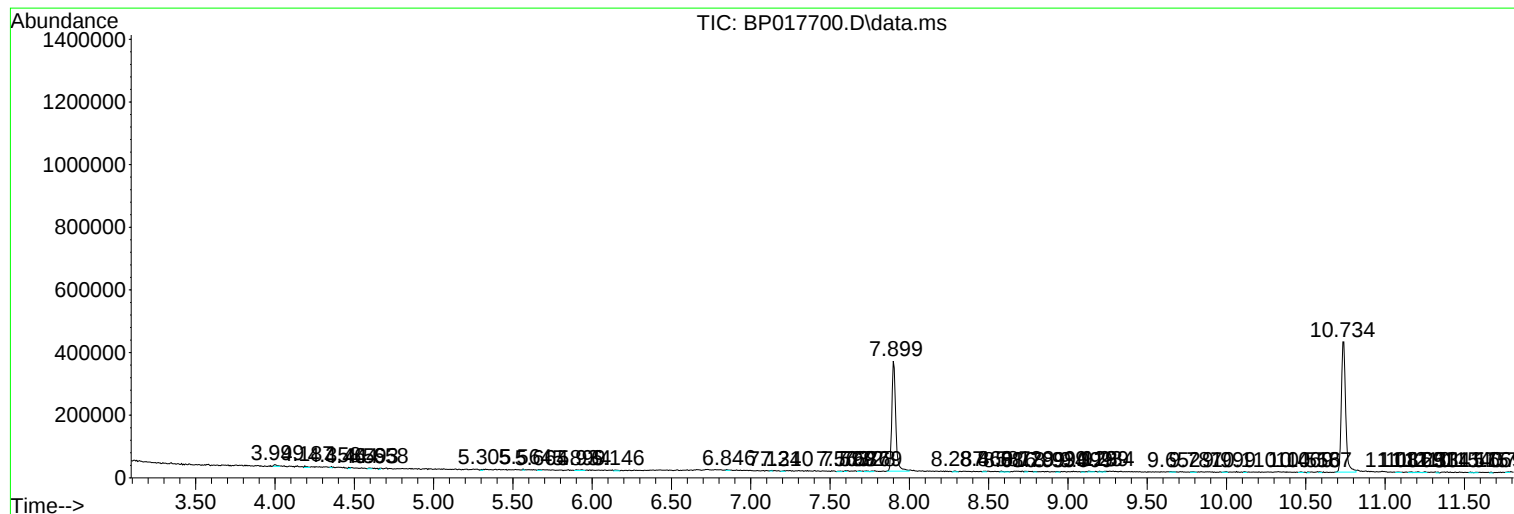

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017700.D
Acq On : 17 Oct 2023 16:21
Operator : MA/JU
Sample : 04889-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017700.D
Acq On : 17 Oct 2023 16:21
Operator : MA/JU
Sample : 04889-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc