

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017705.D
 Acq On : 17 Oct 2023 19:15
 Operator : MA/JU
 Sample : PB156344TB 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	36	rVB	47396	65457	1.37%	0.167%
2	3.693	99	103	116	rBV	538698	827882	17.35%	2.112%
3	7.058	668	675	689	rBV	654250	1105076	23.15%	2.819%
4	7.246	701	707	720	rVB	550724	881617	18.47%	2.249%
5	7.417	730	736	758	rVB	702413	1161030	24.33%	2.962%
6	7.899	811	818	833	rBV	343835	566725	11.87%	1.446%
7	8.264	874	880	881	rBV6	2616	4800	0.10%	0.012%
8	8.622	934	941	957	rBV	756872	1347047	28.22%	3.436%
9	9.111	1014	1024	1038	rBV	640982	1093890	22.92%	2.790%
10	9.346	1060	1064	1068	rBV7	2311	4810	0.10%	0.012%
11	9.822	1139	1145	1156	rBV	527662	906539	18.99%	2.312%
12	10.358	1229	1236	1258	rBV	684646	1370271	28.71%	3.495%
13	10.734	1292	1300	1308	rBV	473462	784542	16.44%	2.001%
14	10.910	1321	1330	1346	rBV	740076	1365125	28.60%	3.482%
15	11.893	1494	1497	1504	rBV8	3080	4859	0.10%	0.012%
16	12.346	1570	1574	1580	rBV7	10228	21295	0.45%	0.054%
17	13.104	1700	1703	1708	rVB7	3930	5957	0.12%	0.015%
18	13.434	1754	1759	1767	rBV9	8396	18622	0.39%	0.048%
19	14.016	1851	1858	1871	rBV	1542280	2076164	43.50%	5.296%
20	14.299	1899	1906	1922	rBV	1644083	2373624	49.74%	6.055%
21	14.598	1950	1957	1966	rBV	695633	1046432	21.93%	2.669%
22	14.851	1993	2000	2020	rBV2	324978	908096	19.03%	2.316%
23	15.075	2036	2038	2048	rVV2	5469	9218	0.19%	0.024%
24	15.246	2063	2067	2071	rVB7	3821	6503	0.14%	0.017%
25	15.604	2121	2128	2143	rBV	2187153	3130365	65.59%	7.985%
26	15.751	2147	2153	2166	rVV	536626	806124	16.89%	2.056%
27	15.845	2166	2169	2176	rVB7	14193	25968	0.54%	0.066%
28	17.392	2425	2432	2441	rBV	955517	1307403	27.39%	3.335%
29	17.492	2443	2449	2464	rVV	2440975	3487156	73.07%	8.895%
30	17.822	2502	2505	2508	rBV5	4468	6374	0.13%	0.016%
31	18.251	2574	2578	2580	rBV4	6238	7532	0.16%	0.019%
32	19.322	2753	2760	2765	rBV6	32745	55426	1.16%	0.141%
33	19.392	2768	2772	2776	rVV	30137	40488	0.85%	0.103%
34	19.751	2827	2833	2845	rBV	3394258	4357786	91.31%	11.116%
35	21.533	3132	3136	3148	rBV2	1092333	1533037	32.12%	3.911%
36	23.927	3536	3543	3558	rVB2	2294583	4772538	100.00%	12.174%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017705.D
Acq On : 17 Oct 2023 19:15
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	24.104	3566	3573	3587	rVB	768117	1717125	35.98%	4.380%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 39202903

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017705.D
Acq On : 17 Oct 2023 19:15
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

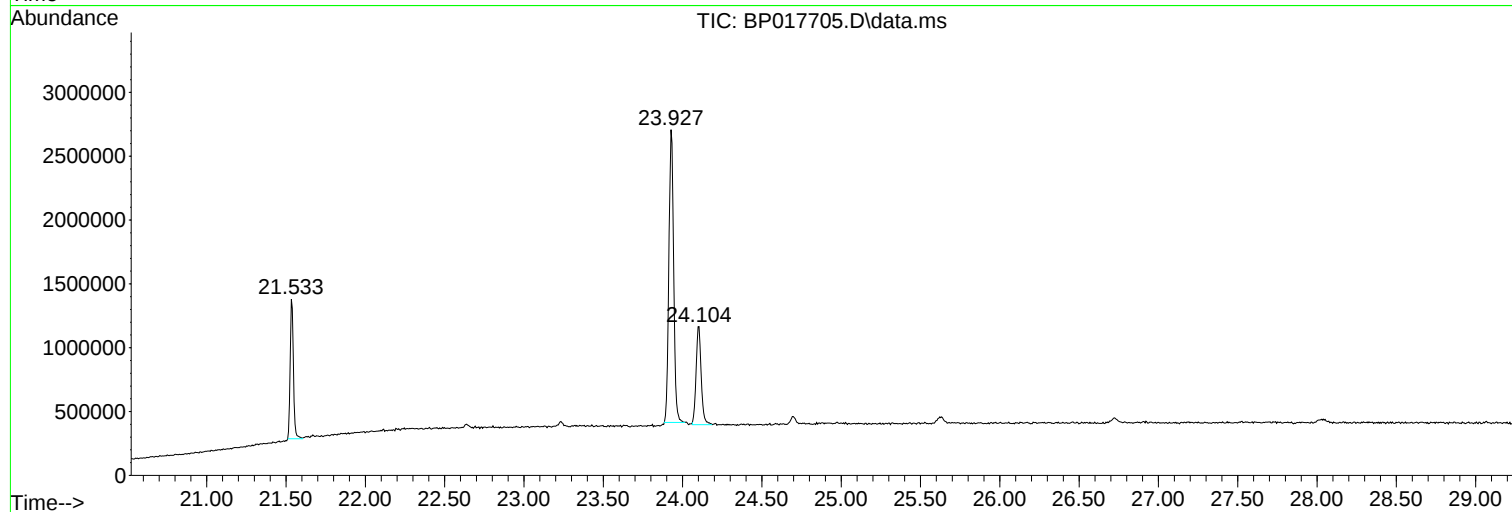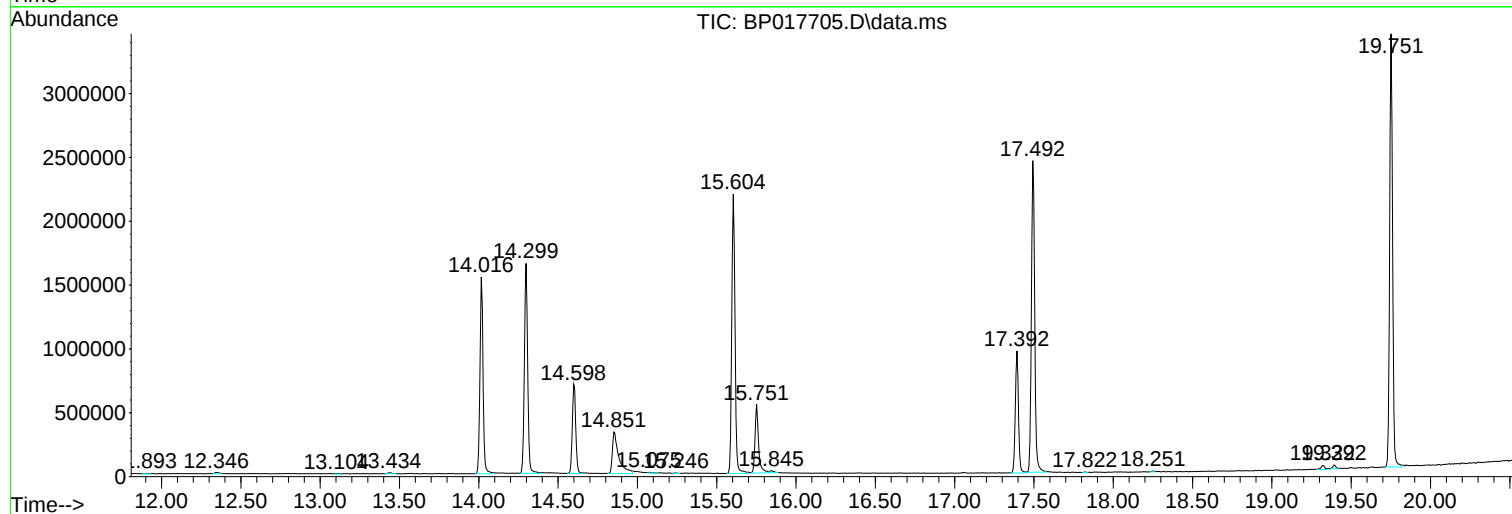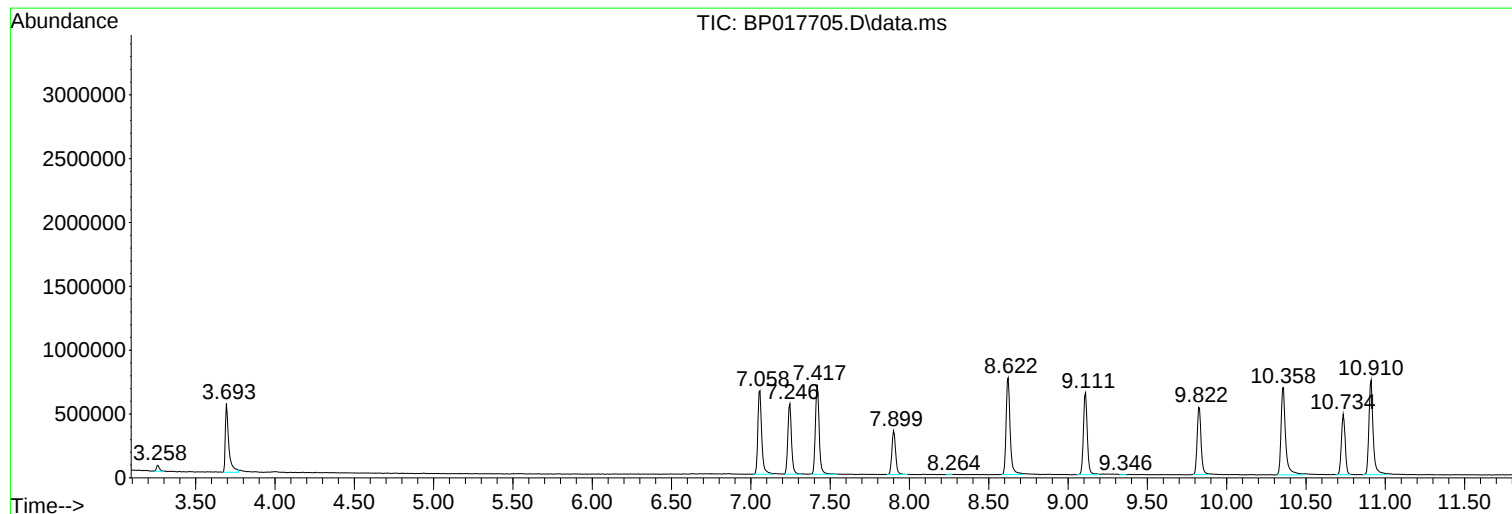

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017705.D
Acq On : 17 Oct 2023 19:15
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017705.D
Acq On : 17 Oct 2023 19:15
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc