

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
 Data File : BP017712.D
 Acq On : 17 Oct 2023 23:14
 Operator : MA/JU
 Sample : PB156379BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK379

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	34	rVB	53476	63269	1.15%	0.138%
2	3.693	99	103	127	rBV	642445	981841	17.80%	2.139%
3	3.993	152	154	157	rBV3	6873	7926	0.14%	0.017%
4	7.058	669	675	688	rBV	787646	1302357	23.62%	2.837%
5	7.240	699	706	717	rBV	637249	993579	18.02%	2.164%
6	7.416	729	736	747	rBV	850594	1315630	23.86%	2.866%
7	7.899	811	818	829	rVB	449267	704869	12.78%	1.536%
8	8.622	933	941	955	rBV	927767	1590990	28.85%	3.466%
9	9.104	1014	1023	1039	rVV	769784	1249773	22.66%	2.723%
10	9.822	1137	1145	1155	rBV	651006	1061602	19.25%	2.313%
11	9.934	1163	1164	1170	rVB6	4031	5694	0.10%	0.012%
12	10.351	1228	1235	1253	rBV	896733	1646302	29.85%	3.586%
13	10.734	1293	1300	1307	rBV	604200	989790	17.95%	2.156%
14	10.904	1321	1329	1344	rBV	920671	1637730	29.70%	3.568%
15	12.334	1567	1572	1577	rBV4	12063	22984	0.42%	0.050%
16	13.434	1754	1759	1764	rBV9	9842	16886	0.31%	0.037%
17	13.551	1776	1779	1782	rBV5	3422	5587	0.10%	0.012%
18	14.016	1851	1858	1871	rBV	1748608	2358989	42.78%	5.139%
19	14.298	1899	1906	1920	rBV	1853967	2723027	49.38%	5.932%
20	14.598	1948	1957	1968	rBV	913533	1311744	23.79%	2.858%
21	14.851	1993	2000	2023	rBV	483478	1170091	21.22%	2.549%
22	15.604	2117	2128	2141	rBV	2492869	3556554	64.49%	7.748%
23	15.751	2147	2153	2165	rBV	632124	956203	17.34%	2.083%
24	15.845	2165	2169	2178	rVB7	16666	33481	0.61%	0.073%
25	15.998	2193	2195	2201	rVB7	3939	5531	0.10%	0.012%
26	16.398	2260	2263	2267	rBV6	4525	7248	0.13%	0.016%
27	17.063	2372	2376	2381	rVB8	4774	7784	0.14%	0.017%
28	17.392	2425	2432	2442	rBV	1150202	1646440	29.86%	3.587%
29	17.492	2442	2449	2463	rBV	2811303	3920354	71.09%	8.540%
30	18.245	2572	2577	2583	rBV10	14163	28802	0.52%	0.063%
31	19.322	2756	2760	2765	rBV5	32840	47012	0.85%	0.102%
32	19.392	2769	2772	2778	rVB3	34630	46772	0.85%	0.102%
33	19.751	2827	2833	2841	rBV	3838668	4847220	87.90%	10.560%
34	21.533	3131	3136	3142	rBV	1505938	2007124	36.40%	4.372%
35	23.927	3536	3543	3559	rVB2	2672403	5514730	100.00%	12.014%
36	24.098	3566	3572	3583	rVB	983738	2117760	38.40%	4.613%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017712.D
Acq On : 17 Oct 2023 23:14
Operator : MA/JU
Sample : PB156379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 45903675

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017712.D
Acq On : 17 Oct 2023 23:14
Operator : MA/JU
Sample : PB156379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

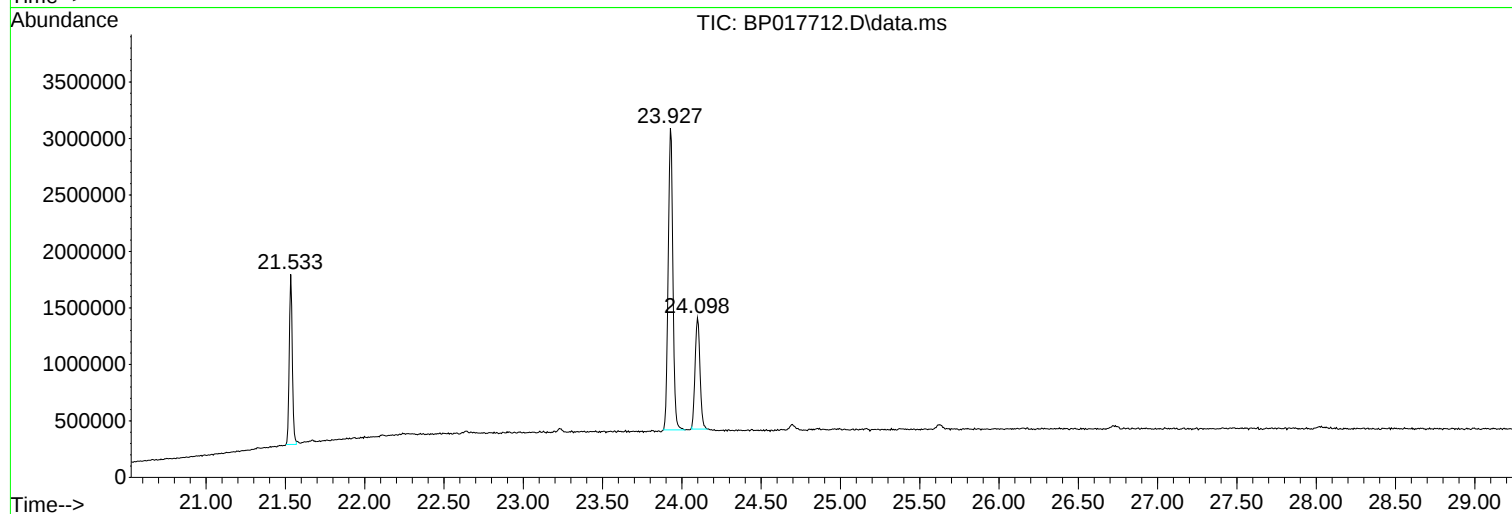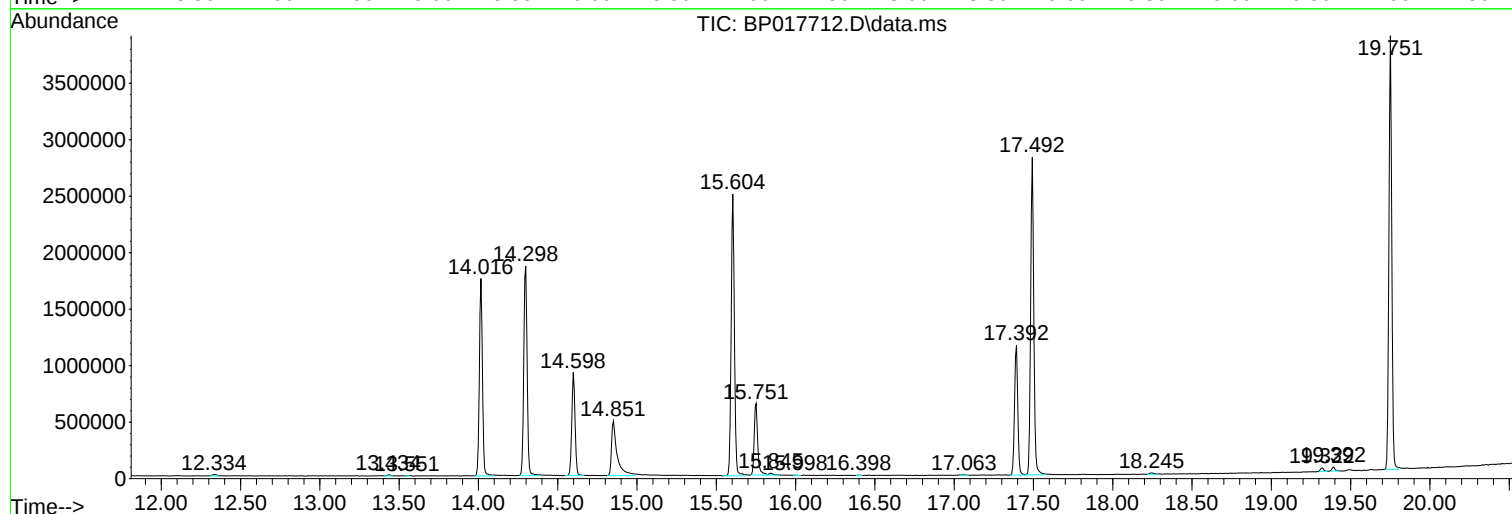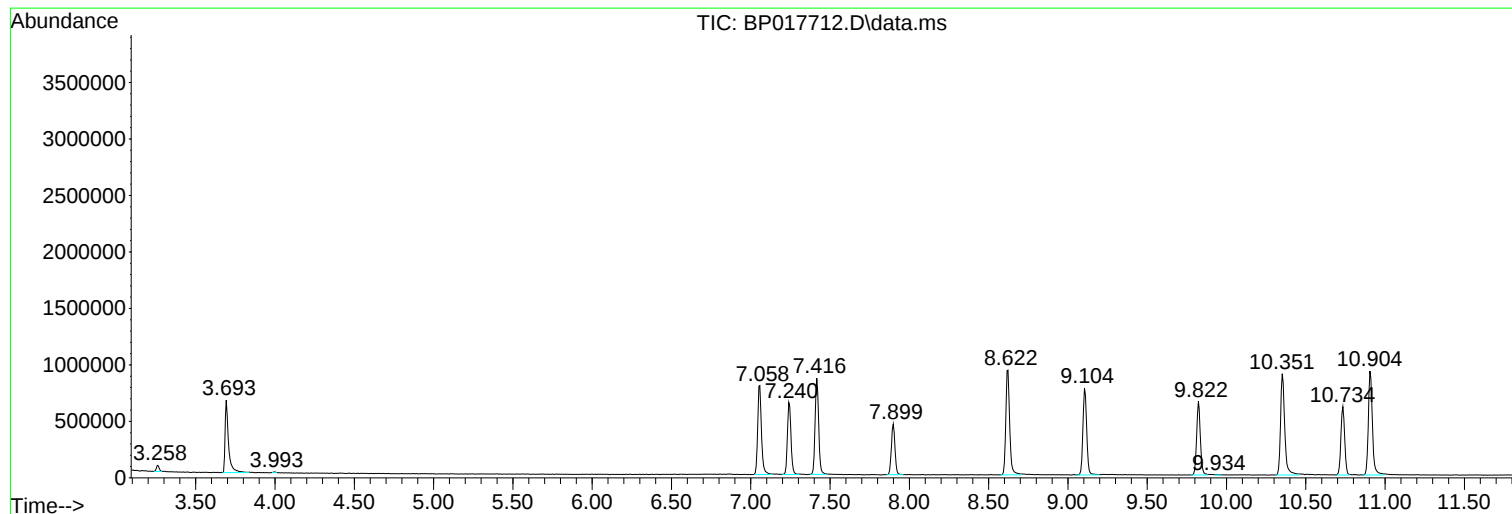

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017712.D
Acq On : 17 Oct 2023 23:14
Operator : MA/JU
Sample : PB156379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101723\
Data File : BP017712.D
Acq On : 17 Oct 2023 23:14
Operator : MA/JU
Sample : PB156379BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------