
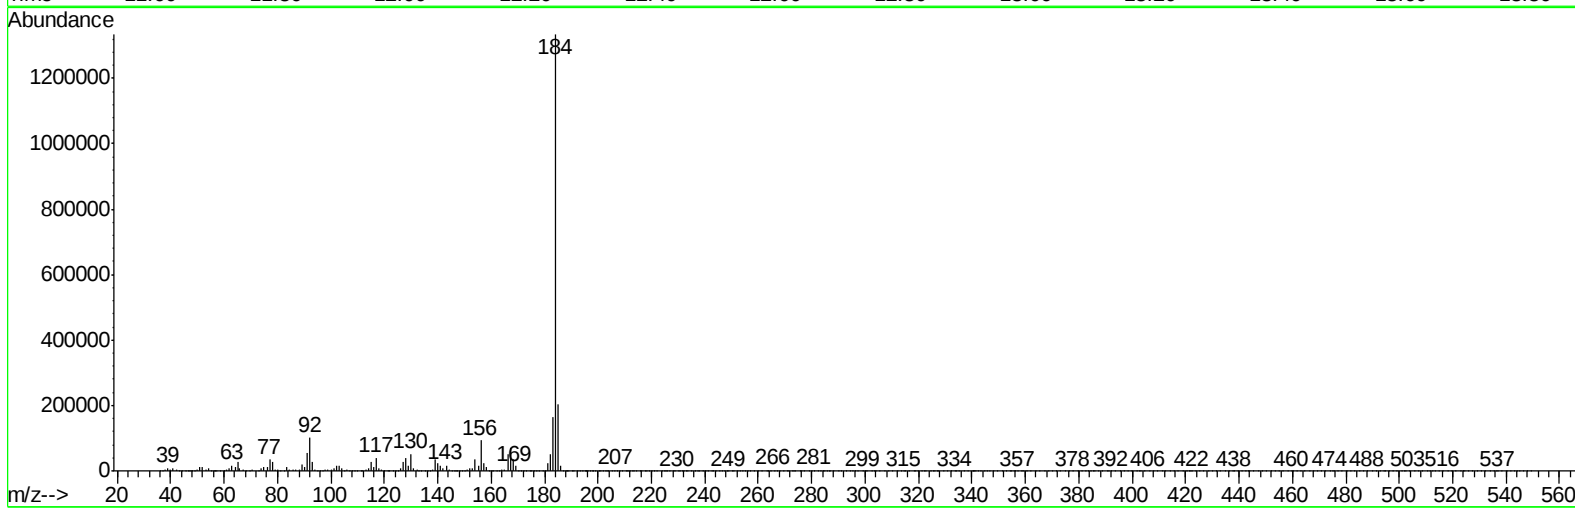


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101819\
Data File : BP000845.D
Acq On : 17 Oct 2019 17:54
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 09:24:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 19:03:29 2019
Response via : Initial Calibration

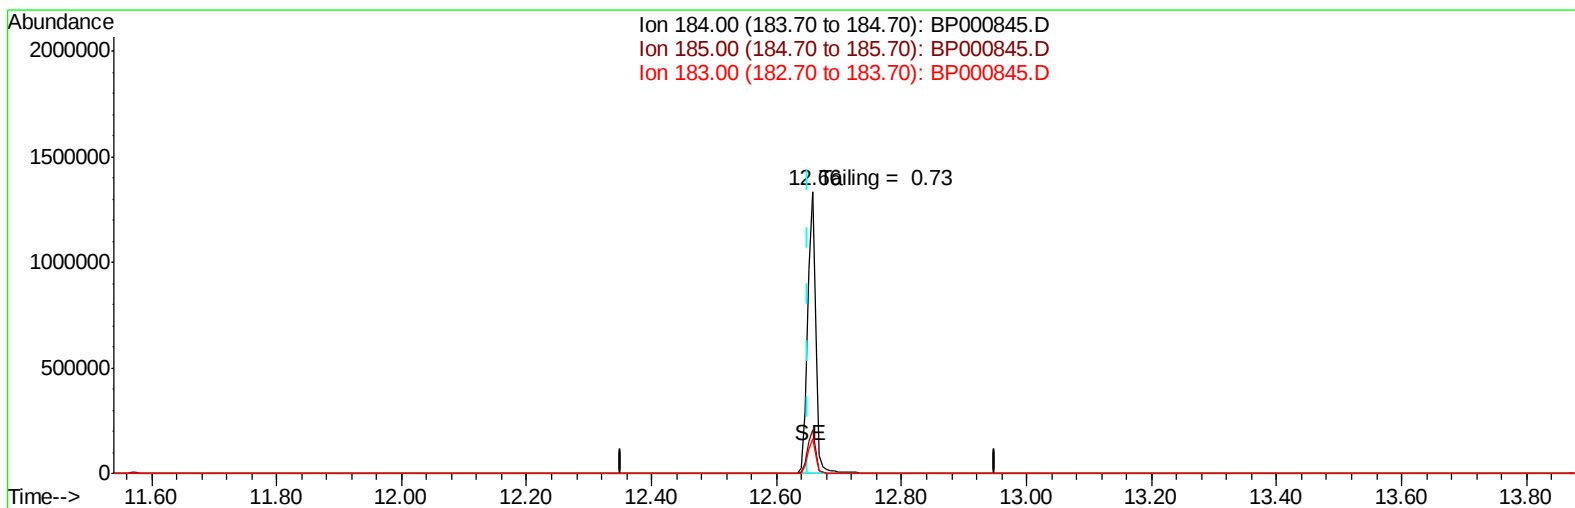

TIC: BP000845.D

(77) Benzidine

12.657min (+0.006) 1241689.06ng

response 1197679

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.30
183.00	11.10	12.20
0.00	0.00	0.00