
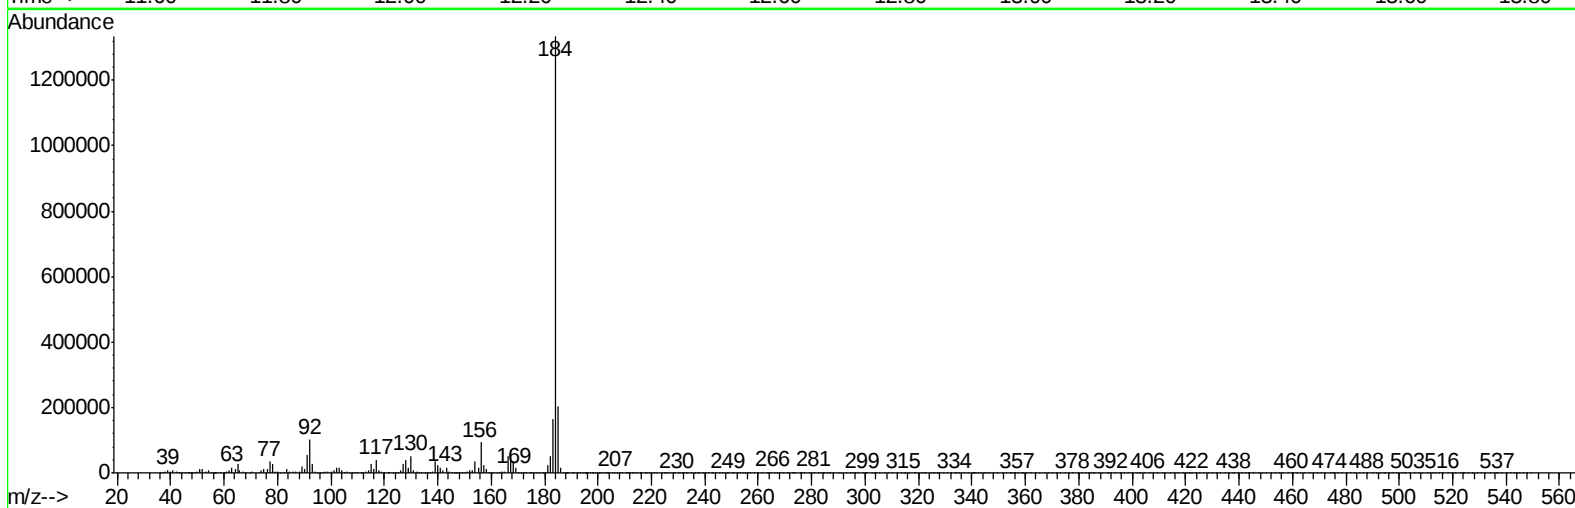


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101819\
 Data File : BP000845.D
 Acq On : 17 Oct 2019 17:54
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 09:24:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 19:03:29 2019
 Response via : Initial Calibration

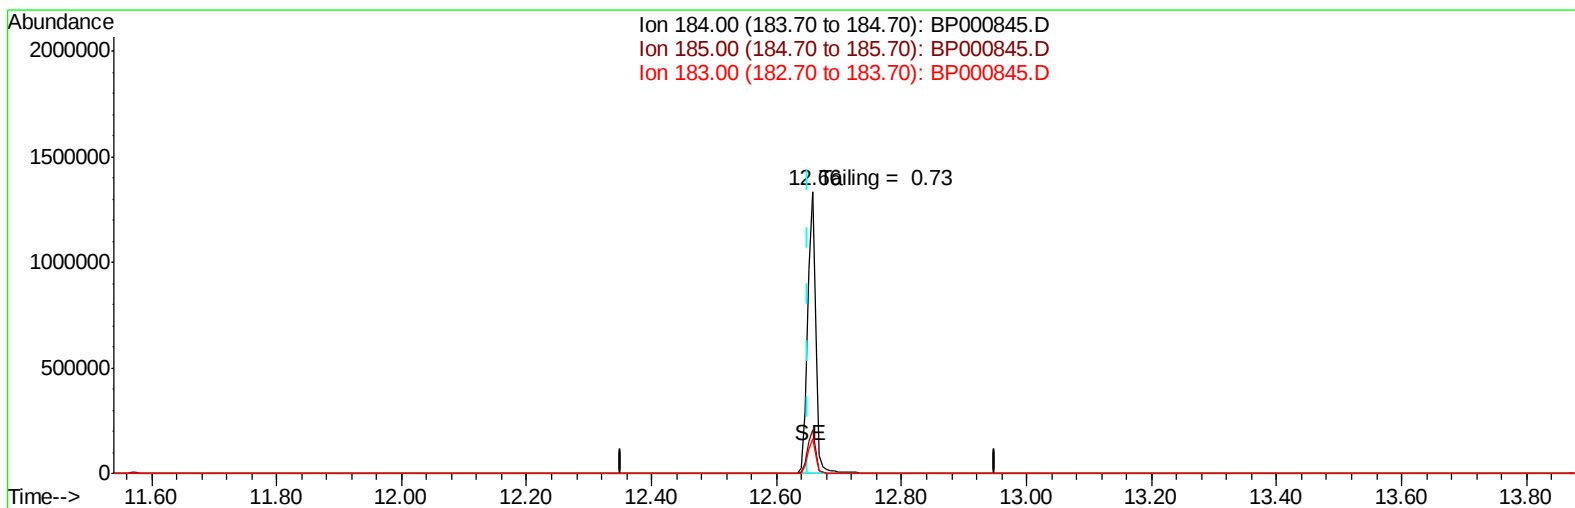

TIC: BP000845.D

(77) Benzidine



12.657min (+0.006) 1241689.06ng

response 1197679

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.30
183.00	11.10	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101819\
 Data File : BP000845.D
 Acq On : 17 Oct 2019 17:54
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 09:24:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 19:03:29 2019
 Response via : Initial Calibration

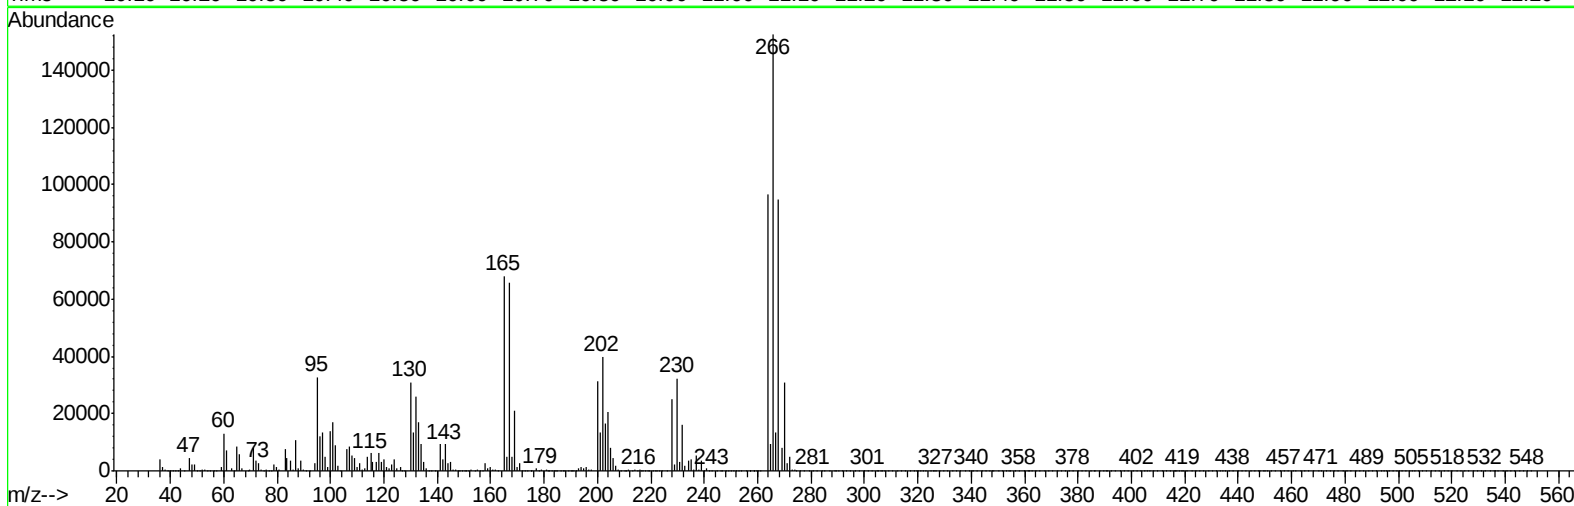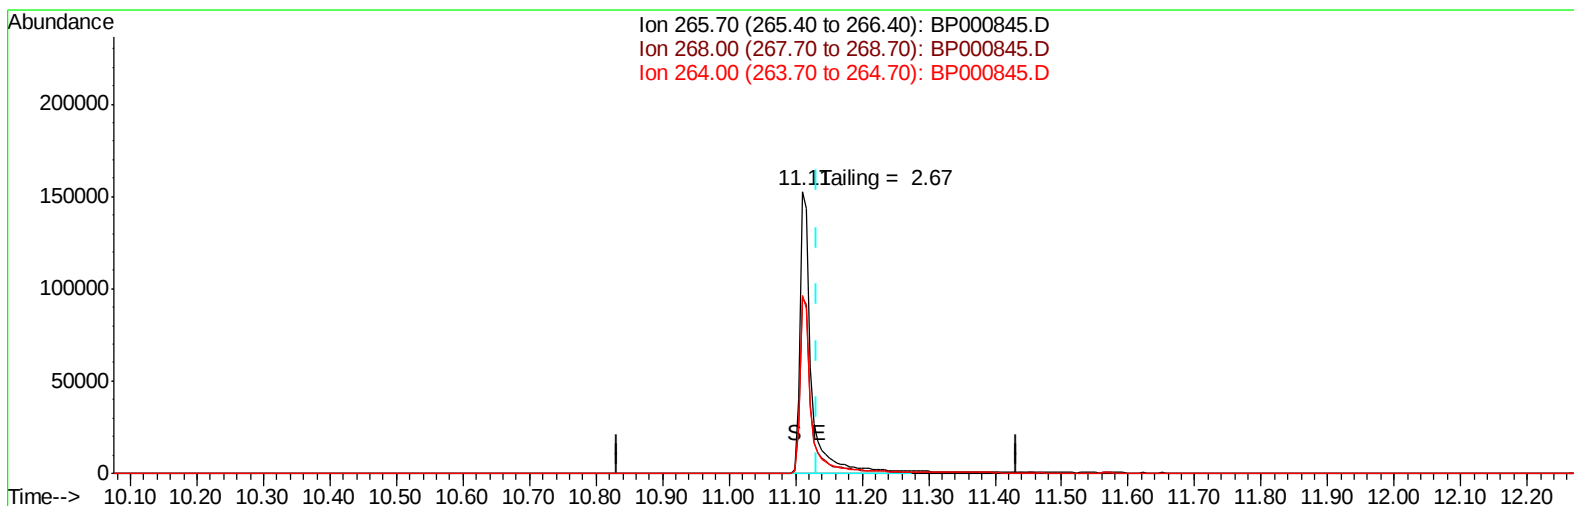

TIC: BP000845.D

(70) Pentachlorophenol (C)

11.110min (-0.023) 248463.74ng

response 186499

Ion	Exp%	Act%
265.70	100	100
268.00	59.70	62.27
264.00	53.60	63.34
0.00	0.00	0.00