


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101819\
 Data File : BP000845.D
 Acq On : 17 Oct 2019 17:54
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 16:40:44 2019

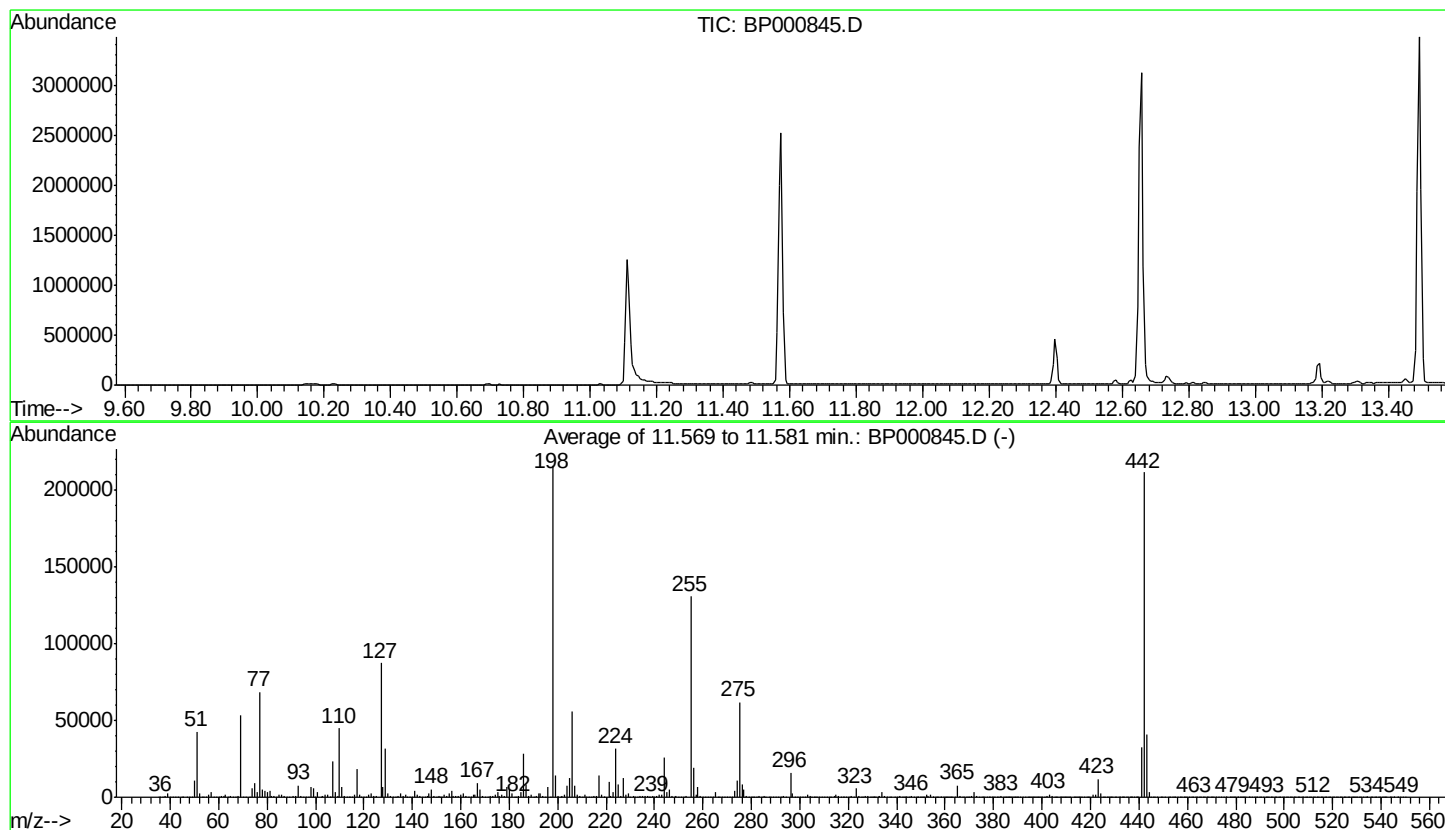

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.9	42831	PASS
68	69	0.00	2	1.8	970	PASS
69	198	0.00	100	24.5	52893	PASS
70	69	0.00	2	0.5	286	PASS
127	198	10	80	40.5	87184	PASS
197	198	0.00	2	0.1	129	PASS
198	198	100	100	100.0	215458	PASS
199	198	5	9	6.7	14520	PASS
275	198	10	60	28.7	61738	PASS
365	198	1	100	3.5	7528	PASS
441	198	0.01	100	15.0	32384	PASS
442	198	50	100	98.1	211362	PASS
443	442	15	24	19.3	40701	PASS