


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101819\
 Data File : BP000873.D
 Acq On : 18 Oct 2019 14:12
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 16:40:44 2019

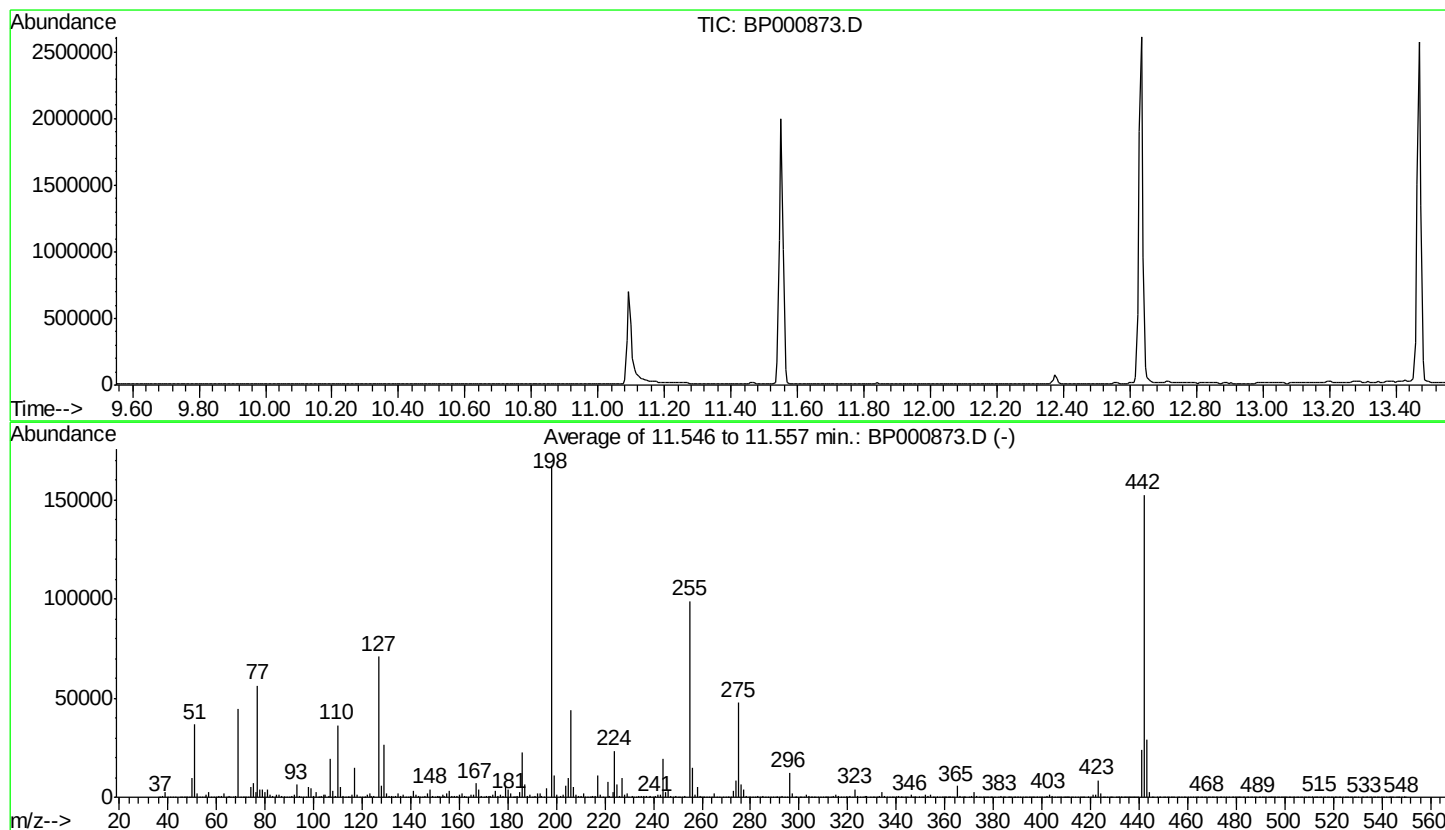

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.9	36588	PASS
68	69	0.00	2	1.7	780	PASS
69	198	0.00	100	26.7	44703	PASS
70	69	0.00	2	0.6	281	PASS
127	198	10	80	42.4	70936	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	167284	PASS
199	198	5	9	6.7	11189	PASS
275	198	10	60	28.5	47642	PASS
365	198	1	100	3.4	5764	PASS
441	198	0.01	100	14.4	24035	PASS
442	198	50	100	91.3	152669	PASS
443	442	15	24	19.1	29164	PASS