

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101823\
 Data File : BP017721.D
 Acq On : 18 Oct 2023 21:48
 Operator : MA/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Quant Time: Oct 19 01:33:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	120198	20.000	ng/u1	0.00
20) Naphthalene-d8	10.722	136	471292	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	290527	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.375	188	609008	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	530456	20.000	ng/u1	0.00
88) Perylene-d12	24.074	264	542475	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	28303	8.760	ng/uL	0.00
4) Pyridine-d5	3.693	84	174372	20.613	ng/u1	0.00
7) Phenol-d5	7.046	99	203315	20.327	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	136999	22.178	ng/u1	0.00
11) 2-Chlorophenol-d4	7.410	132	169908	20.827	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	160115	20.385	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	80533	21.088	ng/u1	0.00
24) 2-Nitrophenol-d4	9.816	143	88106	20.881	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	164376	19.859	ng/u1	0.00
31) 4-Chloroaniline-d4	10.899	131	210719	19.453	ng/u1	0.00
46) Dimethylphthalate-d6	14.004	166	493032	20.215	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	561641	20.650	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	63056	18.145	ng/u1	0.00
60) Fluorene-d10	15.592	176	418569	19.854	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	74860	18.661	ng/u1	0.00
73) Anthracene-d10	17.481	188	637065	20.470	ng/u1	0.00
81) Pyrene-d10	19.739	212	710411	21.361	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.904	264	612650	20.277	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	29700	8.666	ng/uL	99
5) Pyridine	3.711	79	184943	21.338	ng/u1	98
6) Benzaldehyde	7.052	77	130874	24.323	ng/u1	96
8) Phenol	7.075	94	204342	20.720	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.328	93	175730	21.358	ng/u1	98
12) 2-Chlorophenol	7.440	128	170723	20.836	ng/u1	98
13) 2-Methylphenol	8.340	108	153054	20.564	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.405	45	137397	13.567	ng/u1	99
16) Acetophenone	8.746	105	262417	21.250	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.710	70	135055	23.058	ng/u1	98
18) 4-Methylphenol	8.675	108	163428	20.677	ng/u1	93
19) Hexachloroethane	8.952	117	79005	20.985	ng/u1	87
22) Nitrobenzene	9.140	77	211724	22.266	ng/u1	97
23) Isophorone	9.652	82	374452	22.022	ng/u1	98
25) 2-Nitrophenol	9.846	139	93181	20.689	ng/u1	91
26) 2,4-Dimethylphenol	9.887	107	186232	21.067	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.146	93	228160	21.695	ng/u1	98
29) 2,4-Dichlorophenol	10.369	162	157758	19.932	ng/u1	95
30) Naphthalene	10.775	128	558718	20.600	ng/u1	100
32) 4-Chloroaniline	10.922	127	203086	19.579	ng/u1	96
33) Hexachlorobutadiene	10.999	225	118026	18.365	ng/u1	97
34) Caprolactam	11.757	113	40040	19.646	ng/u1	93
35) 4-Chloro-3-methylphenol	12.034	107	162270	21.777	ng/u1	93
36) 2-Methylnaphthalene	12.393	142	366267	19.992	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101823\
 Data File : BP017721.D
 Acq On : 18 Oct 2023 21:48
 Operator : MA/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SICV602


Quant Time: Oct 19 01:33:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.610	142	378934	20.225	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.745	216	203432	18.923	ng/ul	98
40) Hexachlorocyclopentadiene	12.687	237	101866	16.493	ng/ul	99
41) 2,4,6-Trichlorophenol	13.004	196	128174	19.866	ng/ul	99
42) 2,4,5-Trichlorophenol	13.081	196	130961	19.633	ng/ul	99
43) 1,1'-Biphenyl	13.410	154	493704	20.627	ng/ul	99
44) 2-Chloronaphthalene	13.457	162	393253	20.324	ng/ul	98
45) 2-Nitroaniline	13.710	65	105058	23.894	ng/ul	97
47) Dimethylphthalate	14.051	163	486586	20.243	ng/ul	99
48) 2,6-Dinitrotoluene	14.204	165	93861	21.215	ng/ul	92
50) Acenaphthylene	14.310	152	637470	20.924	ng/ul	99
51) 3-Nitroaniline	14.545	138	84560	20.096	ng/ul	98
52) Acenaphthene	14.651	153	422111	20.495	ng/ul	99
53) 2,4-Dinitrophenol	14.757	184	37887	15.255	ng/ul#	85
55) 4-Nitrophenol	14.845	109	75572	20.544	ng/ul	95
56) Dibenzofuran	14.992	168	581618	20.114	ng/ul	93
57) 2,4-Dinitrotoluene	14.992	165	138250	21.173	ng/ul	93
58) 2,3,4,6-Tetrachlorophenol	15.216	232	110193	18.616	ng/ul#	90
59) Diethylphthalate	15.416	149	483930	20.852	ng/ul	98
61) Fluorene	15.651	166	476012	20.040	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.639	204	240819	19.075	ng/ul	91
63) 4-Nitroaniline	15.728	138	76312	20.107	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.751	198	80187	18.663	ng/ul	92
67) N-Nitrosodiphenylamine	15.869	169	394511	21.383	ng/ul	99
68) 4-Bromophenyl-phenylether	16.551	248	133384	18.719	ng/ul#	93
69) Hexachlorobenzene	16.628	284	145356	17.768	ng/ul#	86
70) Atrazine	16.834	200	132402	19.525	ng/ul	99
71) Pentachlorophenol	17.004	266	81208	16.512	ng/ul	97
72) Phenanthrene	17.422	178	736491	20.644	ng/ul	100
74) Anthracene	17.516	178	750729	20.777	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.363	216	205721	20.132	ng/uL	98
76) Pentachlorobenzene	14.881	250	186608	18.843	ng/uL	98
77) Carbazole	17.810	167	635228	20.801	ng/ul	99
78) Di-n-butylphthalate	18.322	149	771334	21.756	ng/ul	99
80) Fluoranthene	19.404	202	841585	22.025	ng/ul	97
82) Pyrene	19.769	202	875479	21.626	ng/ul	97
83) Butylbenzylphthalate	20.639	149	325237	23.359	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.445	252	225692	18.832	ng/ul#	98
85) Benzo(a)anthracene	21.504	228	840539	20.844	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.380	149	459387	23.635	ng/ul#	98
87) Chrysene	21.557	228	787675	20.655	ng/ul	99
89) Di-n-octyl phthalate	22.363	149	778832	22.666	ng/ul	100
90) Benzo(b)fluoranthene	23.274	252	766027	20.749	ng/ul	98
91) Benzo(k)fluoranthene	23.327	252	766695	20.490	ng/ul	99
93) Benzo(a)pyrene	23.957	252	722285	20.839	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.786	276	813451	19.692	ng/ul#	95
95) Dibenzo(a,h)anthracene	26.809	278	670127	19.443	ng/ul	97
96) Benzo(g,h,i)perylene	27.627	276	651285	19.568	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 19 01:33:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration




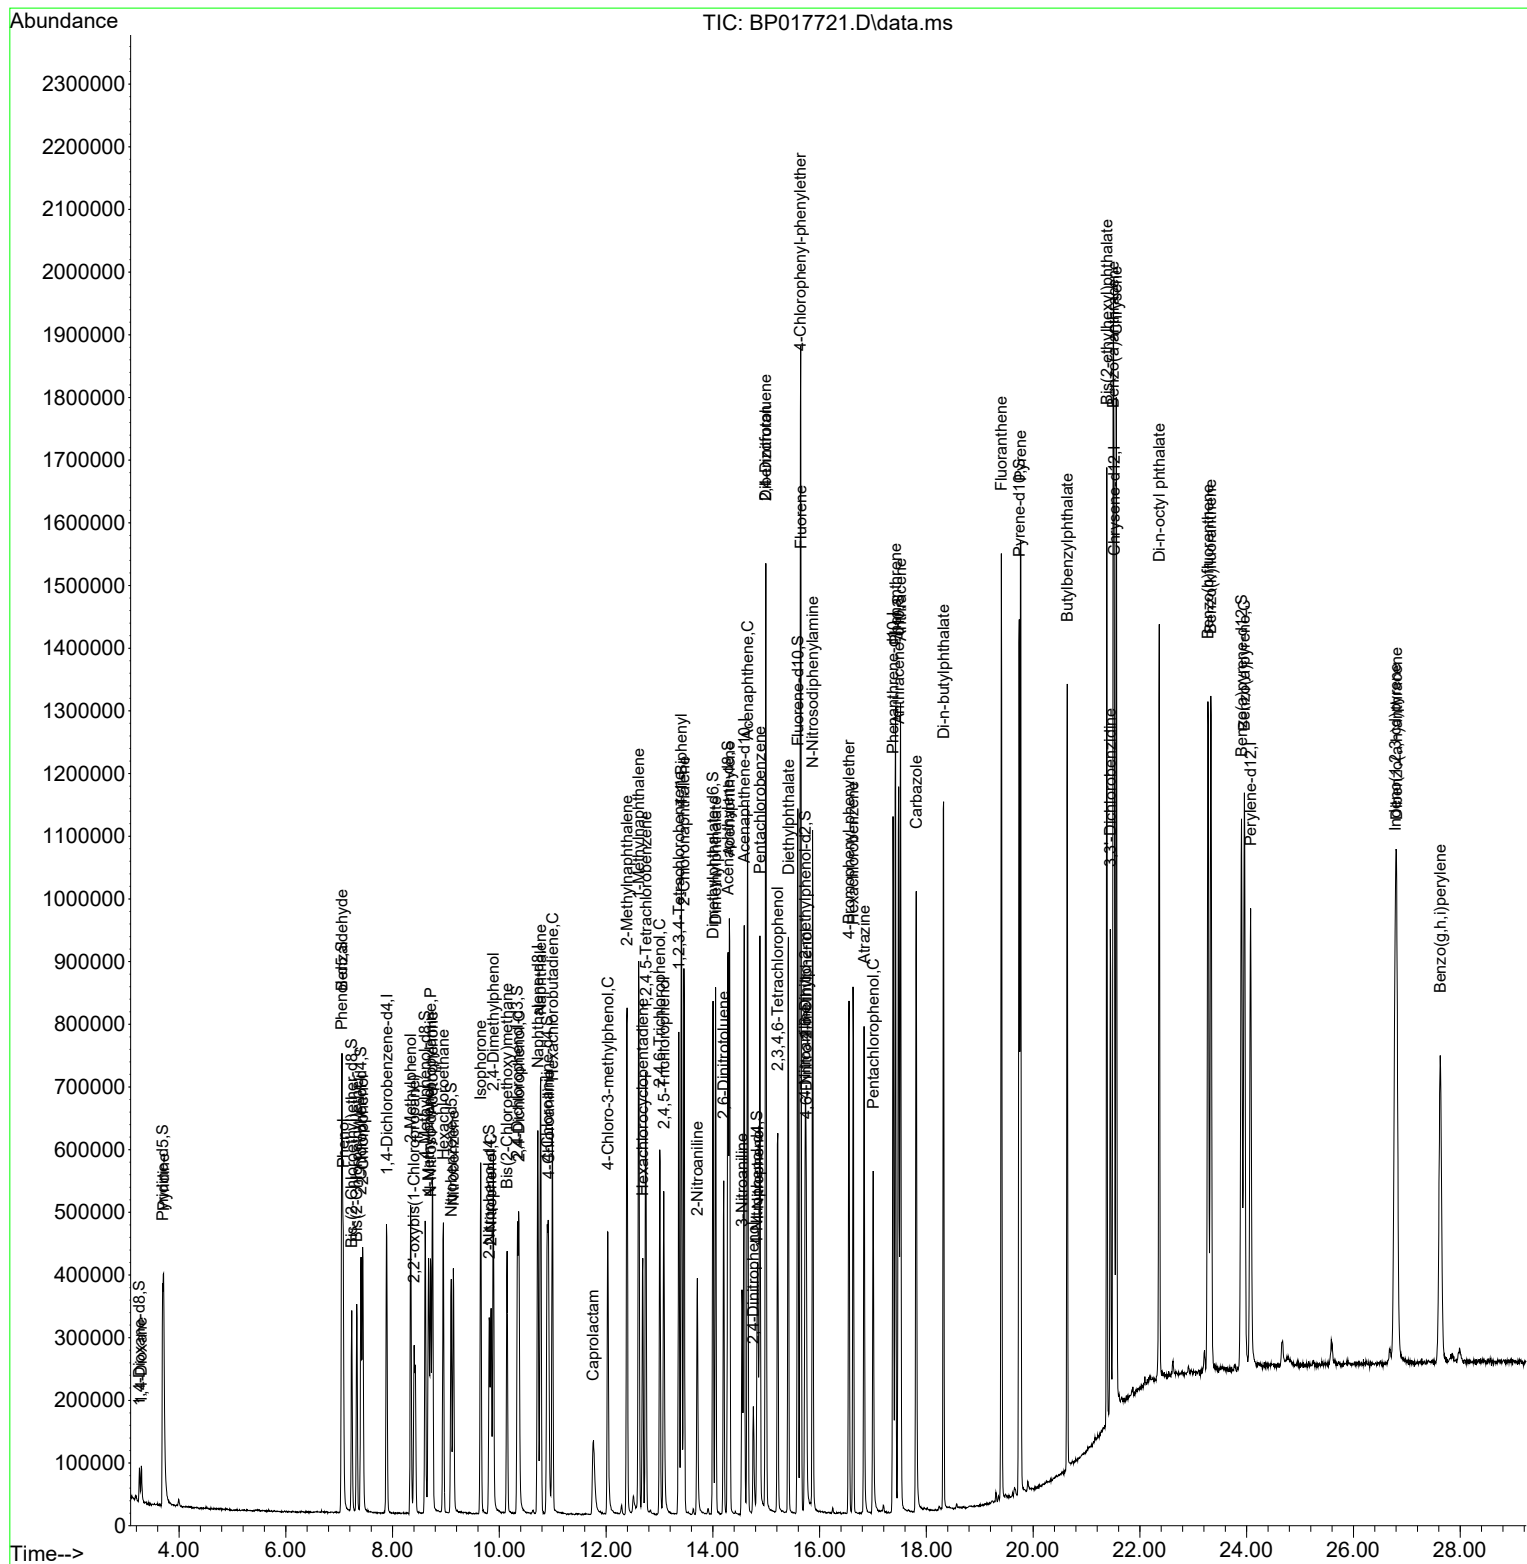




#2
1,4-Dioxane
Concen: 8.666 ng/uL
RT: 3.293 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion: 88	Resp: 29700
Ion Ratio	Lower Upper
88 100	
43 31.2	24.4 36.6
58 65.3	53.0 79.6

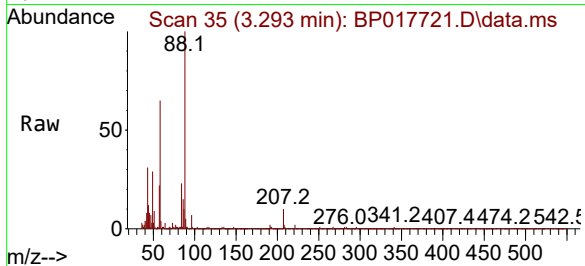

#5
Pyridine
Concen: 21.338 ng/uL
RT: 3.711 min Scan# 106
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion: 79	Resp: 184943
Ion Ratio	Lower Upper
79 100	
52 70.1	57.2 85.8
51 36.8	28.6 42.8




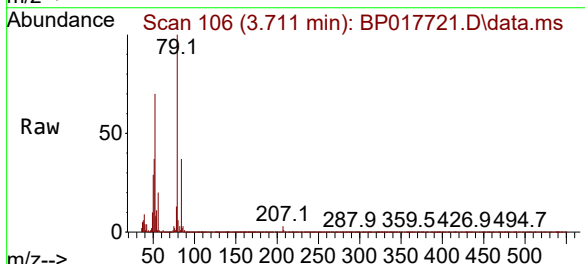




#6
Benzaldehyde
Concen: 24.323 ng/ul
RT: 7.052 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion: 77 Resp: 130874
Ion Ratio Lower Upper
77 100
105 90.1 75.4 113.2
106 86.3 72.3 108.5



#8
Phenol
Concen: 20.720 ng/ul
RT: 7.075 min Scan# 678
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion: 94 Resp: 204342
Ion Ratio Lower Upper
94 100
65 31.1 25.0 37.4
66 42.0 33.0 49.6

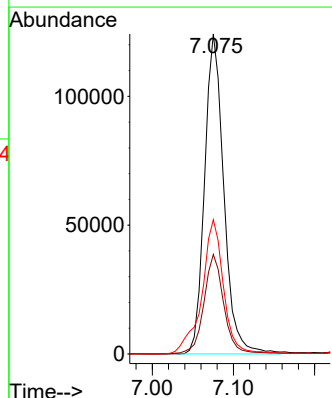







#10
 Bis(2-Chloroethyl)ether
 Concen: 21.358 ng/ul
 RT: 7.328 min Scan# 721
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Tgt Ion: 93 Resp: 175730




Ion	Ratio	Lower	Upper
93	100		
63	75.7	60.7	91.1
95	32.2	27.8	41.6

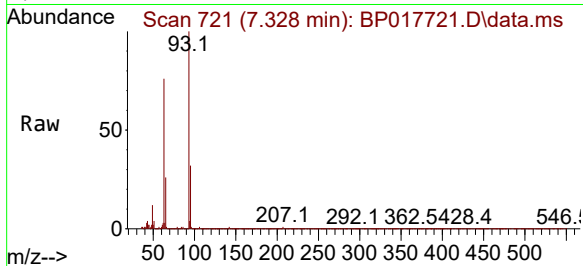


#12
 2-Chlorophenol
 Concen: 20.836 ng/ul
 RT: 7.440 min Scan# 740
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Tgt Ion: 128 Resp: 170723

Ion	Ratio	Lower	Upper
128	100		
64	48.3	36.7	55.1
130	33.1	26.2	39.2

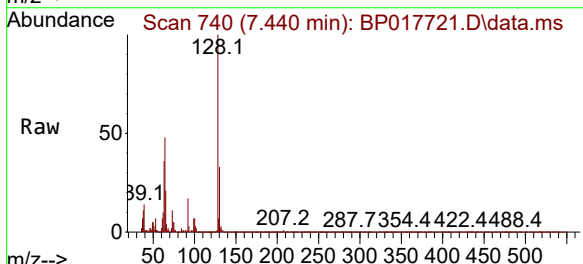



#13

2-Methylphenol

Concen: 20.564 ng/ul

RT: 8.340 min Scan# 893

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :





SICV602

Tgt Ion:108 Resp: 153054

Ion Ratio Lower Upper

108 100

107 90.6 73.4 110.2

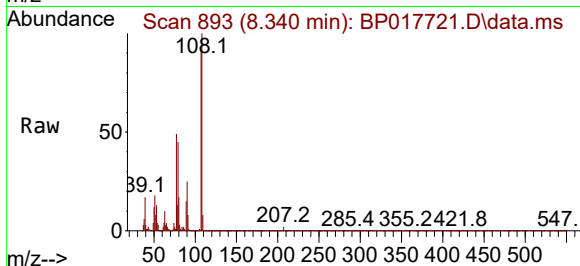

#14

2,2'-oxybis(1-Chloropropane)

Concen: 13.567 ng/ul

RT: 8.405 min Scan# 904

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion: 45 Resp: 137397


Ion Ratio Lower Upper

45 100

77 17.9 14.2 21.4

79 14.0 10.3 15.5



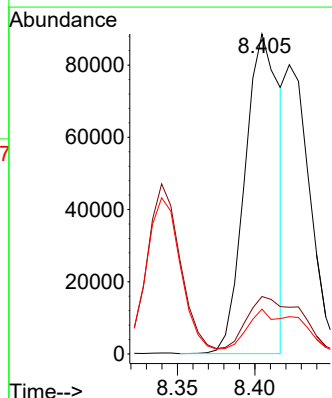
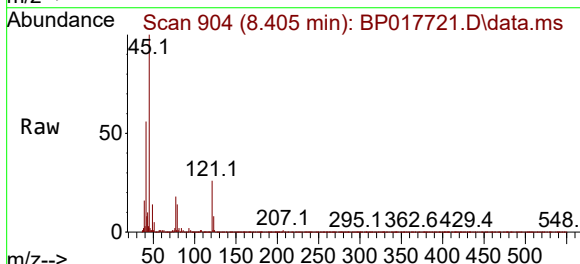




#16
Acetophenone
Concen: 21.250 ng/ul
RT: 8.746 min Scan# 90
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:105 Resp: 262417
Ion Ratio Lower Upper
105 100
77 81.5 64.4 96.6
51 27.2 21.2 31.8



#17
N-Nitroso-di-n-propylamine
Concen: 23.058 ng/ul
RT: 8.710 min Scan# 956
Delta R.T. -0.006 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion: 70 Resp: 135055
Ion Ratio Lower Upper
70 100
42 55.7 44.6 66.8
101 8.7 7.5 11.3
130 19.1 17.3 25.9



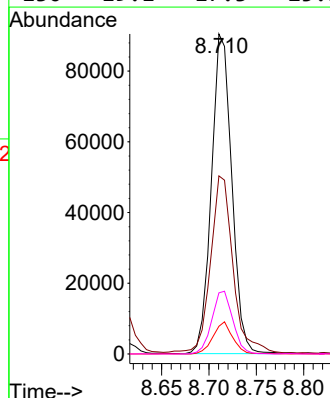





#18
4-Methylphenol
Concen: 20.677 ng/ul
RT: 8.675 min Scan# 911
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:108 Resp: 163428
Ion Ratio Lower Upper
108 100
107 116.3 87.5 131.3



#19
Hexachloroethane
Concen: 20.985 ng/ul
RT: 8.952 min Scan# 997
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:117 Resp: 79005
Ion Ratio Lower Upper
117 100
201 103.1 96.3 144.5
199 65.7 57.7 86.5









#22
Nitrobenzene
Concen: 22.266 ng/ul
RT: 9.140 min Scan# 1029
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion: 77 Resp: 211724
Ion Ratio Lower Upper
77 100
123 39.6 33.5 50.3
65 13.2 10.8 16.2



#23
Isophorone
Concen: 22.022 ng/ul
RT: 9.652 min Scan# 1116
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion: 82 Resp: 374452
Ion Ratio Lower Upper
82 100
95 7.8 6.2 9.2
138 16.6 14.4 21.6









#25
2-Nitrophenol
Concen: 20.689 ng/ul
RT: 9.846 min Scan# 1149
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:139 Resp: 93181
Ion Ratio Lower Upper
139 100
65 58.5 40.4 60.6
109 35.1 25.4 38.2



#26
2,4-Dimethylphenol
Concen: 21.067 ng/ul
RT: 9.887 min Scan# 1156
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:107 Resp: 186232
Ion Ratio Lower Upper
107 100
121 48.9 40.6 61.0
122 80.5 66.9 100.3









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.695 ng/ul
 RT: 10.146 min Scan# 1200
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48




Instrument :
 BNA_P
 ClientSampleId :
 SICV602


Tgt Ion: 93 Resp: 228160
 Ion Ratio Lower Upper
 93 100
 95 32.5 24.7 37.1
 123 11.1 8.9 13.3



#29
 2,4-Dichlorophenol
 Concen: 19.932 ng/ul
 RT: 10.369 min Scan# 1238
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Tgt Ion: 162 Resp: 157758
 Ion Ratio Lower Upper
 162 100
 164 64.7 53.8 80.8
 98 36.4 25.5 38.3









#30
Naphthalene
Concen: 20.600 ng/ul
RT: 10.775 min Scan# 1307
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:128 Resp: 558718
Ion Ratio Lower Upper
128 100
129 10.6 8.7 13.1
127 13.2 10.5 15.7



#32
4-Chloroaniline
Concen: 19.579 ng/ul
RT: 10.922 min Scan# 1332
Delta R.T. 0.006 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:127 Resp: 203086
Ion Ratio Lower Upper
127 100
129 33.4 25.1 37.7









#33
Hexachlorobutadiene
Concen: 18.365 ng/ul
RT: 10.999 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:225 Resp: 118026
Ion Ratio Lower Upper
225 100
223 58.8 50.6 75.8
227 61.7 50.1 75.1

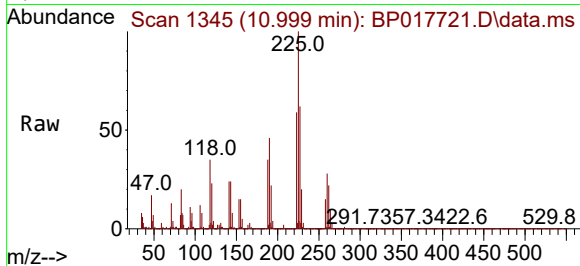

#34
Caprolactam
Concen: 19.646 ng/ul
RT: 11.757 min Scan# 1474
Delta R.T. -0.012 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:113 Resp: 40040
Ion Ratio Lower Upper
113 100
55 149.0 112.1 168.1
56 115.3 87.0 130.6




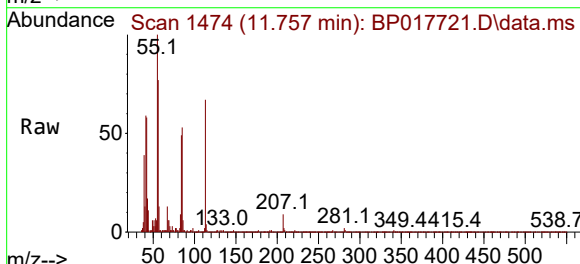




#35
4-Chloro-3-methylphenol
Concen: 21.777 ng/ul
RT: 12.034 min Scan# 1521
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:107 Resp: 162270
Ion Ratio Lower Upper
107 100
144 25.3 22.9 34.3
142 78.9 68.1 102.1



#36
2-Methylnaphthalene
Concen: 19.992 ng/ul
RT: 12.393 min Scan# 1582
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:142 Resp: 366267
Ion Ratio Lower Upper
142 100
141 90.4 71.5 107.3

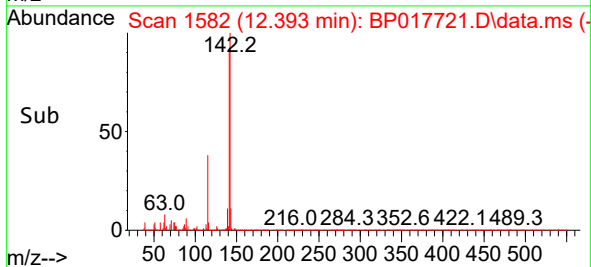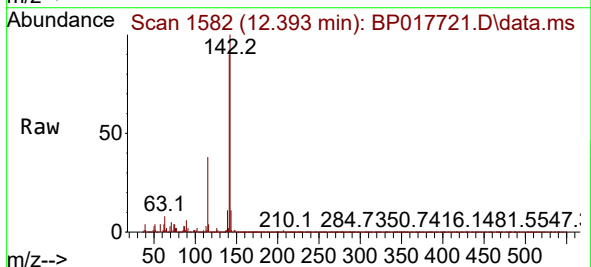



#37

1-Methylnaphthalene

Concen: 20.225 ng/ul

RT: 12.610 min Scan# 1619

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:142 Resp: 378934

Ion Ratio Lower Upper

142 100

141 92.5 72.5 108.7

116 4.4 3.4 5.2



#39

1,2,4,5-Tetrachlorobenzene

Concen: 18.923 ng/ul

RT: 12.745 min Scan# 1642

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Tgt Ion:216 Resp: 203432




Ion Ratio Lower Upper


216 100

214 78.4 62.2 93.2

179 21.7 15.8 23.8

108 18.6 12.6 18.8









#40
Hexachlorocyclopentadiene
Concen: 16.493 ng/ul
RT: 12.687 min Scan# 1632
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:237 Resp: 101866
Ion Ratio Lower Upper
237 100
235 62.8 50.3 75.5
272 11.6 11.1 16.7



#41
2,4,6-Trichlorophenol
Concen: 19.866 ng/ul
RT: 13.004 min Scan# 1686
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:196 Resp: 128174
Ion Ratio Lower Upper
196 100
198 92.7 74.7 112.1
200 31.1 23.7 35.5









#42
2,4,5-Trichlorophenol
Concen: 19.633 ng/ul
RT: 13.081 min Scan# 1699
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:196 Resp: 130961
Ion Ratio Lower Upper
196 100
198 93.9 76.0 114.0
200 31.3 24.3 36.5

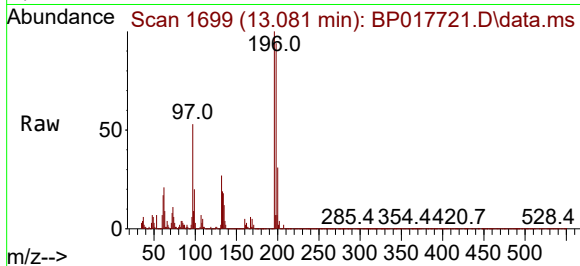

#43
1,1'-Biphenyl
Concen: 20.627 ng/ul
RT: 13.410 min Scan# 1755
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:154 Resp: 493704
Ion Ratio Lower Upper
154 100
153 40.4 32.6 49.0
76 12.8 9.8 14.8

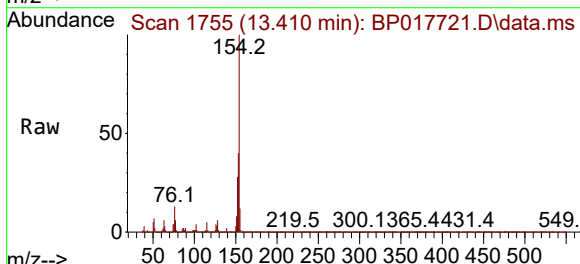



#44

2-Chloronaphthalene

Concen: 20.324 ng/ul

RT: 13.457 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:162 Resp: 393253

Ion Ratio Lower Upper

162 100

164 32.3 25.9 38.9

127 39.7 29.9 44.9

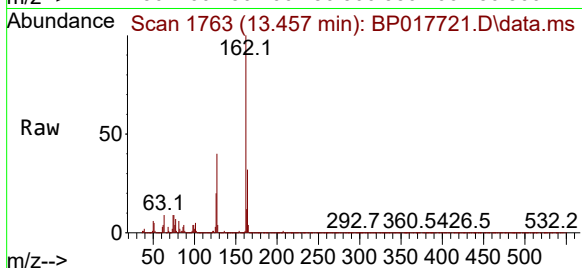

#45

2-Nitroaniline

Concen: 23.894 ng/ul

RT: 13.710 min Scan# 1806

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion: 65 Resp: 105058


Ion Ratio Lower Upper

65 100

92 70.0 56.2 84.4

138 102.1 85.9 128.9




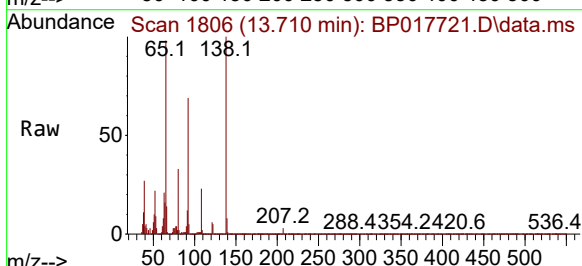


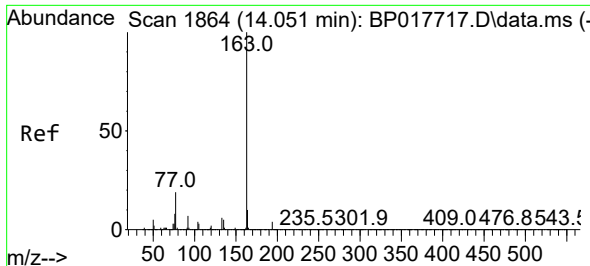

#47
Dimethylphthalate
Concen: 20.243 ng/ul
RT: 14.051 min Scan# 1864
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:163 Resp: 486586
Ion Ratio Lower Upper
163 100
194 4.4 3.4 5.0
164 9.9 8.2 12.4

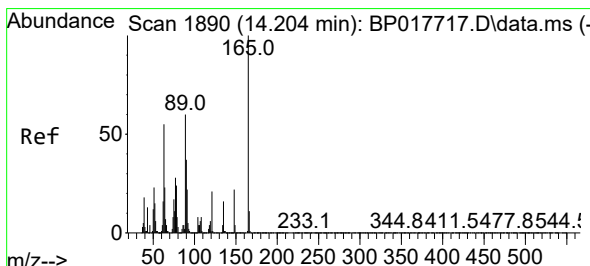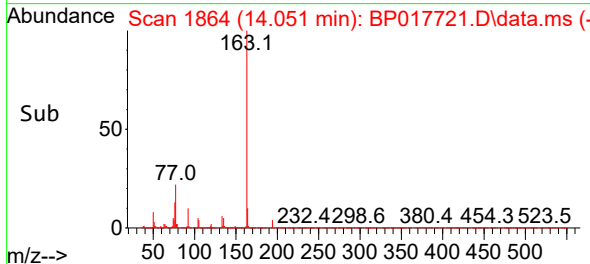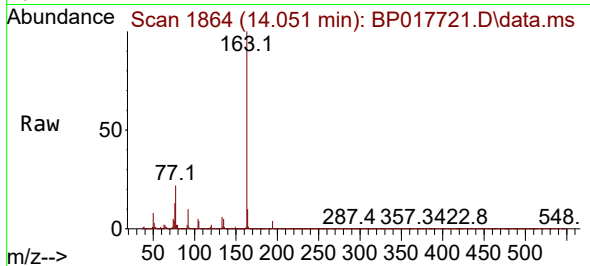

#48
2,6-Dinitrotoluene
Concen: 21.215 ng/ul
RT: 14.204 min Scan# 1890
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:165 Resp: 93861
Ion Ratio Lower Upper
165 100
89 66.7 48.0 72.0
121 23.2 16.6 24.8

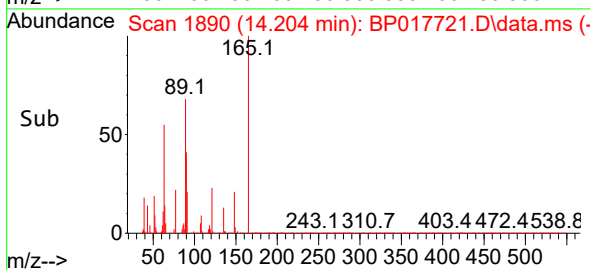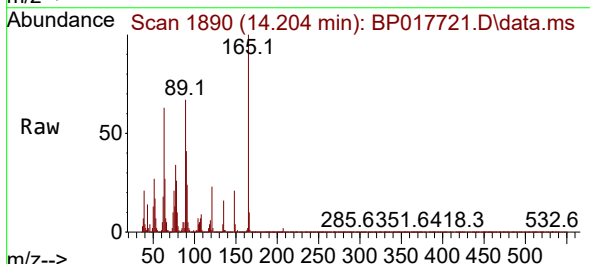



#50

Acenaphthylene

Concen: 20.924 ng/ul

RT: 14.310 min Scan# 1908

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:152 Resp: 637470

Ion Ratio Lower Upper

152 100

151 19.1 15.9 23.9

153 13.3 10.8 16.2

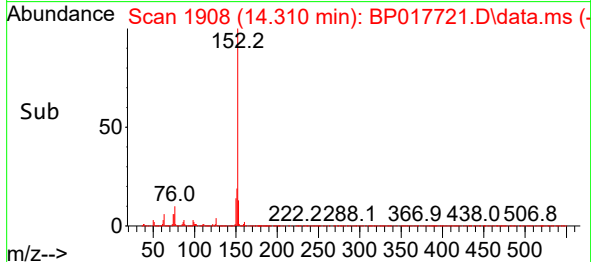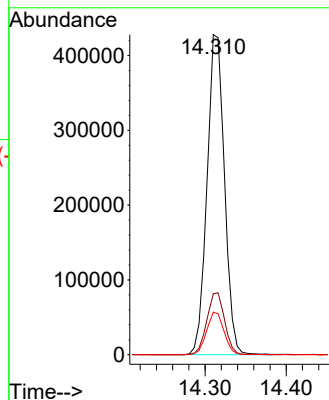

#51

3-Nitroaniline

Concen: 20.096 ng/ul

RT: 14.545 min Scan# 1948

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:138 Resp: 84560


Ion Ratio Lower Upper

138 100

108 10.8 9.3 13.9

92 121.7 95.2 142.8

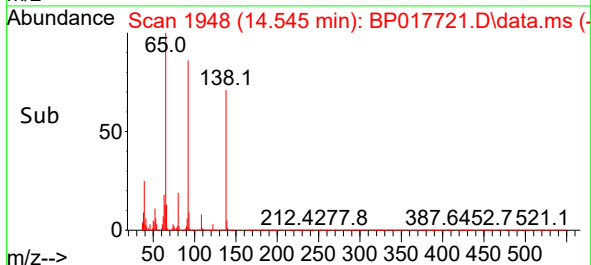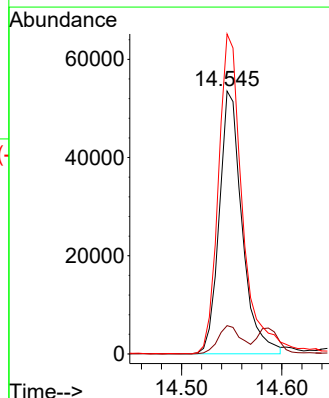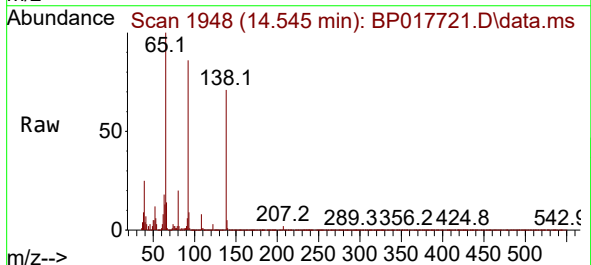

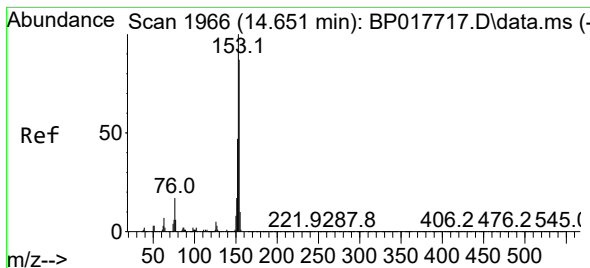

#52

Acenaphthene

Concen: 20.495 ng/ul

RT: 14.651 min Scan# 1966

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:153 Resp: 422111

Ion Ratio Lower Upper

153 100

152 48.0 37.6 56.4

154 87.5 70.0 105.0

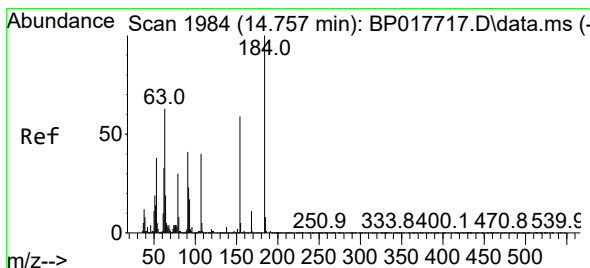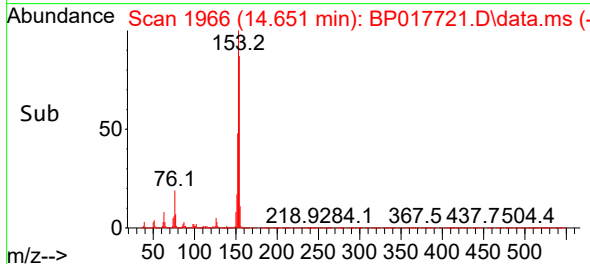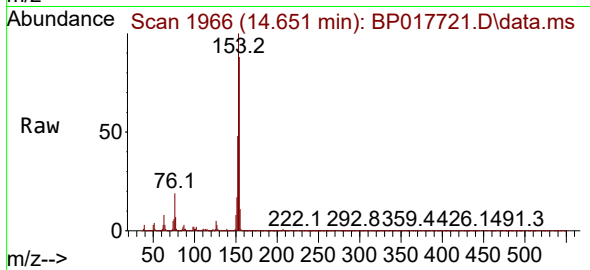

#53

2,4-Dinitrophenol

Concen: 15.255 ng/ul

RT: 14.757 min Scan# 1984

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:184 Resp: 37887


Ion Ratio Lower Upper

184 100

63 80.1 50.6 76.0#

154 65.4 47.9 71.9


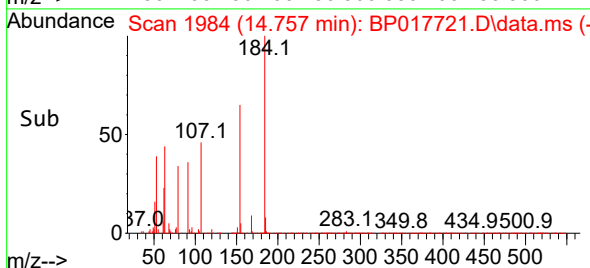
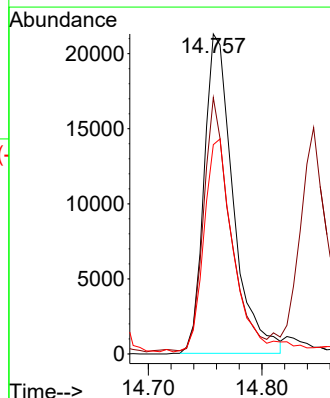
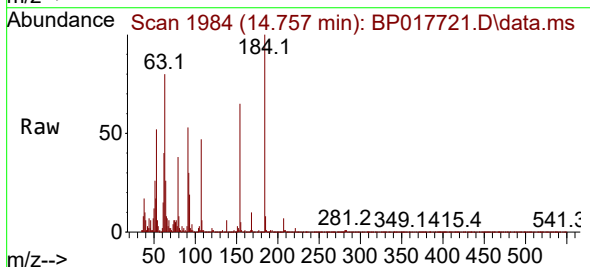




#55
4-Nitrophenol
Concen: 20.544 ng/ul
RT: 14.845 min Scan# 1999
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion	Ratio	Lower	Upper
109	100		
139	110.6	92.9	139.3
65	123.2	94.5	141.7

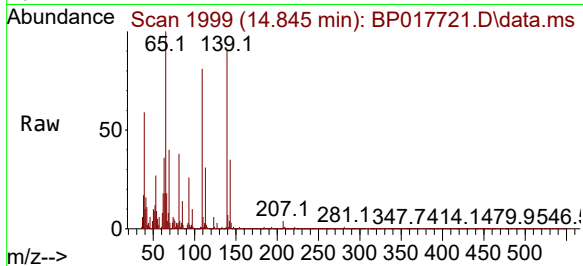

#56
Dibenzofuran
Concen: 20.114 ng/ul
RT: 14.992 min Scan# 2024
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion	Ratio	Lower	Upper
168	100		
139	39.6	28.6	43.0




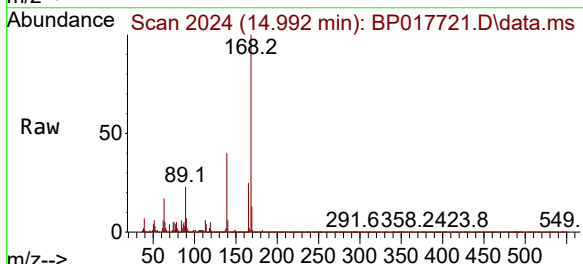


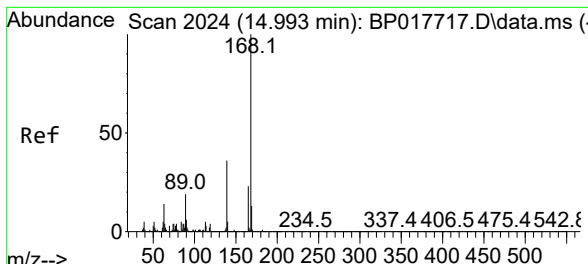

#57
 2,4-Dinitrotoluene
 Concen: 21.173 ng/ul
 RT: 14.992 min Scan# 2024
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48




Instrument :
 BNA_P
 ClientSampleId :
 SICV602


Tgt Ion:	165	Resp:	138250
Ion Ratio	Lower	Upper	
165	100		
63	69.7	51.1	76.7
182	2.8	2.7	4.1

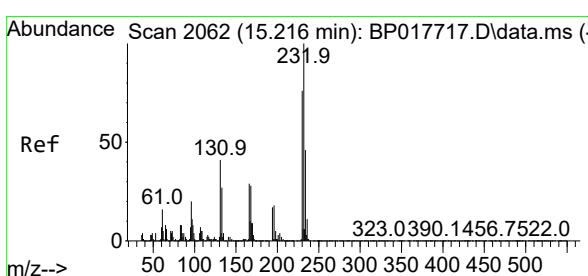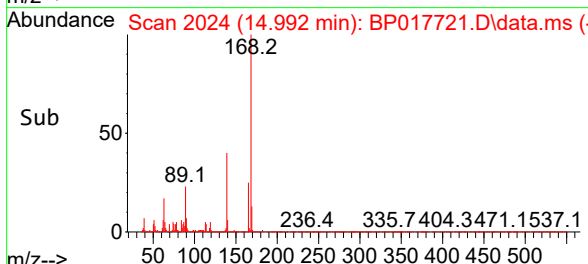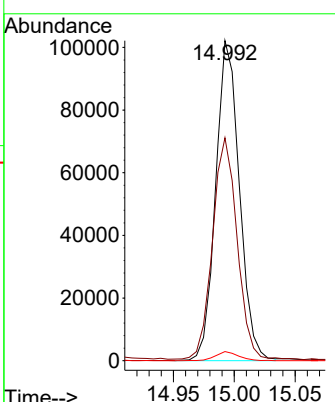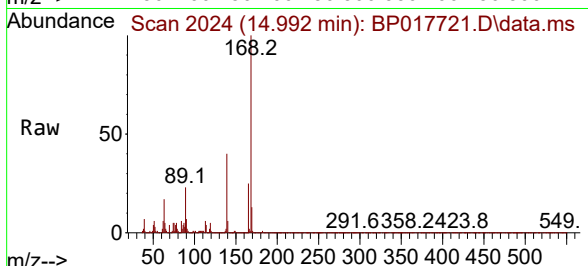

#58
 2,3,4,6-Tetrachlorophenol
 Concen: 18.616 ng/ul
 RT: 15.216 min Scan# 2062
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Tgt Ion:	232	Resp:	110193
Ion Ratio	Lower	Upper	
232	100		
131	48.9	32.9	49.3
130	2.9	1.8	2.8#
166	32.9	23.3	34.9

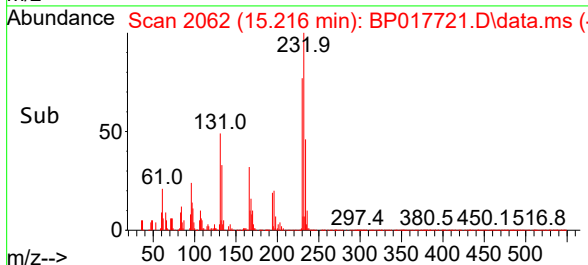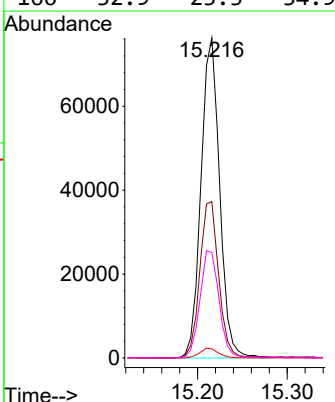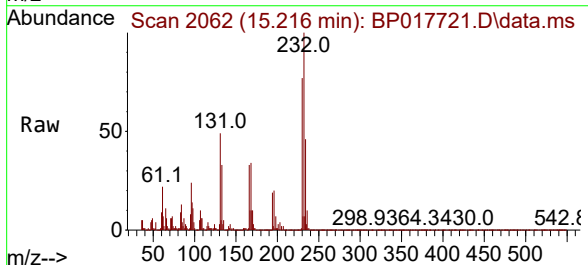



#59

Diethylphthalate

Concen: 20.852 ng/ul

RT: 15.416 min Scan# 2095

Delta R.T. 0.006 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:149 Resp: 483930

Ion Ratio Lower Upper

149 100

177 21.2 18.0 27.0

150 12.3 10.2 15.4

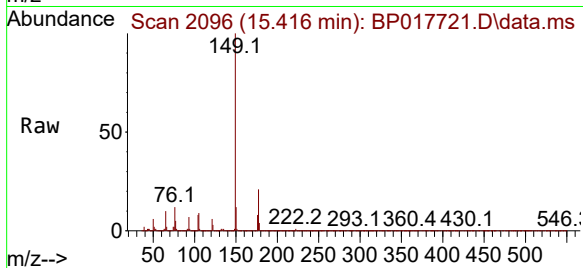

#61

Fluorene

Concen: 20.040 ng/ul

RT: 15.651 min Scan# 2136

Delta R.T. 0.006 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:166 Resp: 476012


Ion Ratio Lower Upper

166 100

165 97.3 77.4 116.0

167 13.2 10.9 16.3




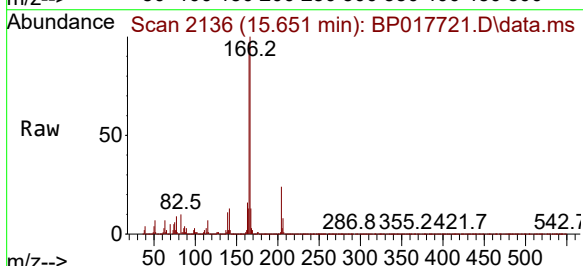




#62
4-Chlorophenyl-phenylether
Concen: 19.075 ng/ul
RT: 15.639 min Scan# 2134
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:204 Resp: 240819
Ion Ratio Lower Upper
204 100
206 34.1 26.2 39.4
141 62.4 42.9 64.3

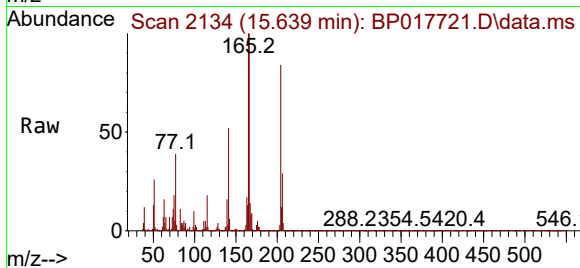

#63
4-Nitroaniline
Concen: 20.107 ng/ul
RT: 15.728 min Scan# 2149
Delta R.T. 0.006 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:138 Resp: 76312
Ion Ratio Lower Upper
138 100
92 57.0 43.0 64.6
108 113.8 82.7 124.1




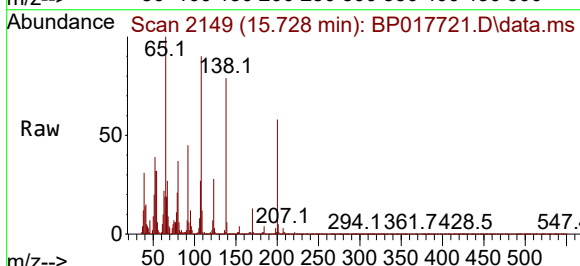


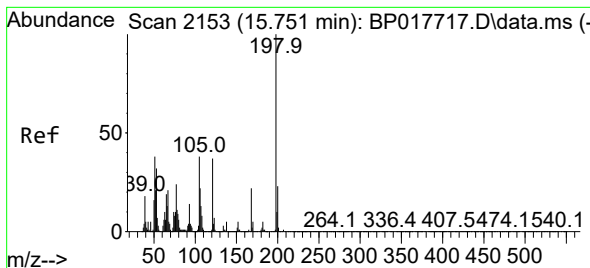

#66
4,6-Dinitro-2-methylphenol
Concen: 18.663 ng/ul
RT: 15.751 min Scan# 2153
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:198 Resp: 80187
Ion Ratio Lower Upper
198 100
182 5.5 3.9 5.9
77 29.7 19.8 29.8

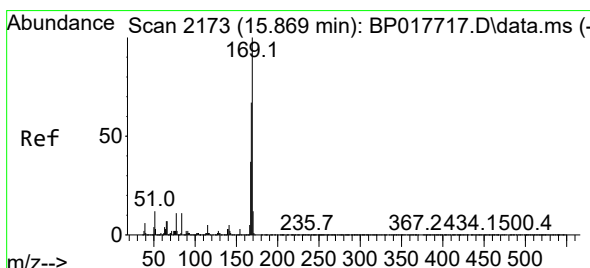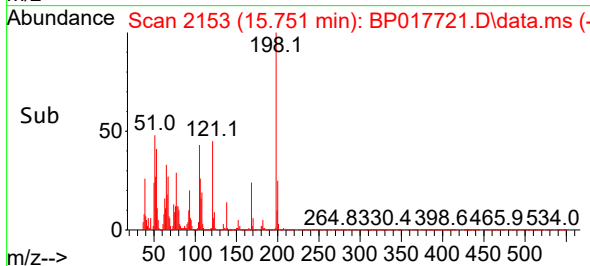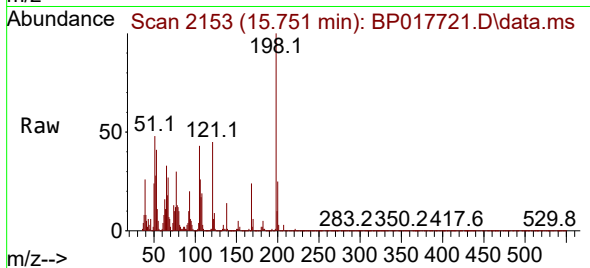

#67
N-Nitrosodiphenylamine
Concen: 21.383 ng/ul
RT: 15.869 min Scan# 2173
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:169 Resp: 394511
Ion Ratio Lower Upper
169 100
168 66.4 53.7 80.5
167 35.7 29.4 44.0


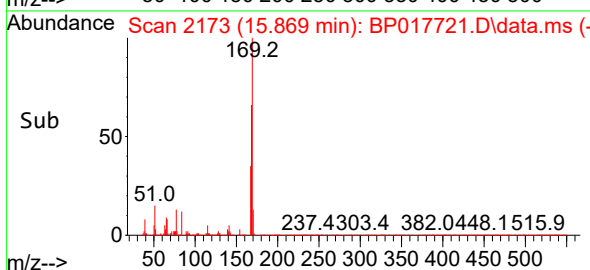

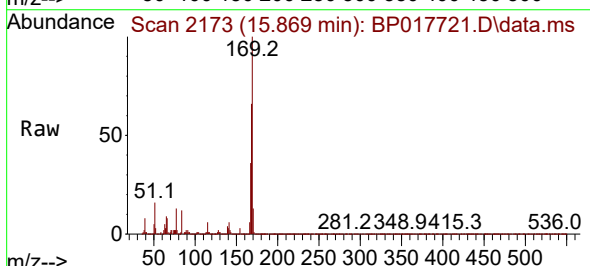




#68
4-Bromophenyl-phenylether
Concen: 18.719 ng/ul
RT: 16.551 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:248 Resp: 133384
Ion Ratio Lower Upper
248 100
250 96.1 76.8 115.2
141 79.0 52.4 78.6#



#69
Hexachlorobenzene
Concen: 17.768 ng/ul
RT: 16.628 min Scan# 2302
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:284 Resp: 145356
Ion Ratio Lower Upper
284 100
142 43.7 27.6 41.4#
249 36.7 24.5 36.7#

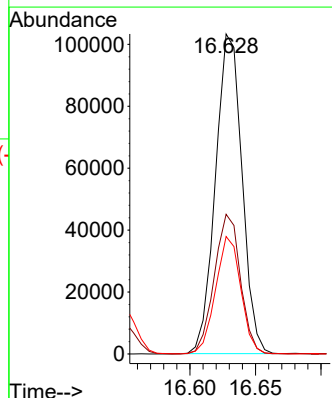



#70

Atrazine

Concen: 19.525 ng/ul

RT: 16.834 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:200 Resp: 132402

Ion Ratio Lower Upper

200 100

173 25.6 19.8 29.6

215 48.7 38.5 57.7

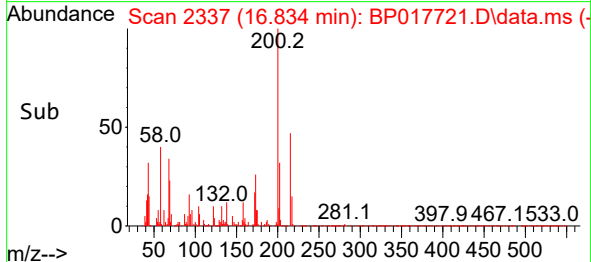

#71

Pentachlorophenol

Concen: 16.512 ng/ul

RT: 17.004 min Scan# 2366

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:266 Resp: 81208


Ion Ratio Lower Upper

266 100

264 59.0 49.4 74.2

268 60.5 50.3 75.5

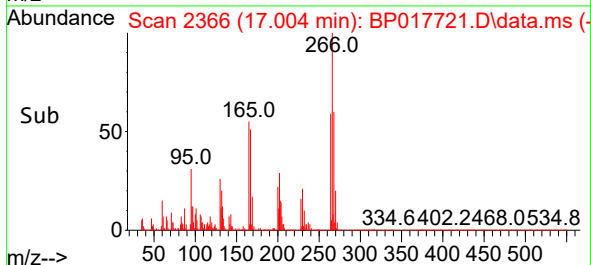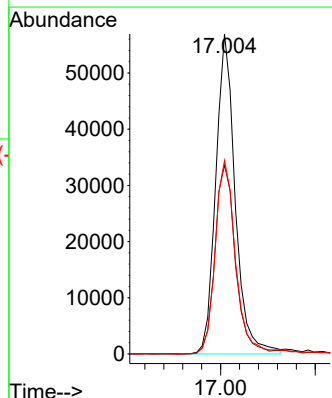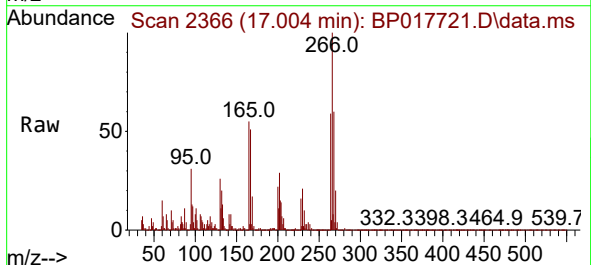



#72

Phenanthrene

Concen: 20.644 ng/ul

RT: 17.422 min Scan# 2437

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:178 Resp: 736491

Ion Ratio Lower Upper

178 100

179 15.4 12.2 18.2

176 18.9 15.3 22.9



#74

Anthracene

Concen: 20.777 ng/ul

RT: 17.516 min Scan# 2453

Delta R.T. 0.006 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:178 Resp: 750729


Ion Ratio Lower Upper

178 100

179 15.0 12.0 18.0

176 19.0 14.8 22.2


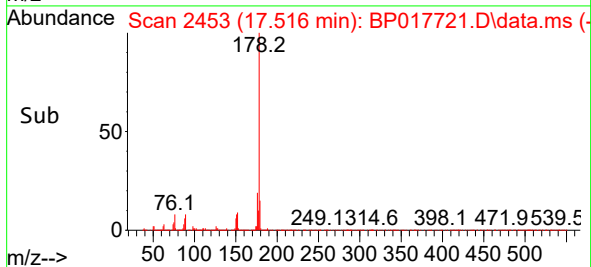

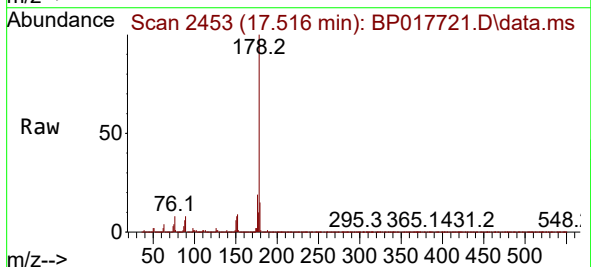


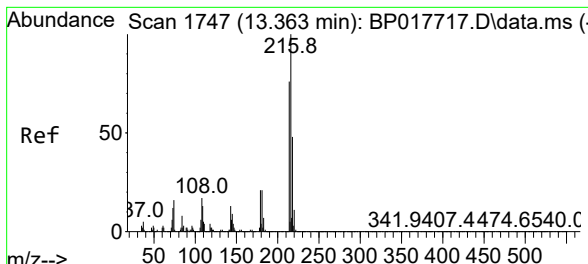

#75
1,2,3,4-Tetrachlorobenzene
Concen: 20.132 ng/uL
RT: 13.363 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:216 Resp: 205721
Ion Ratio Lower Upper
216 100
214 76.7 60.7 91.1
218 46.0 38.2 57.4

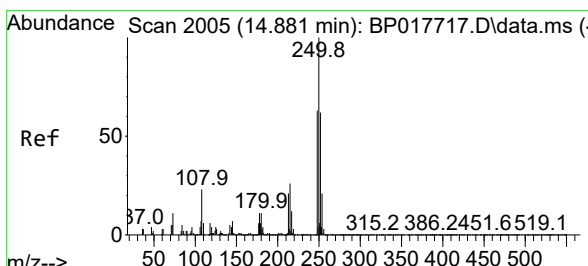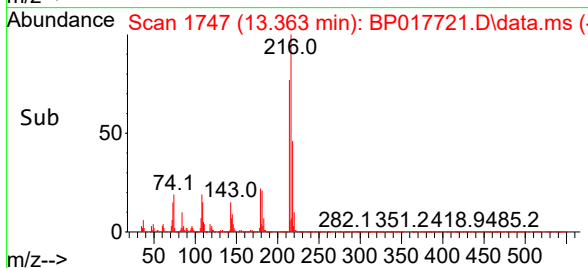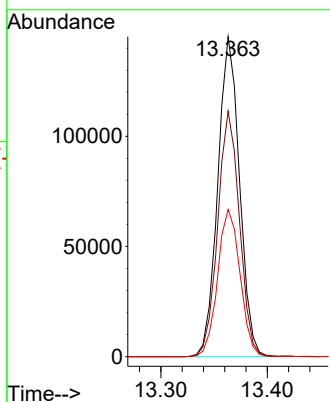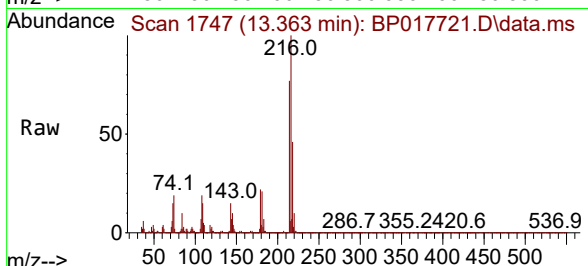

#76
Pentachlorobenzene
Concen: 18.843 ng/uL
RT: 14.881 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:250 Resp: 186608
Ion Ratio Lower Upper
250 100
248 64.2 50.2 75.4
252 63.5 49.6 74.4


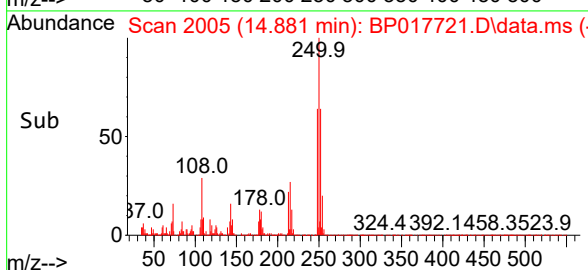

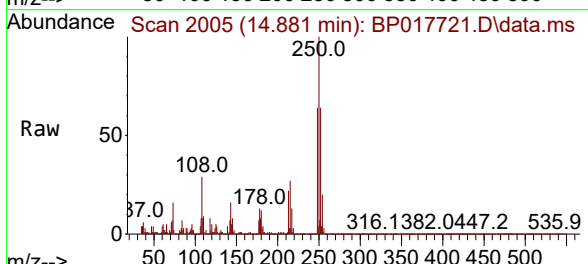




#77
 Carbazole
 Concen: 20.801 ng/ul
 RT: 17.810 min Scan# 2503
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48




Instrument :
 BNA_P
 ClientSampleId :
 SICV602


Tgt Ion:167 Resp: 635228
 Ion Ratio Lower Upper
 167 100
 166 21.1 16.7 25.1
 139 12.9 9.8 14.6

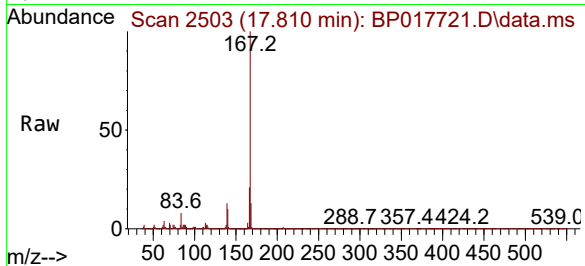

#78
 Di-n-butylphthalate
 Concen: 21.756 ng/ul
 RT: 18.322 min Scan# 2590
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Tgt Ion:149 Resp: 771334
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.2 10.8
 104 5.8 4.3 6.5




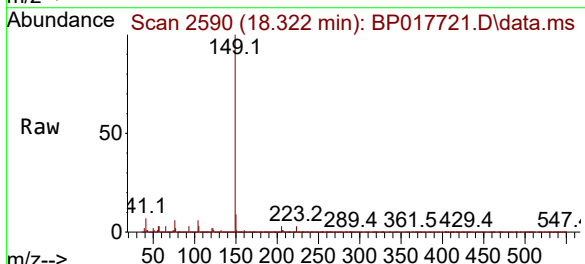




#80
Fluoranthene
Concen: 22.025 ng/ul
RT: 19.404 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48




Instrument :
BNA_P
ClientSampleId :
SICV602


Tgt Ion:202 Resp: 841585
Ion Ratio Lower Upper
202 100
101 10.4 7.1 10.7
100 7.8 5.7 8.5



#82
Pyrene
Concen: 21.626 ng/ul
RT: 19.769 min Scan# 2836
Delta R.T. 0.006 min
Lab File: BP017721.D
Acq: 18 Oct 2023 21:48

Tgt Ion:202 Resp: 875479
Ion Ratio Lower Upper
202 100
101 11.7 8.3 12.5
100 9.8 7.4 11.0

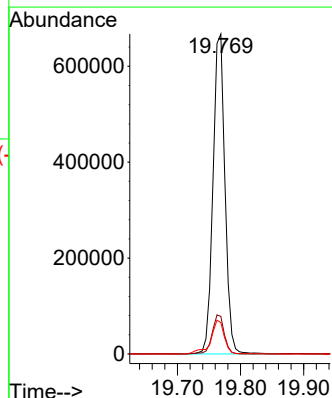



#83

Butylbenzylphthalate

Concen: 23.359 ng/ul

RT: 20.639 min Scan# 2983

Delta R.T. 0.006 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:149 Resp: 325237

Ion Ratio Lower Upper

149 100

91 74.5 58.8 88.2

206 21.6 17.5 26.3

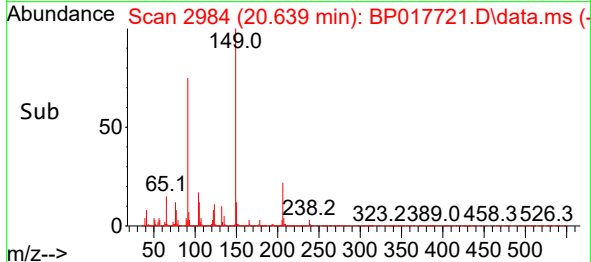

#84

3,3'-Dichlorobenzidine

Concen: 18.832 ng/ul

RT: 21.445 min Scan# 3121

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:252 Resp: 225692


Ion Ratio Lower Upper

252 100

254 64.1 51.8 77.8

126 13.3 7.8 11.6#

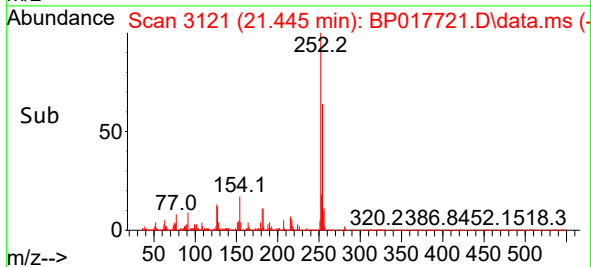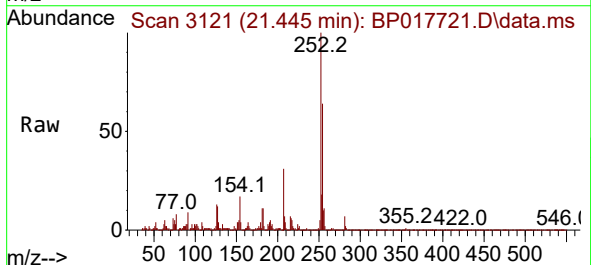



#85

Benzo(a)anthracene

Concen: 20.844 ng/ul

RT: 21.504 min Scan# 3131

Delta R.T. 0.006 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:228 Resp: 840539

Ion Ratio Lower Upper

228 100

229 18.8 15.6 23.4

226 27.1 21.1 31.7



#86

Bis(2-ethylhexyl)phthalate

Concen: 23.635 ng/ul

RT: 21.380 min Scan# 3110

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:149 Resp: 459387


Ion Ratio Lower Upper

149 100

167 26.1 21.6 32.4

279 3.5 3.6 5.4#

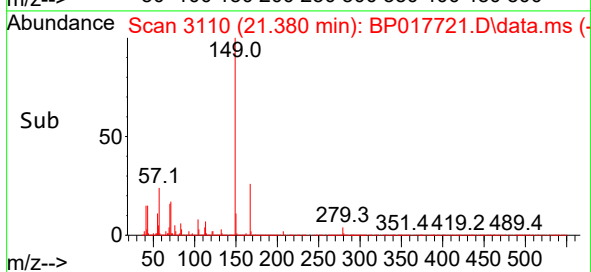

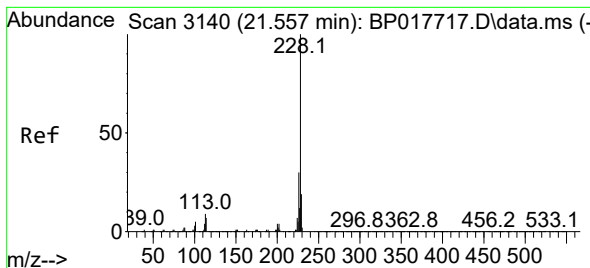

#87

Chrysene

Concen: 20.655 ng/ul

RT: 21.557 min Scan# 3140

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:228 Resp: 787675

Ion Ratio Lower Upper

228 100

226 30.5 24.0 36.0

229 19.3 15.5 23.3

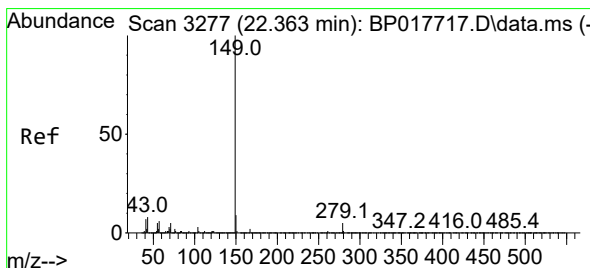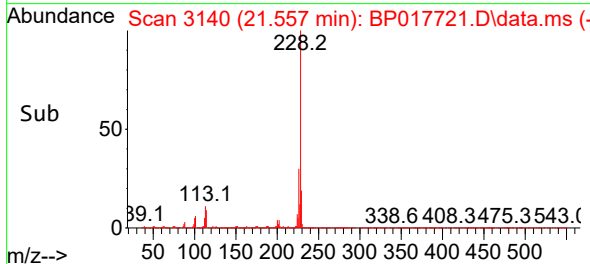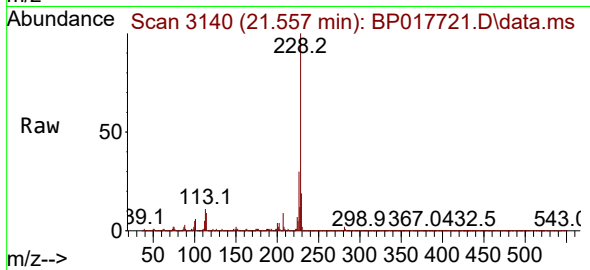

#89

Di-n-octyl phthalate

Concen: 22.666 ng/ul




RT: 22.363 min Scan# 3277


Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Tgt Ion:149 Resp: 778832

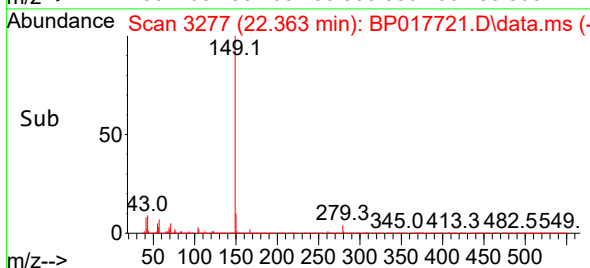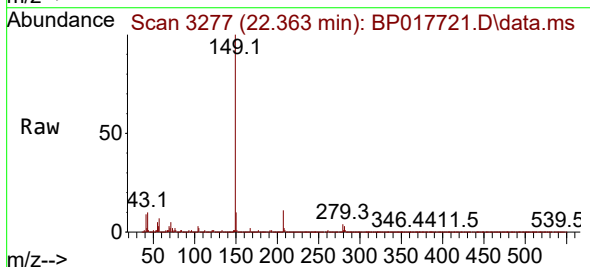



#90

Benzo(b)fluoranthene

Concen: 20.749 ng/ul

RT: 23.274 min Scan# 3432

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:252 Resp: 766027

Ion Ratio Lower Upper

252 100

253 21.4 17.4 26.0

125 10.4 7.1 10.7



#91

Benzo(k)fluoranthene

Concen: 20.490 ng/ul

RT: 23.327 min Scan# 3441

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:252 Resp: 766695


Ion Ratio Lower Upper

252 100

253 22.4 17.5 26.3

125 9.5 7.0 10.6





#93

Benzo(a)pyrene

Concen: 20.839 ng/ul

RT: 23.957 min Scan# 3548

Delta R.T. -0.000 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48

Instrument :

BNA_P

ClientSampleId :

SICV602





Tgt Ion:252 Resp: 722285

Ion Ratio Lower Upper

252 100

253 21.7 17.4 26.2

125 10.9 7.8 11.6

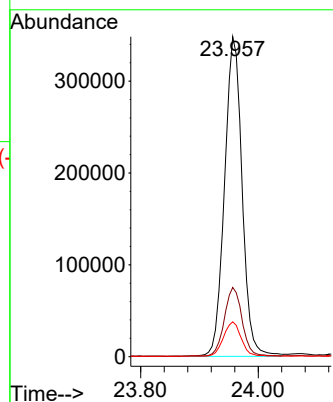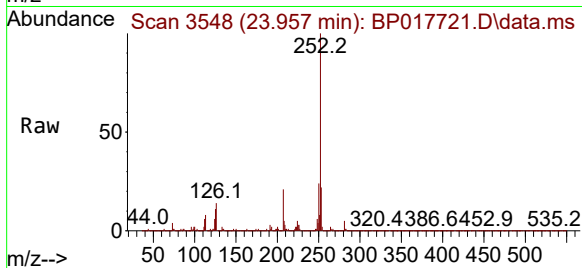

#94

Indeno(1,2,3-cd)pyrene

Concen: 19.692 ng/ul

RT: 26.786 min Scan# 4029

Delta R.T. 0.006 min

Lab File: BP017721.D

Acq: 18 Oct 2023 21:48




Tgt Ion:276 Resp: 813451


Ion Ratio Lower Upper

276 100

138 23.9 15.6 23.4#

277 24.0 19.4 29.2



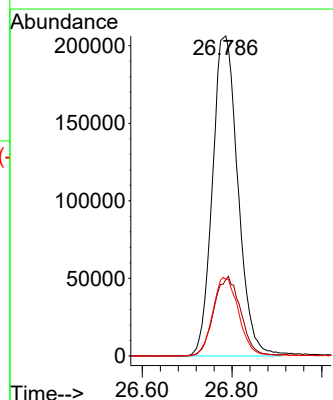
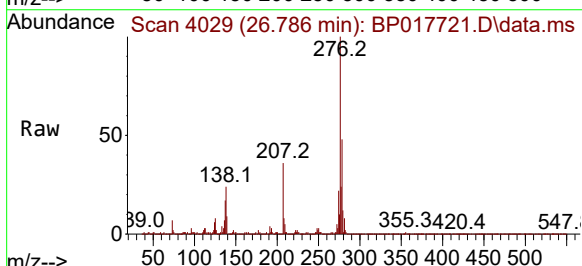




#95
 Dibenzo(a,h)anthracene
 Concen: 19.443 ng/ul
 RT: 26.809 min Scan# 4033
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Instrument :
 BNA_P
 ClientSampleId :
 SICV602

Tgt Ion:278 Resp: 670127
 Ion Ratio Lower Upper
 278 100
 139 16.8 11.4 17.2
 279 23.9 18.8 28.2



#96
 Benzo(g,h,i)perylene
 Concen: 19.568 ng/ul
 RT: 27.627 min Scan# 4172
 Delta R.T. -0.000 min
 Lab File: BP017721.D
 Acq: 18 Oct 2023 21:48

Tgt Ion:276 Resp: 651285
 Ion Ratio Lower Upper
 276 100
 138 22.5 15.0 22.6
 277 23.3 18.5 27.7

