

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
 Data File : BP017730.D
 Acq On : 19 Oct 2023 15:15
 Operator : MA/JU
 Sample : 04864-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJV6

Quant Time: Oct 20 00:45:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	109702	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	442057	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	268066	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.375	188	584700	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.522	240	516654	20.000	ng/ul	0.00
88) Perylene-d12	24.074	264	530597	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	14262	4.836	ng/uL	0.00
4) Pyridine-d5	3.699	84	106738	13.825	ng/ul	0.00
7) Phenol-d5	7.052	99	81446	8.922	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	226090	40.103	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	221646	29.769	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	143242	19.981	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	129941	36.276	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	143729	36.316	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	244965	31.553	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	174871	17.211	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	849858	37.766	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	933081	37.181	ng/ul	0.00
54) 4-Nitrophenol-d4	14.851	143	18862	5.883	ng/ul	0.02
60) Fluorene-d10	15.592	176	726410	37.343	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	114896	29.833	ng/ul	0.00
73) Anthracene-d10	17.475	188	1105463	36.997	ng/ul	0.00
81) Pyrene-d10	19.733	212	1304626	40.277	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.904	264	1110798	37.587	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.140	77	86658	9.716	ng/ul	98
78) Di-n-butylphthalate	18.322	149	3843718	112.921	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017730.D
Acq On : 19 Oct 2023 15:15
Operator : MA/JU
Sample : 04864-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCJV6

Quant Time: Oct 20 00:45:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration




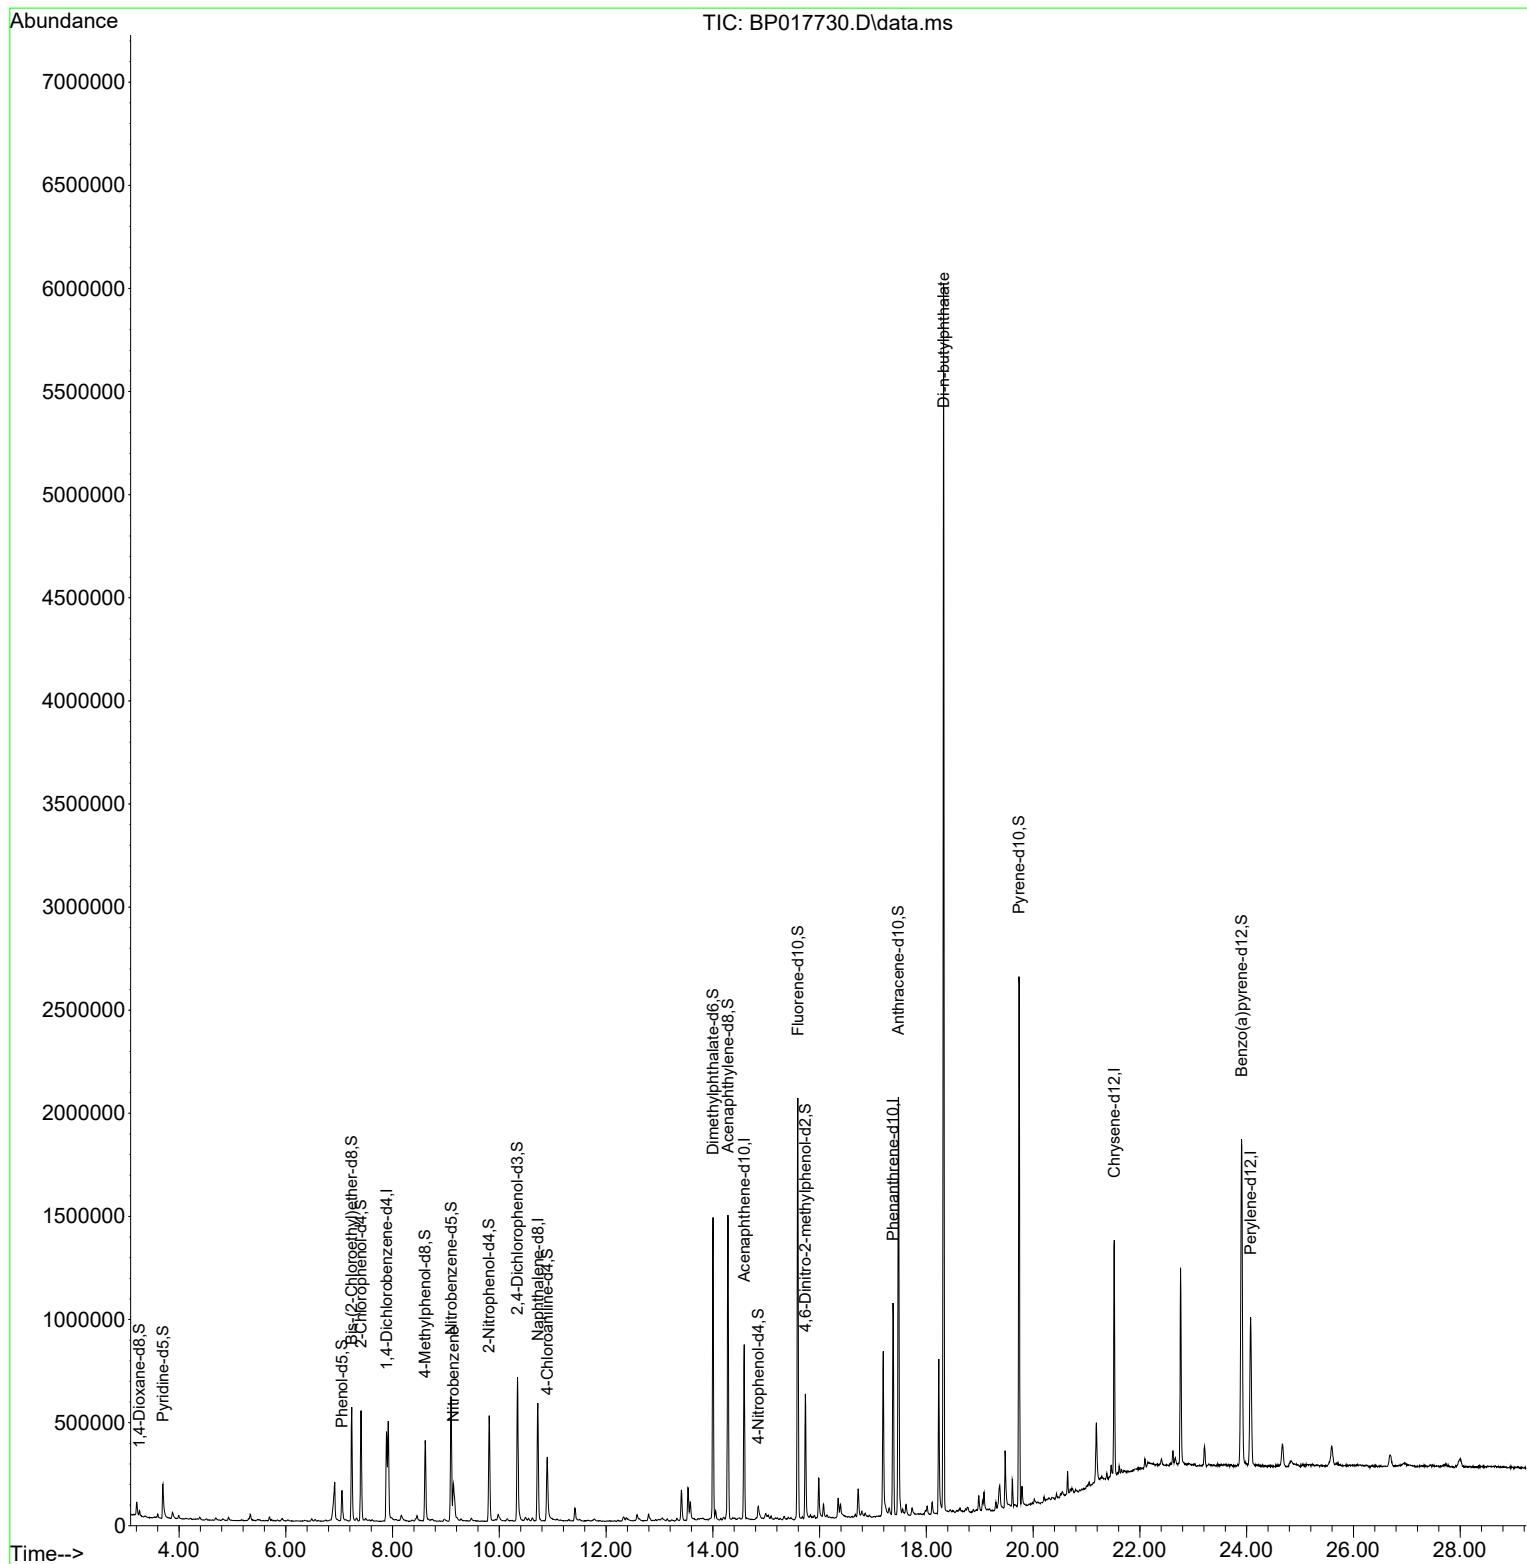


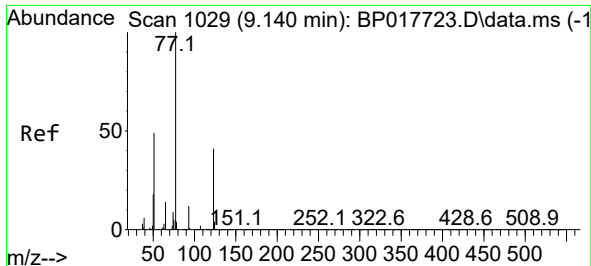

#22
Nitrobenzene
Concen: 9.716 ng/ul
RT: 9.140 min Scan# 1029
Delta R.T. -0.000 min
Lab File: BP017730.D
Acq: 19 Oct 2023 15:15

Instrument :
BNA_P
ClientSampleId :
DCJV6

Tgt Ion: 77 Resp: 86658
Ion Ratio Lower Upper
77 100
123 40.7 33.5 50.3
65 12.5 10.8 16.2

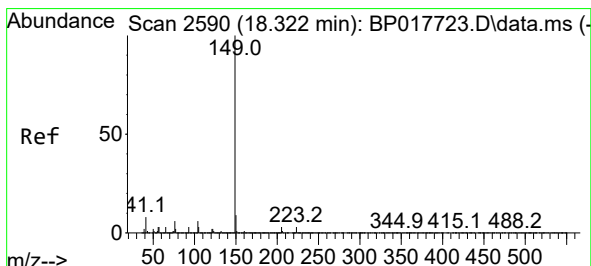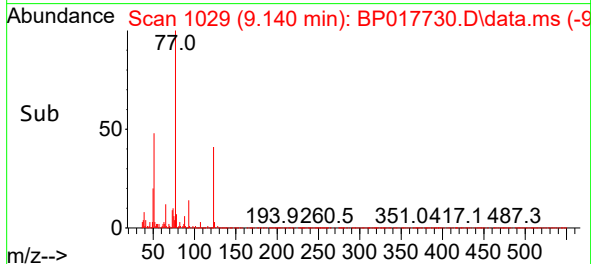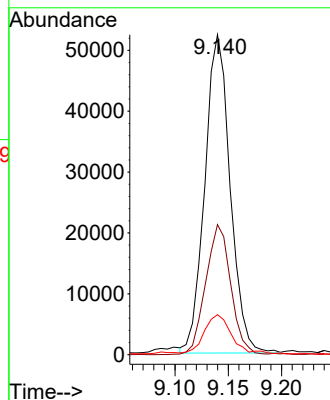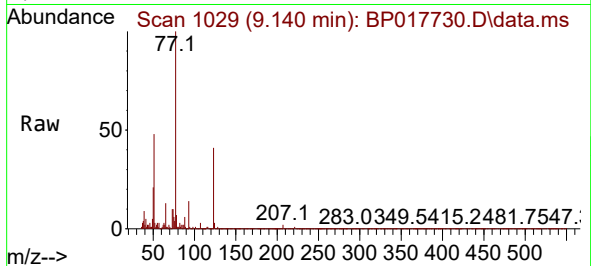

#78
Di-n-butylphthalate
Concen: 112.921 ng/ul
RT: 18.322 min Scan# 2590
Delta R.T. -0.000 min
Lab File: BP017730.D
Acq: 19 Oct 2023 15:15

Tgt Ion: 149 Resp: 3843718
Ion Ratio Lower Upper
149 100
150 9.4 7.2 10.8
104 6.1 4.3 6.5

