




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
 Data File : BP017731.D
 Acq On : 19 Oct 2023 16:57
 Operator : MA/JU
 Sample : 04824-01 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JYCA4

Manual IntegrationsAPPROVED

Quant Time: Oct 20 00:45:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/20/2023
 Supervised By :mohammad ahmed 10/20/2023

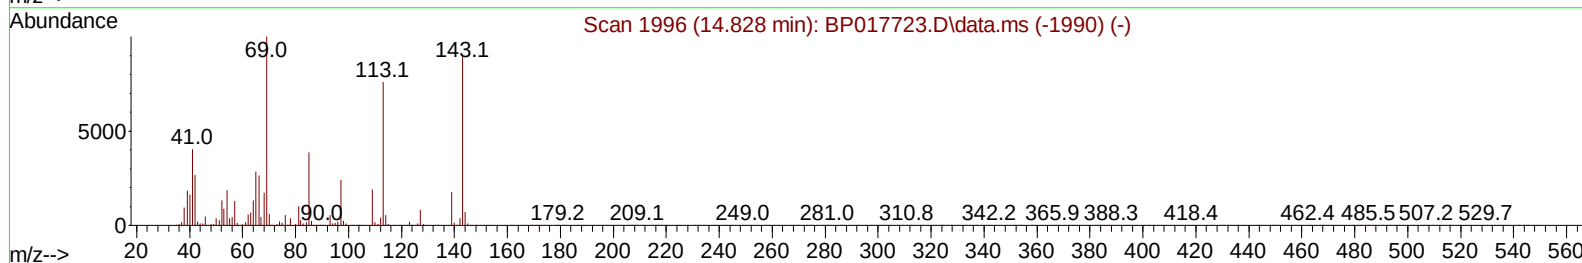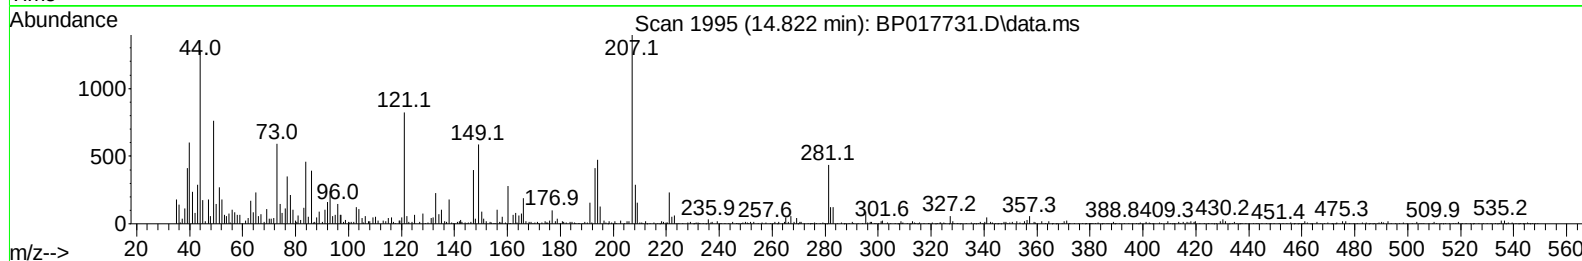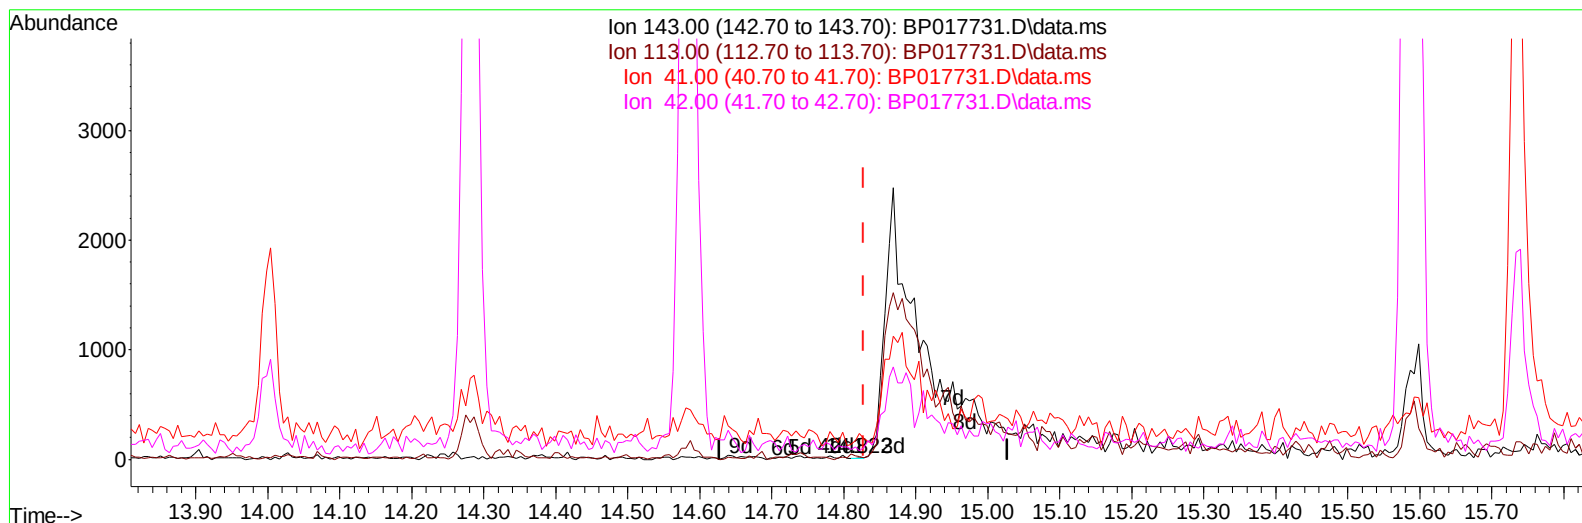

TIC: BP017731.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.822min (-0.006) 0.00 ng/ul

response 3

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.70	200.00#
41.00	39.20	1838.46#
42.00	25.60	607.69#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017731.D
Acq On : 19 Oct 2023 16:57
Operator : MA/JU
Sample : 04824-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JYCA4

Manual IntegrationsAPPROVED

Quant Time: Oct 20 00:45:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/20/2023
Supervised By :mohammad ahmed 10/20/2023

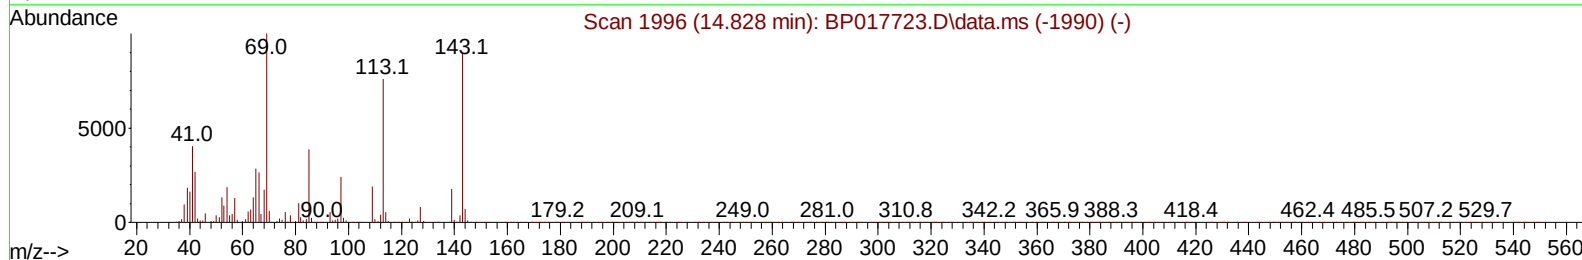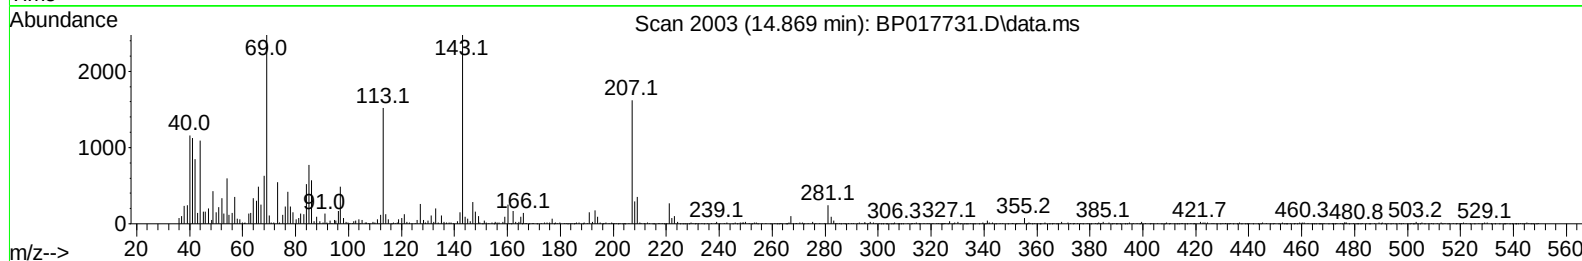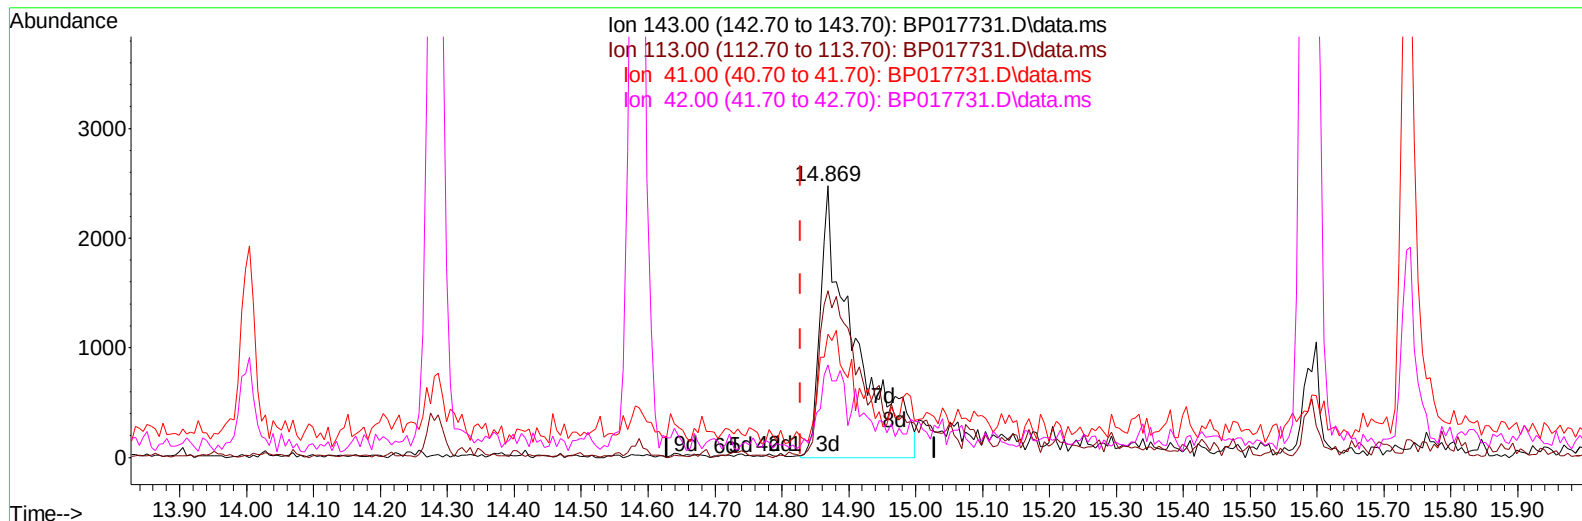

TIC: BP017731.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (+ 0.041) 2.29 ng/ul m

response 8828

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.70	61.51#
41.00	39.20	45.48
42.00	25.60	34.17#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
 Data File : BP017731.D
 Acq On : 19 Oct 2023 16:57
 Operator : MA/JU
 Sample : 04824-01 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JYCA4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/20/2023
 Supervised By :mohammad ahmed 10/20/2023

Quant Time: Oct 20 01:05:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 19 01:32:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	139087	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	539522	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	322149	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.375	188	678786	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.522	240	566353	20.000	ng/ul	0.00
88) Perylene-d12	24.074	264	588405	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	7408	1.981	ng/uL	0.00
4) Pyridine-d5	3.699	84	89502	9.143	ng/ul	0.00
7) Phenol-d5	7.052	99	54985	4.751	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	209915	29.367	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	189715	20.097	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	105629	11.621	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	119594	27.356	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	125798	26.043	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	206195	21.761	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	241559	19.480	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	756737	27.982	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	818421	27.137	ng/ul	0.00
54) 4-Nitrophenol-d4	14.869	143	8828m	2.291	ng/ul	0.04
60) Fluorene-d10	15.592	176	635861	27.200	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.740	200	81729	18.279	ng/ul	0.00
73) Anthracene-d10	17.475	188	997506	28.757	ng/ul	0.00
81) Pyrene-d10	19.733	212	1130383	31.835	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.904	264	964865	29.441	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017731.D
Acq On : 19 Oct 2023 16:57
Operator : MA/JU
Sample : 04824-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JYCA4

Manual IntegrationsAPPROVED

Quant Time: Oct 20 01:05:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 19 01:32:15 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/20/2023
Supervised By :mohammad ahmed 10/20/2023

