

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
 Data File : BP017726.D
 Acq On : 19 Oct 2023 12:24
 Operator : MA/JU
 Sample : PB156344TB 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	41713	55963	1.51%	0.157%
2	3.646	93	95	99	rBV5	2825	4452	0.12%	0.013%
3	3.693	99	103	125	rVV	395370	714107	19.29%	2.007%
4	3.993	151	154	159	rVB3	6650	10689	0.29%	0.030%
5	4.223	190	193	201	rVB4	13609	19651	0.53%	0.055%
6	4.640	261	264	270	rVB6	8084	13230	0.36%	0.037%
7	6.352	552	555	560	rBV7	2486	5236	0.14%	0.015%
8	6.617	598	600	605	rVB6	4986	6063	0.16%	0.017%
9	6.687	607	612	613	rBV5	4016	5656	0.15%	0.016%
10	7.046	665	673	686	rBV	585806	979699	26.46%	2.753%
11	7.234	698	705	717	rBV	514701	785469	21.22%	2.207%
12	7.411	726	735	750	rBV	649820	1075454	29.05%	3.022%
13	7.887	809	816	828	rBV	477766	752782	20.33%	2.116%
14	8.611	932	939	954	rBV	697455	1166092	31.50%	3.277%
15	9.099	1015	1022	1037	rBV	564219	952294	25.72%	2.676%
16	9.810	1134	1143	1159	rBV	477307	819539	22.14%	2.303%
17	10.340	1226	1233	1259	rBV	670404	1238754	33.46%	3.481%
18	10.722	1290	1298	1308	rBV	592650	985678	26.63%	2.770%
19	10.893	1320	1327	1346	rBV	556251	1099800	29.71%	3.091%
20	11.440	1416	1420	1426	rBV8	3032	5987	0.16%	0.017%
21	12.334	1567	1572	1575	rBV3	8154	15553	0.42%	0.044%
22	13.428	1753	1758	1762	rVB6	8105	12065	0.33%	0.034%
23	13.551	1775	1779	1785	rVB9	3606	5926	0.16%	0.017%
24	14.004	1849	1856	1870	rBV	1353491	1859350	50.23%	5.225%
25	14.287	1897	1904	1920	rBV	1444090	2144989	57.94%	6.028%
26	14.587	1948	1955	1967	rBV	896068	1281093	34.61%	3.600%
27	14.834	1990	1997	2021	rBV	234542	612572	16.55%	1.721%
28	15.593	2119	2126	2144	rBV	1973593	2784725	75.22%	7.826%
29	15.740	2144	2151	2163	rVV	484625	742822	20.07%	2.088%
30	15.840	2163	2168	2175	rVB6	10627	21801	0.59%	0.061%
31	17.045	2368	2373	2375	rBV6	2965	3846	0.10%	0.011%
32	17.381	2423	2430	2437	rBV	1085792	1526849	41.24%	4.291%
33	17.481	2440	2447	2461	rBV	2116665	2917608	78.81%	8.199%
34	18.234	2572	2575	2585	rBV	7538	15773	0.43%	0.044%
35	19.245	2745	2747	2751	rBV4	3974	5509	0.15%	0.015%
36	19.304	2754	2757	2762	rVV2	25121	33414	0.90%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017726.D
Acq On : 19 Oct 2023 12:24
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	19.381	2766	2770	2775	rVB	55739	70731	1.91%	0.199%
38	19.486	2784	2788	2791	rBV6	9619	16860	0.46%	0.047%
39	19.616	2806	2810	2816	rBV	134500	143504	3.88%	0.403%
40	19.739	2825	2831	2841	rBV	2674729	3522482	95.15%	9.899%
41	20.439	2947	2950	2955	rVB6	17704	20078	0.54%	0.056%
42	20.645	2982	2985	2990	rBV2	93154	102528	2.77%	0.288%
43	21.522	3129	3134	3144	rBV	1148196	1628568	43.99%	4.577%
44	23.904	3531	3539	3554	rBV2	1741011	3702024	100.00%	10.404%
45	24.074	3562	3568	3579	rVB	814317	1696506	45.83%	4.768%




Sum of corrected areas: 35583771

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017726.D
Acq On : 19 Oct 2023 12:24
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

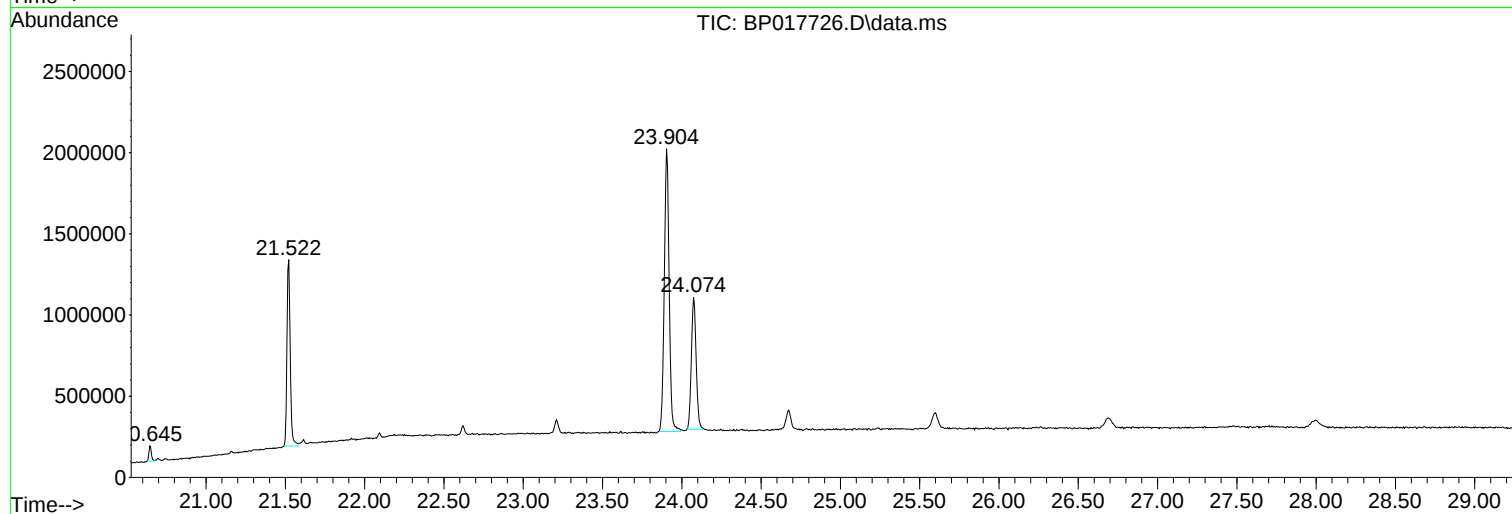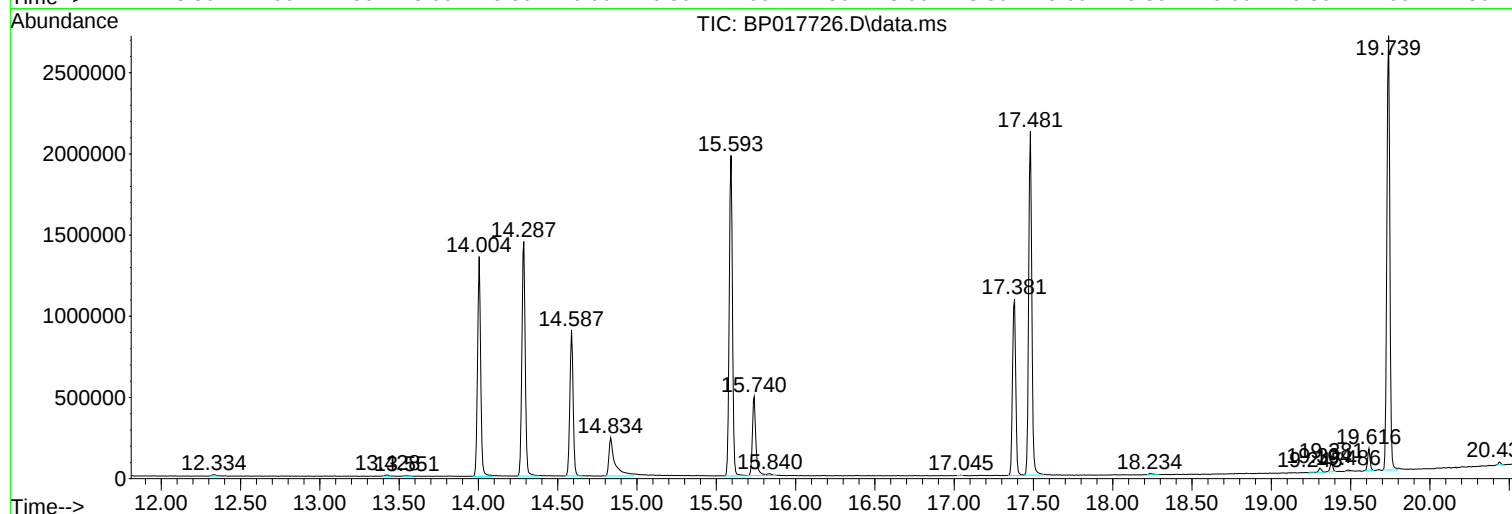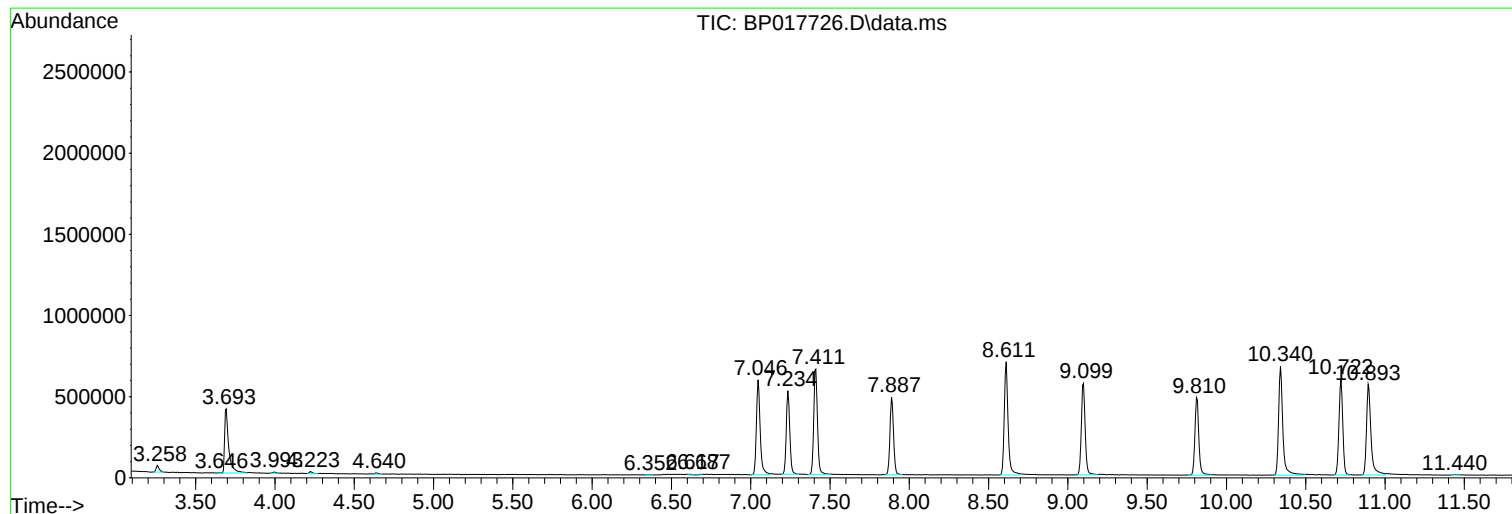

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017726.D
Acq On : 19 Oct 2023 12:24
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101923\
Data File : BP017726.D
Acq On : 19 Oct 2023 12:24
Operator : MA/JU
Sample : PB156344TB 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB344

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc