

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
 Data File : BP017738.D
 Acq On : 20 Oct 2023 11:37
 Operator : MA/JU
 Sample : PB156394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK394

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rBV	47524	61972	1.90%	0.177%
2	3.693	99	103	121	rBV	492753	907155	27.80%	2.587%
3	4.005	152	156	161	rBV3	9469	14066	0.43%	0.040%
4	4.228	192	194	198	rVB4	10519	11944	0.37%	0.034%
5	4.640	262	264	271	rVB6	7287	10195	0.31%	0.029%
6	6.752	620	623	629	rVB6	3074	4317	0.13%	0.012%
7	7.058	668	675	691	rBV	636297	1072721	32.87%	3.059%
8	7.246	700	707	718	rBV	566714	868803	26.62%	2.478%
9	7.416	729	736	748	rBV	747107	1175413	36.02%	3.352%
10	7.899	811	818	826	rVV	493469	784671	24.04%	2.238%
11	8.622	934	941	956	rBV	747860	1285568	39.39%	3.666%
12	9.105	1016	1023	1034	rBV	639475	1037794	31.80%	2.960%
13	9.281	1050	1053	1056	rVB5	3102	3346	0.10%	0.010%
14	9.458	1081	1083	1087	rBV4	2368	3653	0.11%	0.010%
15	9.822	1138	1145	1158	rBV	532889	878558	26.92%	2.506%
16	10.352	1228	1235	1246	rBV	726413	1288297	39.48%	3.674%
17	10.728	1290	1299	1308	rBV	624008	1042205	31.94%	2.972%
18	10.905	1320	1329	1347	rBV	694240	1256639	38.51%	3.584%
19	12.334	1567	1572	1579	rBV4	11547	20890	0.64%	0.060%
20	13.263	1724	1730	1734	rBV7	1737	4215	0.13%	0.012%
21	13.434	1754	1759	1765	rVB7	6824	11154	0.34%	0.032%
22	13.551	1775	1779	1783	rVB7	2173	3685	0.11%	0.011%
23	13.722	1803	1808	1811	rBV6	2436	4823	0.15%	0.014%
24	13.775	1815	1817	1828	rVB6	3430	9153	0.28%	0.026%
25	14.016	1851	1858	1866	rBV	1339122	1865118	57.15%	5.319%
26	14.293	1898	1905	1916	rBV	1524698	2215346	67.88%	6.318%
27	14.598	1950	1957	1968	rVV	896455	1320556	40.46%	3.766%
28	14.681	1968	1971	1975	rVB6	2240	3799	0.12%	0.011%
29	14.787	1984	1989	1991	rBV6	2185	3429	0.11%	0.010%
30	14.845	1993	1999	2018	rBV	282419	690379	21.15%	1.969%
31	15.222	2060	2063	2068	rVB7	2977	3753	0.12%	0.011%
32	15.298	2071	2076	2078	rBV6	1936	3447	0.11%	0.010%
33	15.381	2084	2090	2095	rBV3	7129	12559	0.38%	0.036%
34	15.604	2119	2128	2146	rBV	1905753	2748259	84.21%	7.838%
35	15.745	2146	2152	2165	rVV	537534	780894	23.93%	2.227%
36	15.845	2165	2169	2178	rVV6	13939	31403	0.96%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
 Data File : BP017738.D
 Acq On : 20 Oct 2023 11:37
 Operator : MA/JU
 Sample : PB156394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK394

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

37	16.192	2225	2228	2232	rBV6	2536	3965	0.12%	0.011%
38	16.457	2267	2273	2277	rBV8	3366	5442	0.17%	0.016%
39	16.651	2302	2306	2310	rBV3	5658	8065	0.25%	0.023%
40	17.051	2371	2374	2378	rVV6	4139	5951	0.18%	0.017%
41	17.269	2408	2411	2412	rBV3	4828	4335	0.13%	0.012%
42	17.387	2424	2431	2442	rBV	1063766	1509979	46.27%	4.306%
43	17.492	2442	2449	2466	rVV	1924097	2780417	85.20%	7.930%
44	17.739	2487	2491	2495	rBV5	5244	7062	0.22%	0.020%
45	17.981	2526	2532	2533	rBV6	1822	3631	0.11%	0.010%
46	18.028	2535	2540	2543	rBV7	5320	8511	0.26%	0.024%
47	18.245	2574	2577	2582	rBV5	12026	18587	0.57%	0.053%
48	18.651	2644	2646	2652	rVB5	5212	8934	0.27%	0.025%
49	18.798	2667	2671	2674	rVB6	7504	10770	0.33%	0.031%
50	19.316	2756	2759	2764	rVB2	23334	28792	0.88%	0.082%
51	19.386	2768	2771	2778	rVV	24469	35149	1.08%	0.100%
52	19.498	2786	2790	2794	rBV7	8660	16742	0.51%	0.048%
53	19.628	2809	2812	2816	rBV5	11572	13185	0.40%	0.038%
54	19.751	2827	2833	2842	rBV	2451377	3263455	100.00%	9.307%
55	21.533	3131	3136	3146	rBV	1027464	1443842	44.24%	4.118%
56	23.927	3536	3543	3560	rVB2	1399187	3017683	92.47%	8.606%
57	24.098	3565	3572	3583	rVB	685818	1428771	43.78%	4.075%




Sum of corrected areas: 35063447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017738.D
Acq On : 20 Oct 2023 11:37
Operator : MA/JU
Sample : PB156394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

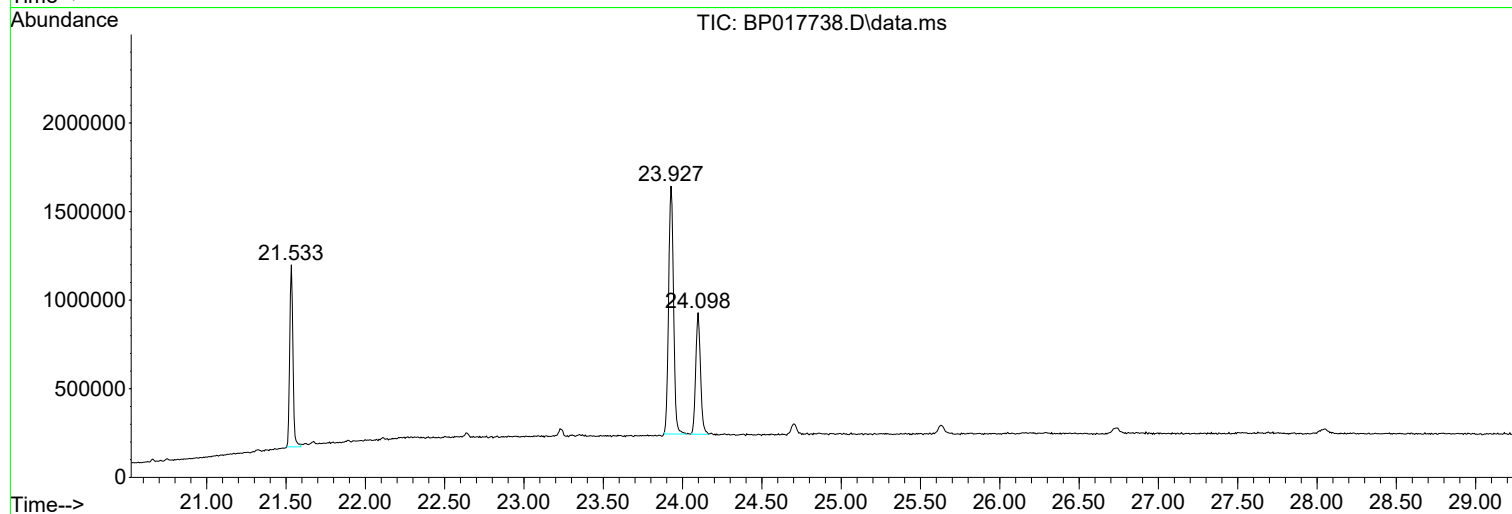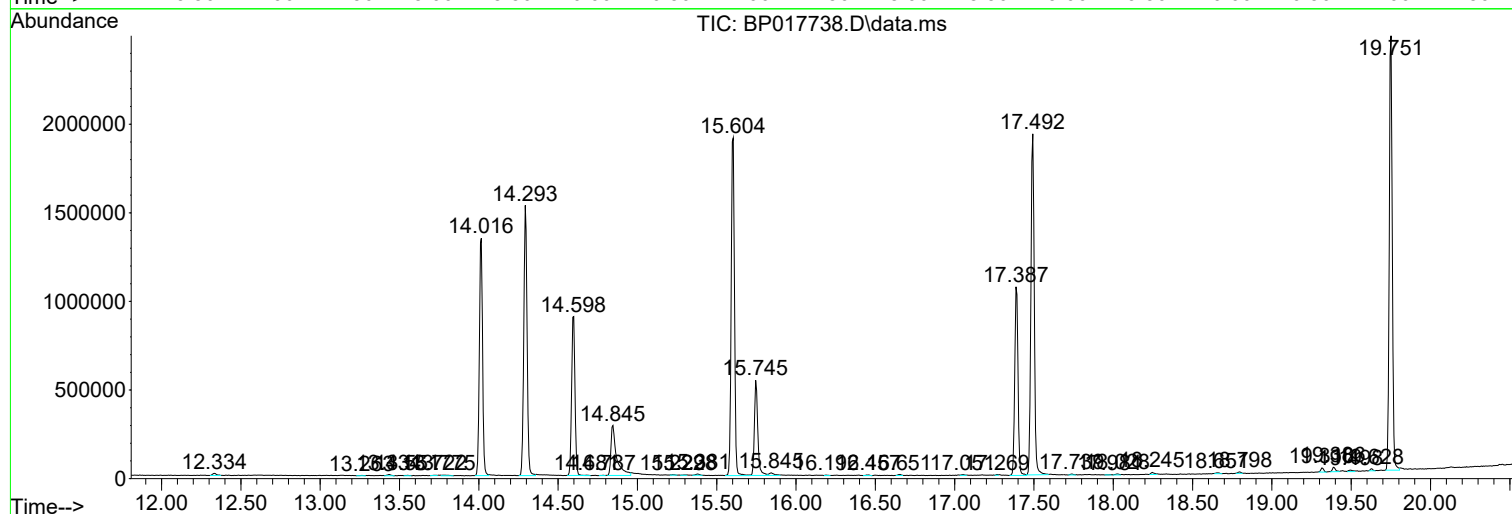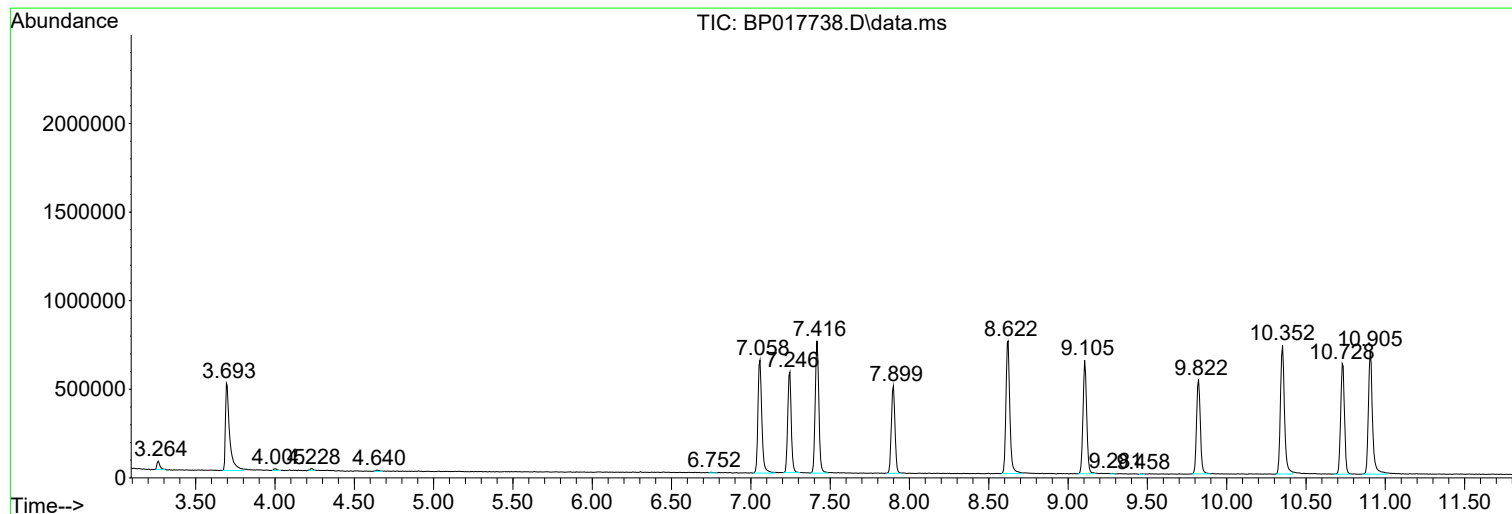

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017738.D
Acq On : 20 Oct 2023 11:37
Operator : MA/JU
Sample : PB156394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017738.D
Acq On : 20 Oct 2023 11:37
Operator : MA/JU
Sample : PB156394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------