

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
 Data File : BP017740.D
 Acq On : 20 Oct 2023 12:45
 Operator : MA/JU
 Sample : PB156398BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK398

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	36	rVB	42498	57811	2.02%	0.192%
2	3.693	99	103	128	rBV	433433	782235	27.27%	2.604%
3	4.222	190	193	197	rVB4	8415	11599	0.40%	0.039%
4	4.646	261	265	270	rBV4	5349	8634	0.30%	0.029%
5	6.858	639	641	646	rVB5	2943	3084	0.11%	0.010%
6	7.046	667	673	687	rBV	541693	894173	31.17%	2.977%
7	7.234	698	705	713	rBV	479739	745172	25.97%	2.481%
8	7.405	728	734	745	rBV	608149	986116	34.37%	3.283%
9	7.887	808	816	826	rBV	428493	673378	23.47%	2.242%
10	8.610	930	939	957	rBV	643689	1105159	38.52%	3.680%
11	9.093	1014	1021	1036	rBV	531942	888698	30.98%	2.959%
12	9.810	1134	1143	1156	rBV	450582	759058	26.46%	2.527%
13	10.340	1223	1233	1252	rBV	593980	1085773	37.85%	3.615%
14	10.716	1290	1297	1305	rBV	512124	866033	30.19%	2.883%
15	10.893	1319	1327	1349	rBV	577614	1080167	37.65%	3.596%
16	11.363	1404	1407	1411	rVB6	2242	3832	0.13%	0.013%
17	12.187	1542	1547	1549	rBV5	1878	2959	0.10%	0.010%
18	12.328	1565	1571	1575	rBV3	7695	15482	0.54%	0.052%
19	13.416	1754	1756	1762	rVB7	5031	8610	0.30%	0.029%
20	13.545	1774	1778	1782	rBV7	2394	3892	0.14%	0.013%
21	14.004	1849	1856	1865	rBV	1185028	1609762	56.11%	5.360%
22	14.281	1896	1903	1919	rBV	1292938	1890420	65.89%	6.294%
23	14.587	1946	1955	1968	rBV	776456	1122393	39.12%	3.737%
24	14.834	1990	1997	2018	rBV	221271	558992	19.48%	1.861%
25	15.592	2118	2126	2144	rBV	1670142	2388173	83.24%	7.952%
26	15.734	2144	2150	2162	rVV	433402	654315	22.81%	2.179%
27	15.834	2164	2167	2175	rVB7	10145	19068	0.66%	0.063%
28	17.039	2369	2372	2378	rVB8	3537	5169	0.18%	0.017%
29	17.257	2406	2409	2412	rBV5	3031	4118	0.14%	0.014%
30	17.375	2423	2429	2440	rBV	934130	1297022	45.21%	4.318%
31	17.481	2440	2447	2459	rBV	1652286	2411572	84.06%	8.029%
32	17.810	2499	2503	2506	rBV5	2825	4875	0.17%	0.016%
33	18.239	2573	2576	2583	rVB8	4415	7069	0.25%	0.024%
34	18.786	2664	2669	2672	rBV7	5092	8969	0.31%	0.030%
35	19.304	2753	2757	2763	rBV3	19899	26671	0.93%	0.089%
36	19.380	2766	2770	2774	rVV	18553	25247	0.88%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017740.D
Acq On : 20 Oct 2023 12:45
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK398

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Title : SVOA CALIBRATION

37	19.616	2807	2810	2813	rBV4	10127	10002	0.35%	0.033%
38	19.739	2825	2831	2847	rBV	2181876	2868895	100.00%	9.552%
39	21.522	3129	3134	3146	rBV	878765	1262708	44.01%	4.204%
40	23.904	3532	3539	3555	rVB2	1283129	2666874	92.96%	8.879%
41	24.074	3562	3568	3578	rVB	567734	1209925	42.17%	4.029%




Sum of corrected areas: 30034104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017740.D
Acq On : 20 Oct 2023 12:45
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

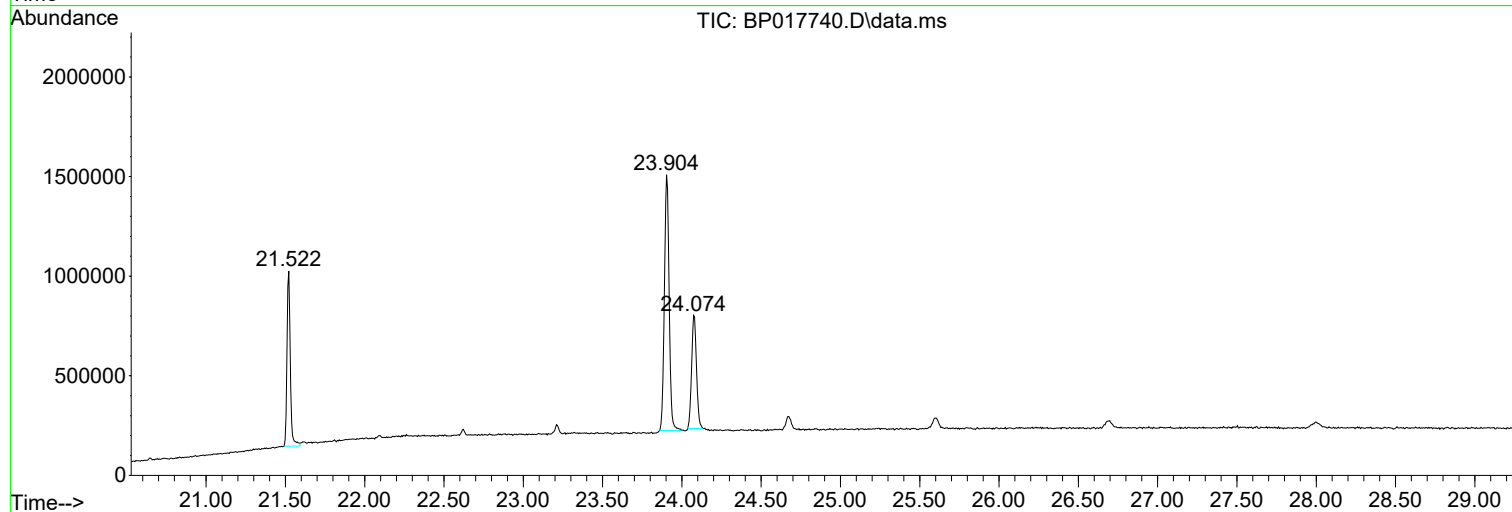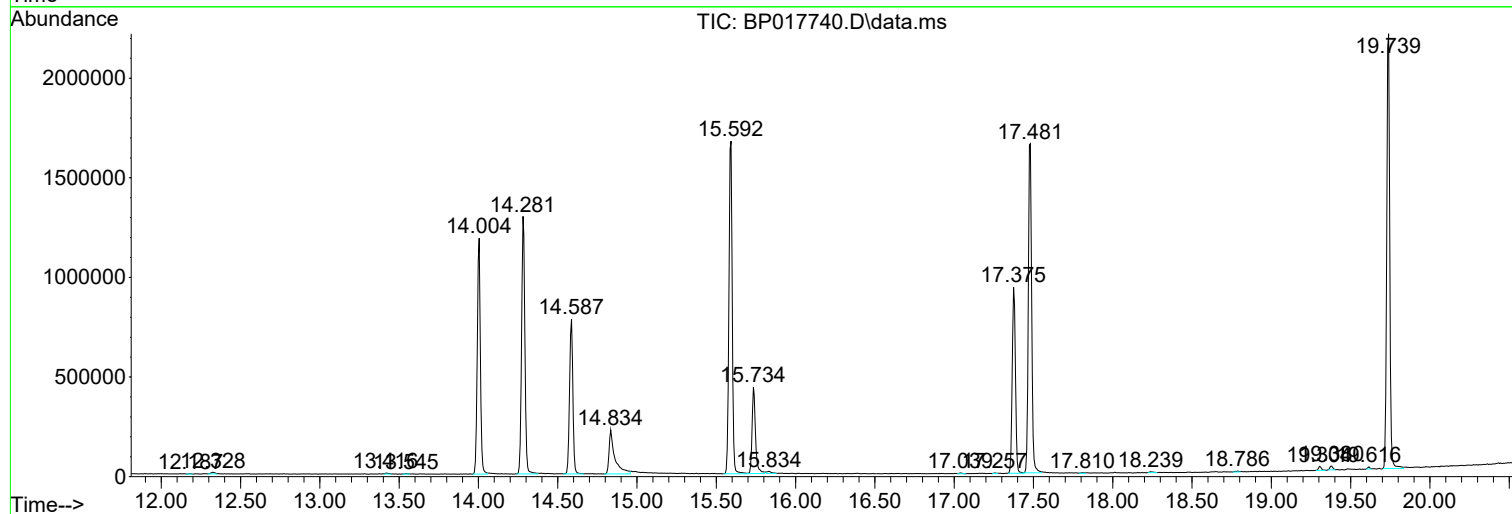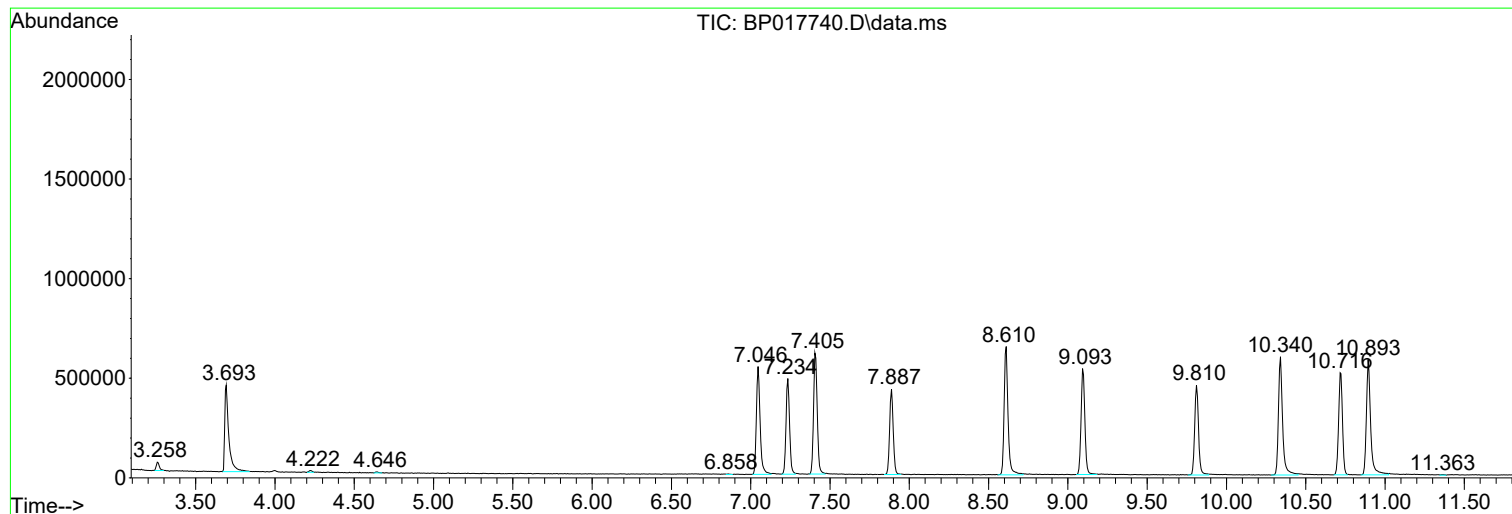

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017740.D
Acq On : 20 Oct 2023 12:45
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102023\
Data File : BP017740.D
Acq On : 20 Oct 2023 12:45
Operator : MA/JU
Sample : PB156398BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------