

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP102119\
 Data File : BP000931.D
 Acq On : 21 Oct 2019 13:12
 Operator : JU
 Sample : K5308-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 X2J20

Manual Integrations
 APPROVED

mohammad
 10/22/2019 3:28:36 PM

Quant Time: Oct 21 14:14:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 19 22:14:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	119966	20.00	ng/ul	0.00
18) Naphthalene-d8	8.02	136	446611	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.79	164	256611	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	500056	20.00	ng/ul	0.00
78) Chrysene-d12	13.96	240	466702	20.00	ng/ul	0.00
86) Perylene-d12	15.44	264	509997	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.34	96	18321	6.34	ng/uL	0.00
5) Phenol-d5	6.39	99	319036	34.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.42	67	158134	34.18	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	281304	36.08	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	254688	36.02	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	132811	39.12	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	150194	41.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	262517	37.94	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	190260	24.73	ng/ul	0.00
44) Dimethylphthalate-d6	9.48	166	727597	40.50	ng/ul	0.00
47) Acenaphthylene-d8	9.63	160	843746	38.18	ng/ul	0.00
52) 4-Nitrophenol-d4	9.92	143	109885	39.71	ng/ul	0.00
58) Fluorene-d10	10.31	176	597355	38.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	85564	35.93	ng/ul	0.00
71) Anthracene-d10	11.35	188	891887	38.51	ng/ul	0.00
79) Pyrene-d10	12.73	212	974749	36.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.35	264	1020897	40.55	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.40	94	292567	31.361	ng/ul 98
11) 2-Methylphenol	7.00	108	267013	36.864	ng/ul 98
48) Acenaphthylene	9.65	152	503334	22.075	ng/ul 99
50) Acenaphthene	9.82	153	355512	22.525	ng/ul 98
54) Dibenzofuran	9.99	168	587798	26.759	ng/ul 99
57) Diethylphthalate	10.21	149	638178	36.919	ng/ul 98
59) Fluorene	10.34	166	387657	22.710	ng/ul 100
65) N-Nitrosodiphenylamine	10.45	169	652208	40.891	ng/ul 99
68) Atrazine	11.00	200	345273	63.783	ng/ul 97
69) Pentachlorophenol	11.10	266	189574	78.567	ng/ul 98
72) Anthracene	11.36	178	409816	14.818	ng/ul 99
76) Di-n-butylphthalate	11.86	149	810644	28.627	ng/ul 100
81) Butylbenzylphthalate	13.37	149	474188	35.043	ng/ul 99
87) Di-n-octyl phthalate	14.57	149	1016070	34.750	ng/ul 100
88) Benzo(b)fluoranthene	15.02	252	1157214m	38.030	ng/ul
89) Benzo(k)fluoranthene	15.04	252	1005904	34.714	ng/ul 99
91) Benzo(a)pyrene	15.38	252	977119	33.916	ng/ul 98
92) Indeno(1,2,3-cd)pyrene	16.92	276	1264094	38.278	ng/ul 96
93) Dibenzo(a,h)anthracene	16.92	278	651766	24.077	ng/ul 97
94) Benzo(g,h,i)perylene	17.36	276	1065840	38.764	ng/ul 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP102119\
Data File : BP000931.D
Acq On : 21 Oct 2019 13:12
Operator : JU
Sample : K5308-02
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
X2J20

Manual Integrations
APPROVED

mohammad
10/22/2019 3:28:36 PM

Quant Time: Oct 21 14:14:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 19 22:14:11 2019
Response via : Initial Calibration

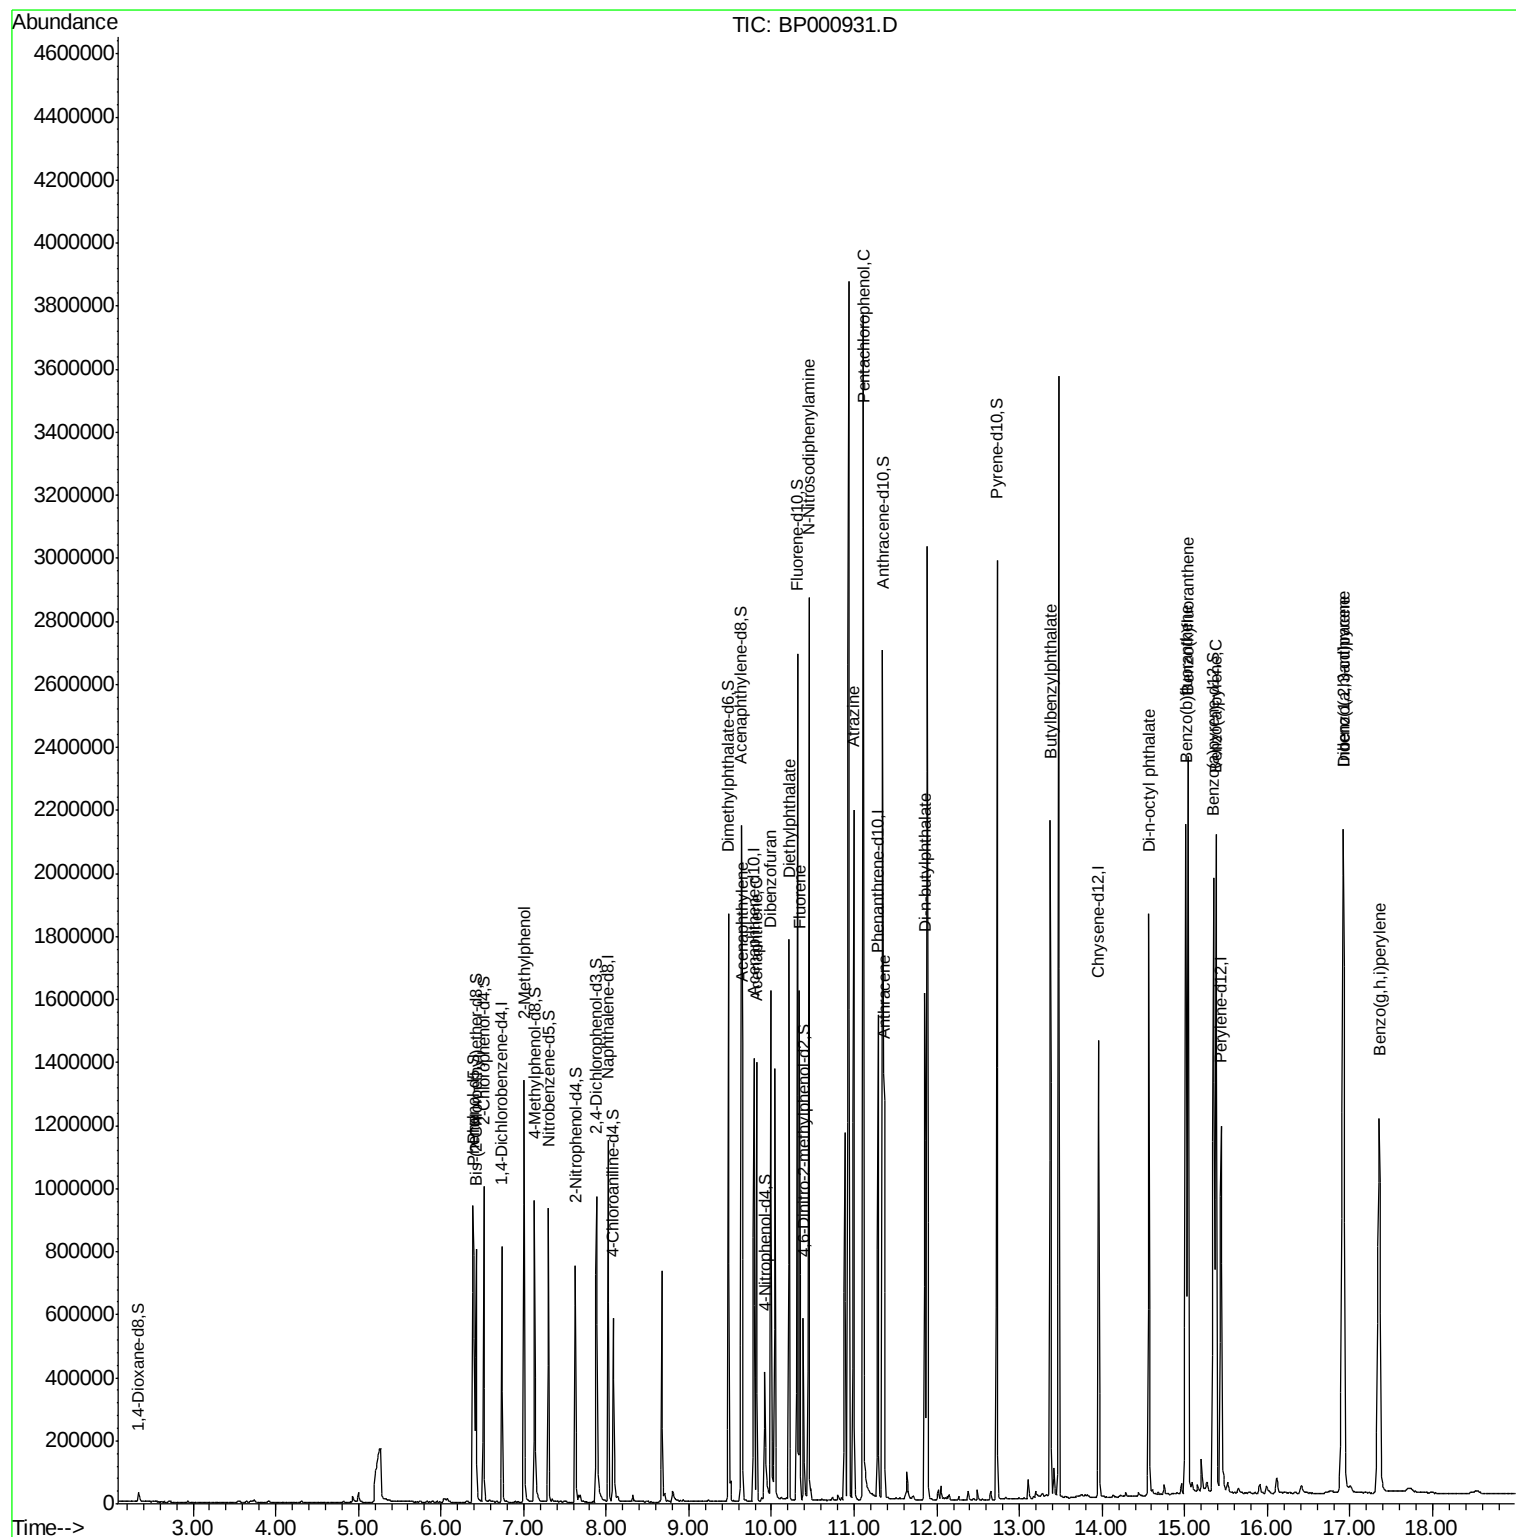

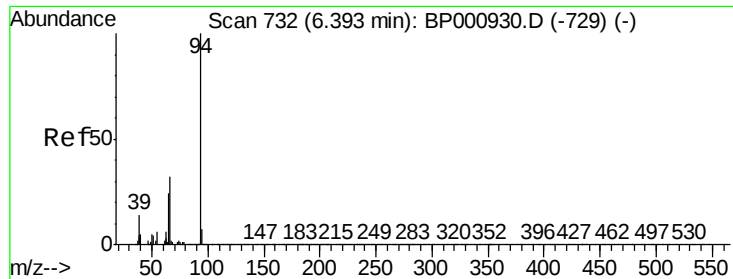

#6

Phenol

Concen: 31.361 ng/ul

RT: 6.40 min Scan# 733

Delta R.T. 0.00 min

Lab File: BP000931.D

Acq: 21 Oct 2019 13:12

Instrument :

BNA_P





ClientSampleId :

X2J20

Tot Ion:	94	Resp:	292567
Ion Ratio	Lower	Upper	
94	100		
65	23.2	19.2	28.8
66	33.2	25.7	38.5

Manual Integrations
APPROVED

mohammad
10/22/2019 3:28:36 PM

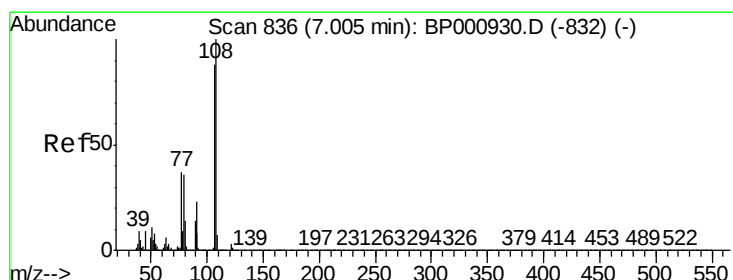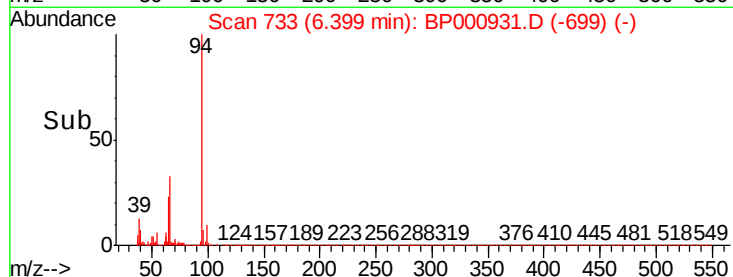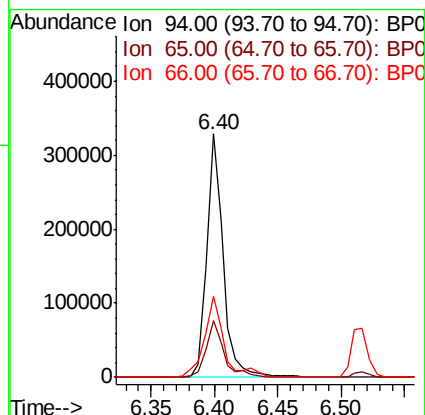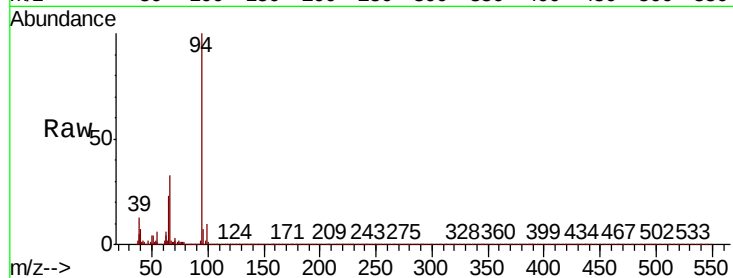

#11

2-Methylphenol

Concen: 36.864 ng/ul




RT: 7.00 min Scan# 836


Delta R.T. 0.00 min

Lab File: BP000931.D

Acq: 21 Oct 2019 13:12

Tgt Ion:	108	Resp:	267013
Ion Ratio	Lower	Upper	
108	100		
107	90.6	71.1	106.7

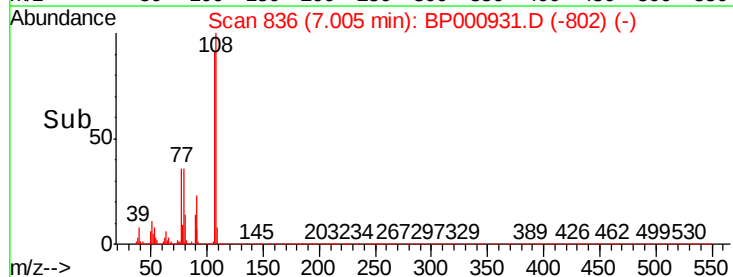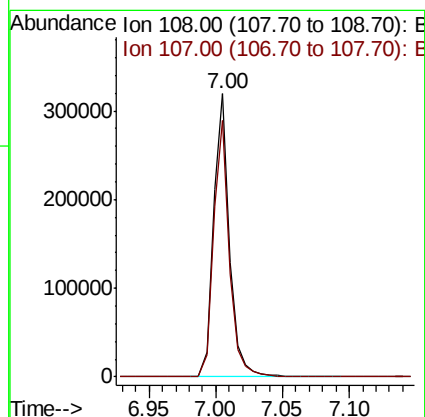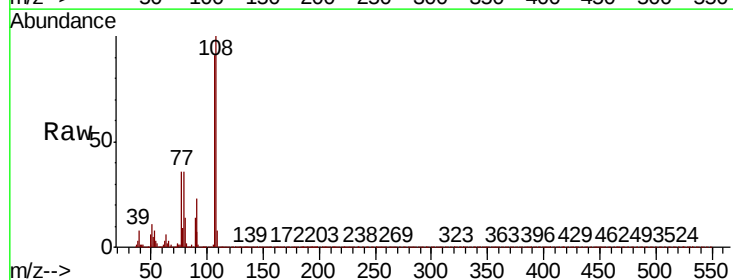

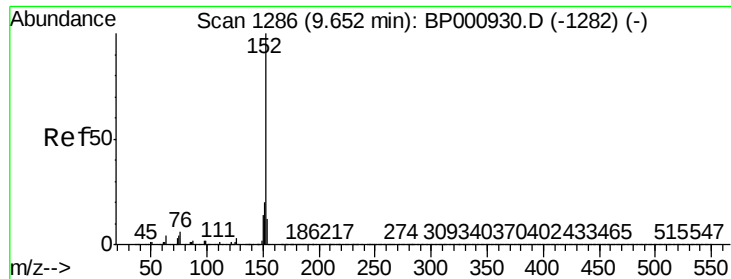





#48
Acenaphthylene
Concen: 22.075 ng/ul
RT: 9.65 min Scan# 1285
Delta R.T. -0.01 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampleId :
X2J20

Tot Ion	Ion	Ratio	Resp	Lower	Upper
152	100		503334		
151	20.8	16.2		24.4	
153	13.4	10.9		16.3	




Manual Integrations
APPROVED


mohammad
10/22/2019 3:28:36 PM

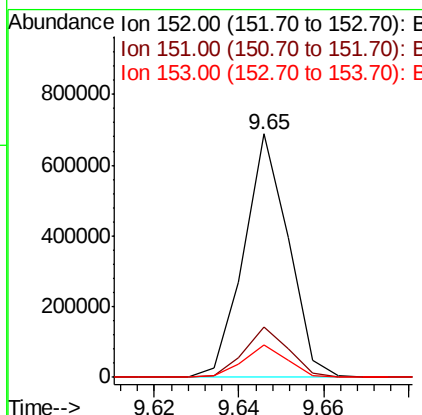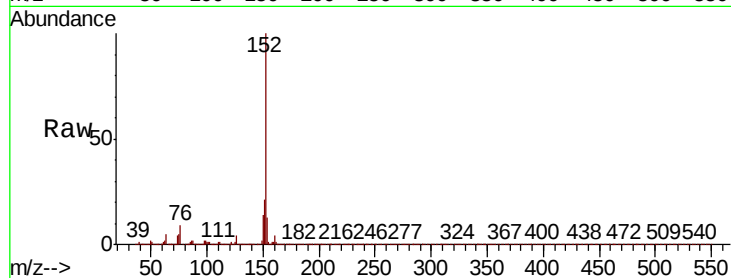

#50
Acenaphthene
Concen: 22.525 ng/ul
RT: 9.82 min Scan# 1315
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
153	100		355512		
152	47.0	38.6		57.8	
154	88.5	71.9		107.9	

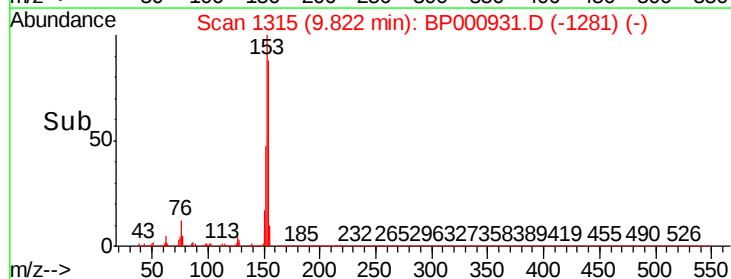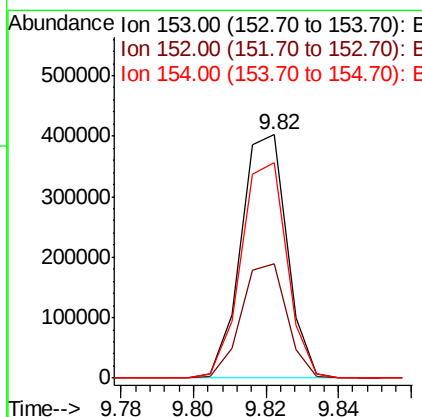

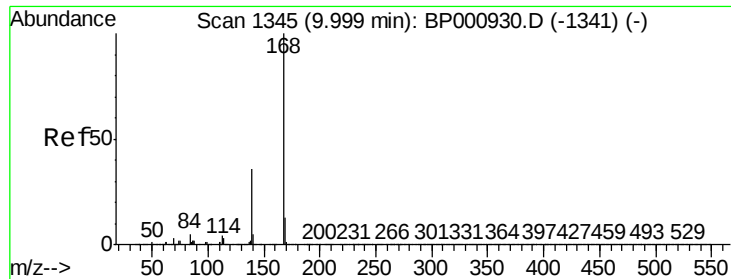





#54
Dibenzofuran
Concen: 26.759 ng/ul
RT: 9.99 min Scan# 1344
Delta R.T. -0.01 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampleId :
X2J20

Tot Ion	Ratio	Lower	Upper
168	100		
139	36.8	29.8	44.6




Manual Integrations
APPROVED


mohammad
10/22/2019 3:28:36 PM

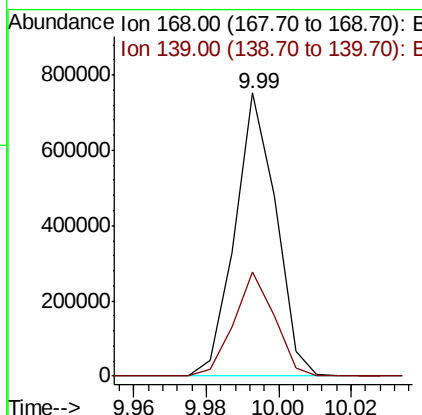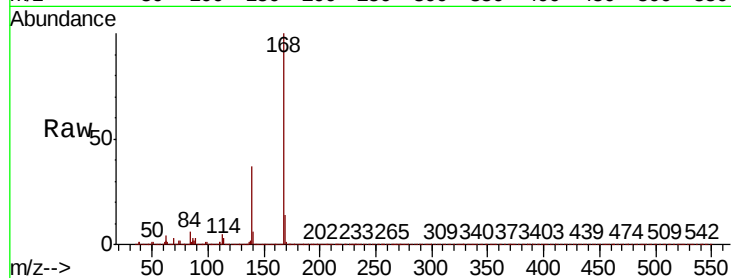

#57
Diethylphthalate
Concen: 36.919 ng/ul
RT: 10.21 min Scan# 1381
Delta R.T. -0.01 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Lower	Upper
149	100		
177	22.5	19.0	28.4
150	12.8	9.8	14.8

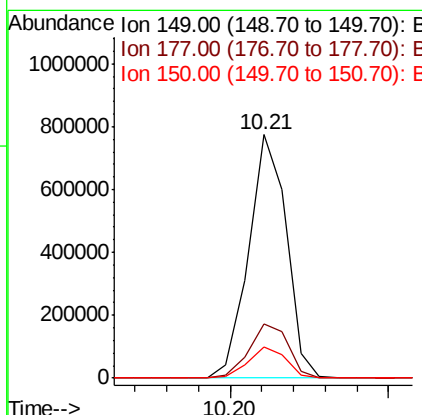

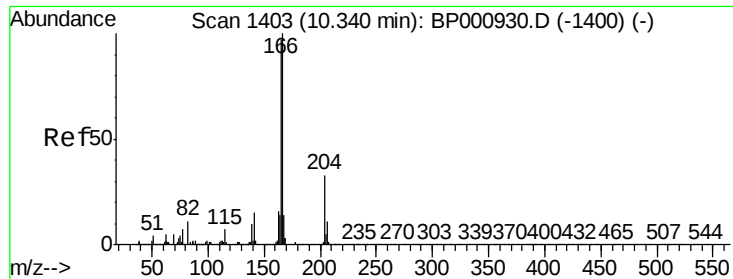





#59
Fluorene
 Concen: 22.710 ng/ul
 RT: 10.34 min Scan# 1403
 Delta R.T. 0.00 min
 Lab File: BP000931.D
 Acq: 21 Oct 2019 13:12

Instrument :
 BNA_P
 ClientSampleId :
 X2J20

Tot Ion	Ratio	Lower	Upper
166	100		
165	96.6	77.4	116.0
167	13.2	10.8	16.2




Manual Integrations
 APPROVED


mohammad
 10/22/2019 3:28:36 PM

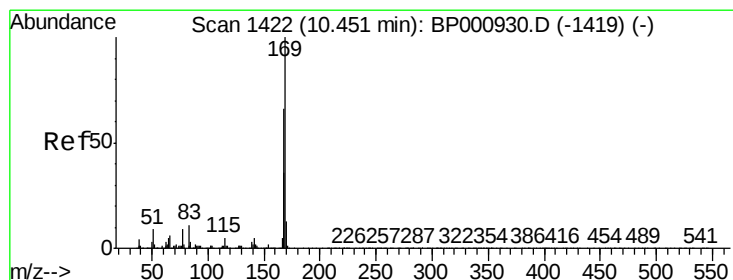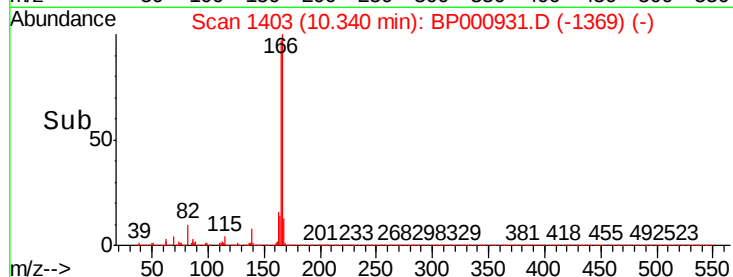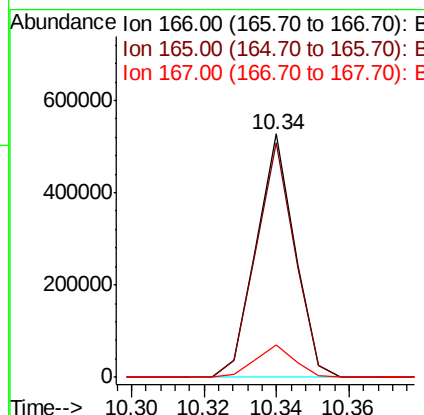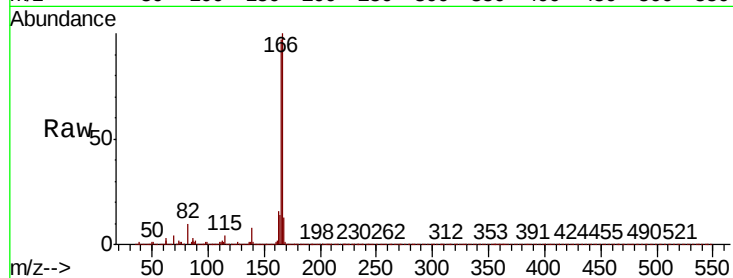

#65
N-Nitrosodiphenylamine
 Concen: 40.891 ng/ul
 RT: 10.45 min Scan# 1422
 Delta R.T. 0.00 min
 Lab File: BP000931.D
 Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Lower	Upper
169	100		
168	66.6	52.4	78.6
167	36.1	28.6	42.8

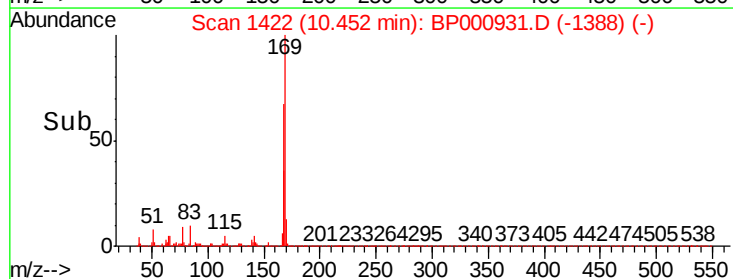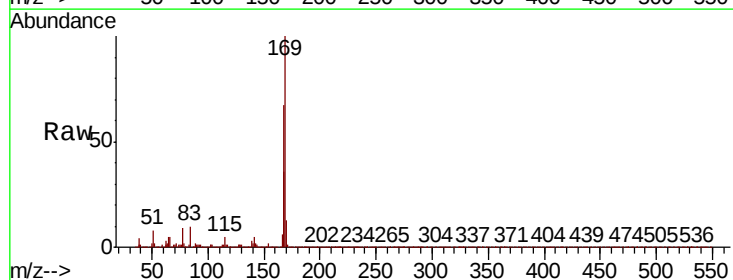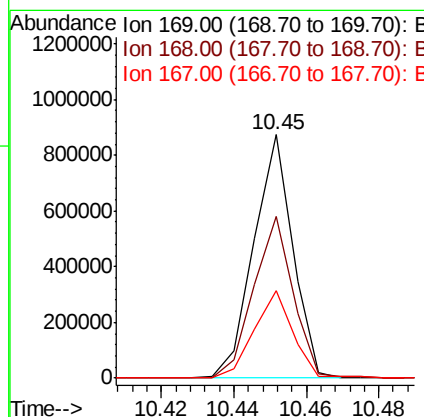

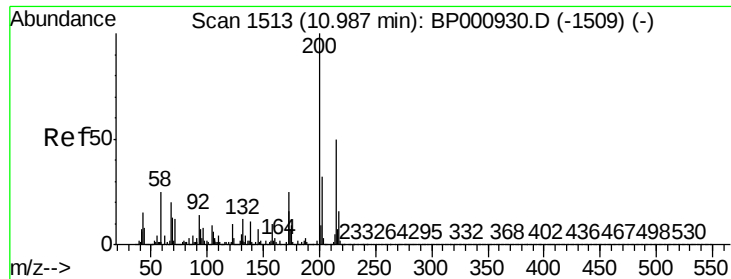





#68
Atrazine
Concen: 63.783 ng/ul
RT: 11.00 min Scan# 1515
Delta R.T. 0.01 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampleId :
X2J20

Tot Ion	Ratio	Resp Lower	Resp Upper
200	100		
173	25.6	22.0	33.0
215	49.5	38.5	57.7




Manual Integrations
APPROVED


mohammad
10/22/2019 3:28:36 PM

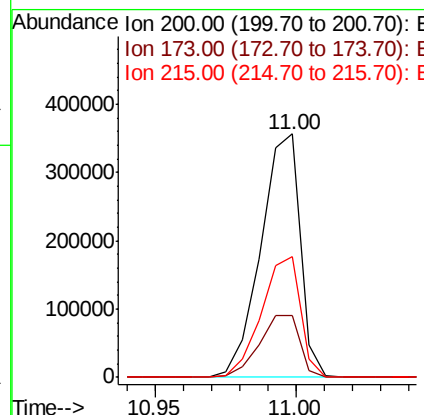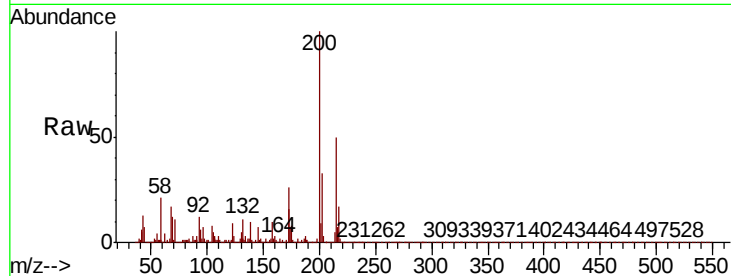

#69
Pentachlorophenol
Concen: 78.567 ng/ul
RT: 11.10 min Scan# 1533
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Resp Lower	Resp Upper
266	100		
264	63.0	49.6	74.4
268	64.4	49.6	74.4

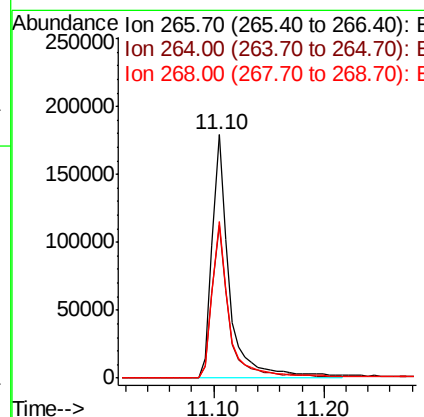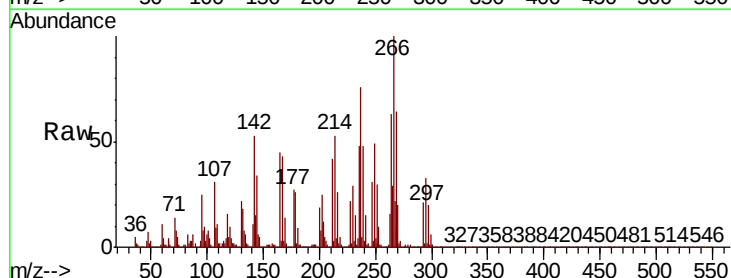

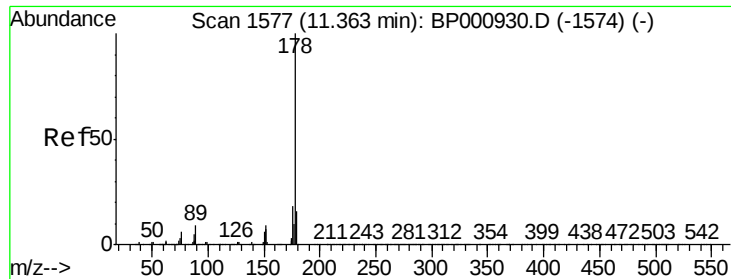





#72
 Anthracene
 Concen: 14.818 ng/ul
 RT: 11.36 min Scan# 1577
 Delta R.T. 0.00 min
 Lab File: BP000931.D
 Acq: 21 Oct 2019 13:12

Instrument :
 BNA_P
 ClientSampleId :
 X2J20

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.8	12.4	18.6
176	18.3	15.1	22.7




Manual Integrations
 APPROVED


mohammad
 10/22/2019 3:28:36 PM

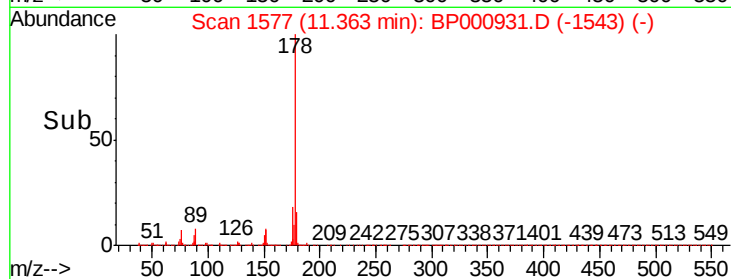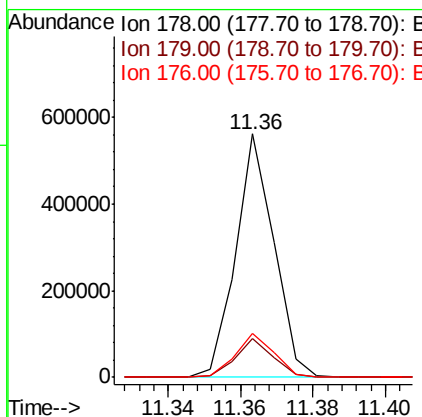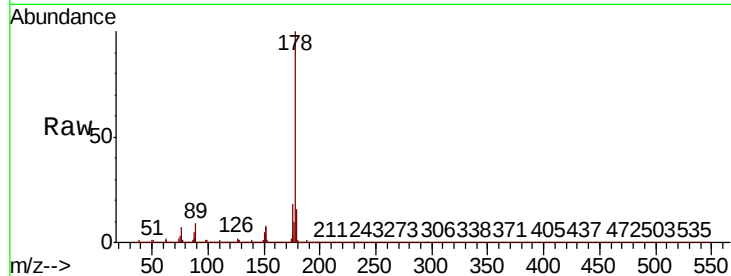

#76
 Di-n-butylphthalate
 Concen: 28.627 ng/ul
 RT: 11.86 min Scan# 1661
 Delta R.T. 0.00 min
 Lab File: BP000931.D
 Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Lower	Upper
149	100		
150	9.4	7.6	11.4
104	4.8	3.7	5.5

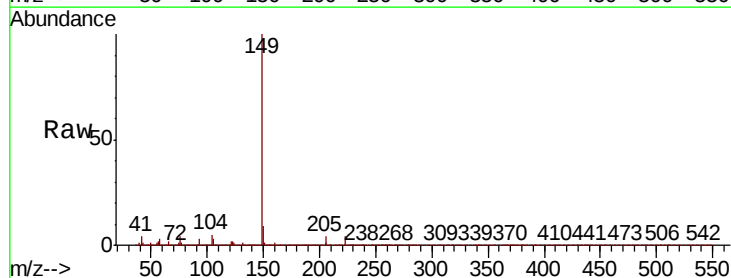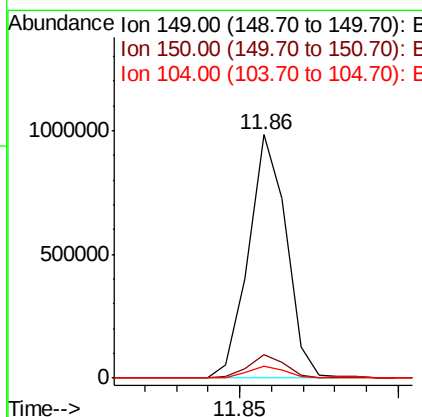

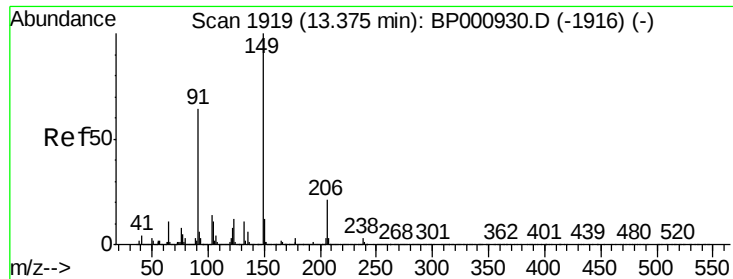





#81
Butylbenzylphthalate
Concen: 35.043 ng/ul
RT: 13.37 min Scan# 1919
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampleId :
X2J20

Tot Ion	Ratio	Lower	Upper
149	100		
91	62.9	50.6	75.8
206	22.7	17.8	26.6




Manual Integrations
APPROVED


mohammad
10/22/2019 3:28:36 PM

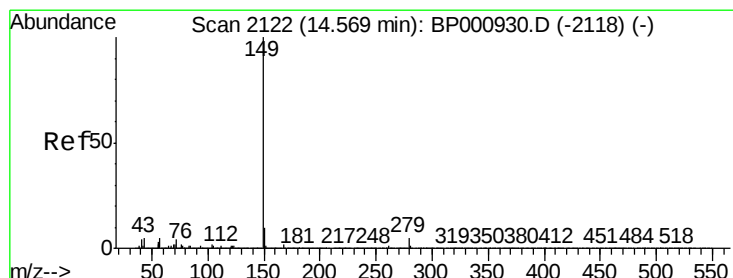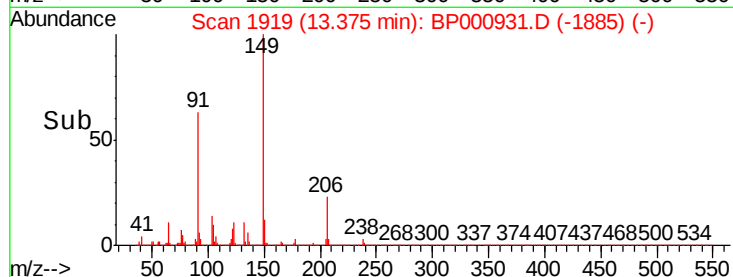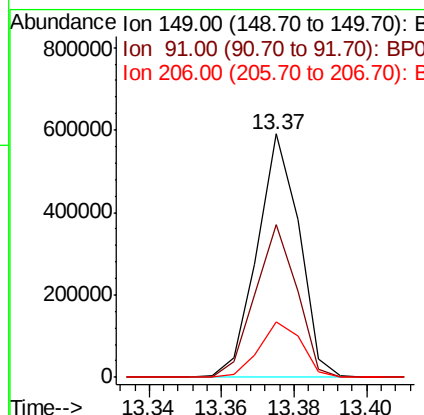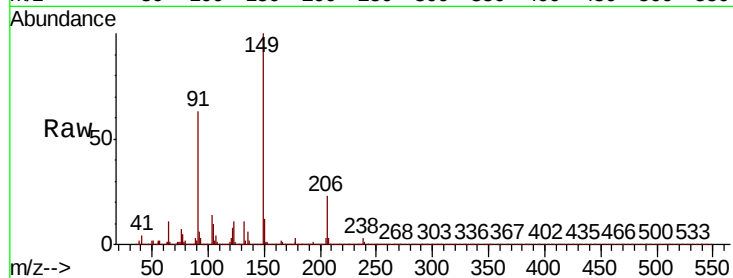

#87
Di-n-octyl phthalate
Concen: 34.750 ng/ul
RT: 14.57 min Scan# 2122
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion:149 Resp: 1016070

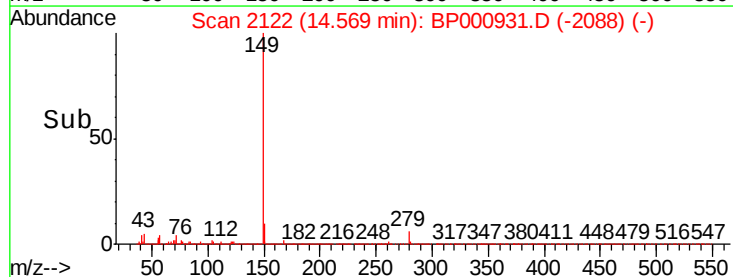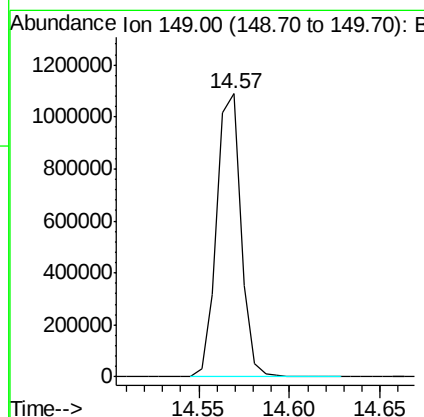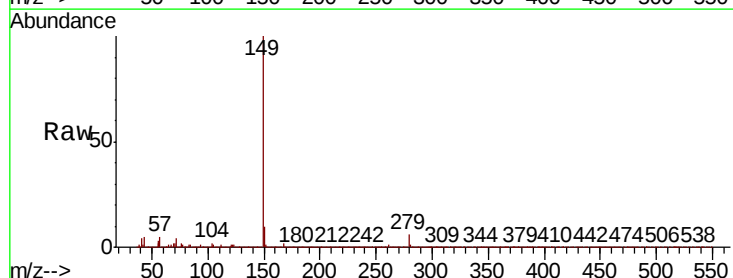

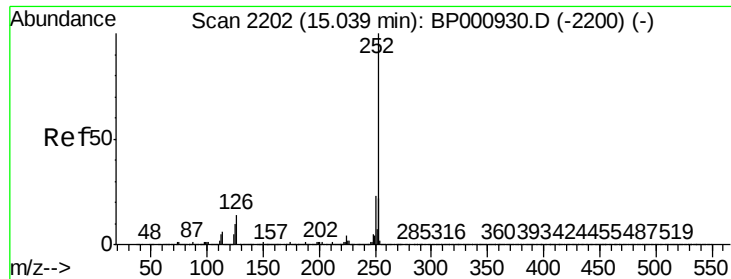





#88
Benzo(b)fluoranthene
Concen: 38.030 ng/ul m
RT: 15.02 min Scan# 2198
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampleId :
X2J20

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.8	17.6	26.4
125	8.2	8.7	13.1#




Manual Integrations
APPROVED


mohammad
10/22/2019 3:28:36 PM

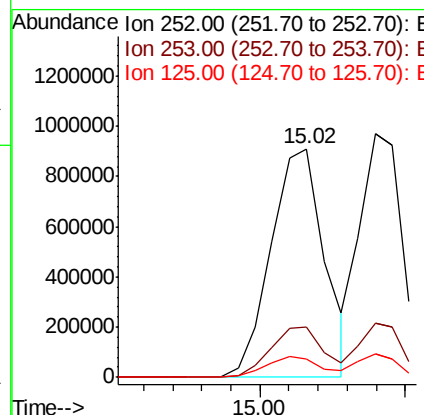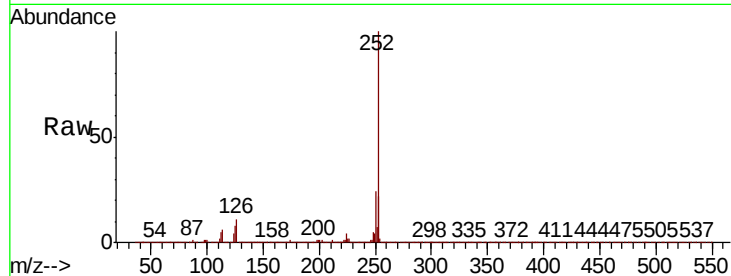

#89
Benzo(k)fluoranthene
Concen: 34.714 ng/ul
RT: 15.04 min Scan# 2202
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.8	26.6
125	9.8	8.2	12.4

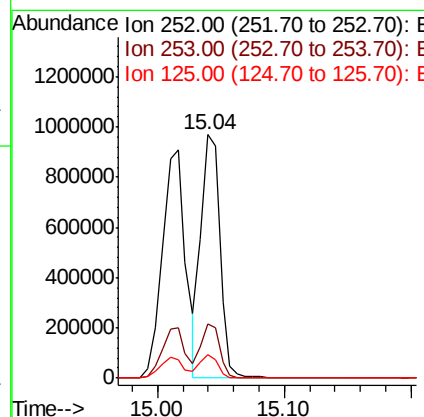

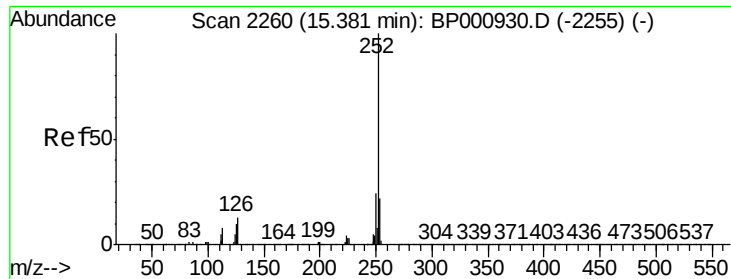





#91
Benzo(a)pyrene
Concen: 33.916 ng/ul
RT: 15.38 min Scan# 2260
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampleId :
X2J20

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.6	26.4
125	9.9	9.7	14.5




Manual Integrations
APPROVED


mohammad
10/22/2019 3:28:36 PM

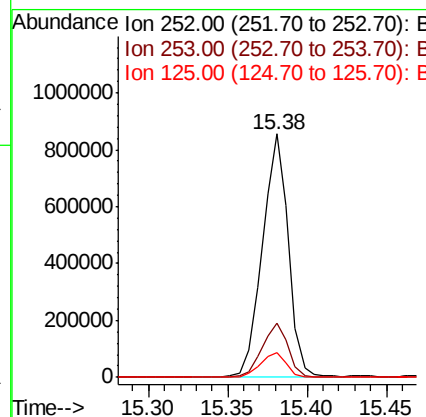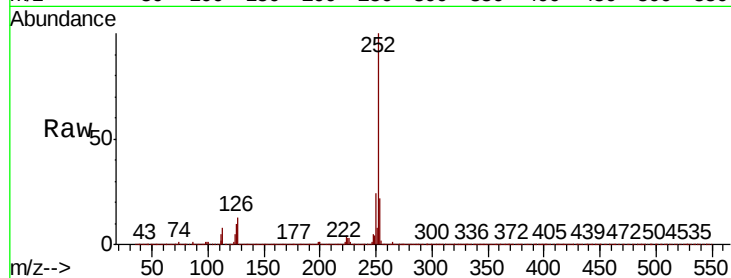

#92
Indeno(1,2,3-cd)pyrene
Concen: 38.278 ng/ul
RT: 16.92 min Scan# 2521
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Lower	Upper
276	100		
138	21.5	20.0	30.0
277	25.0	19.8	29.8

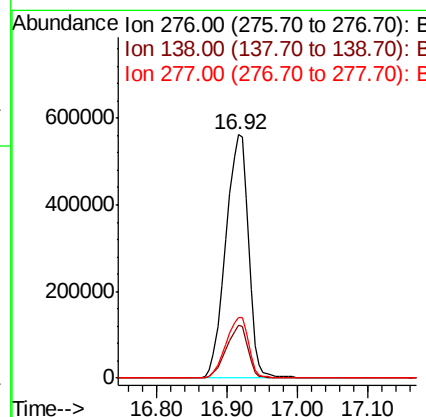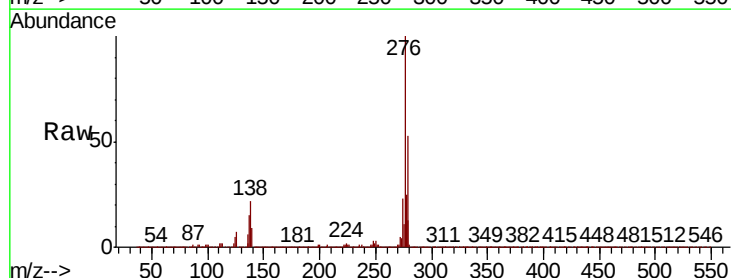

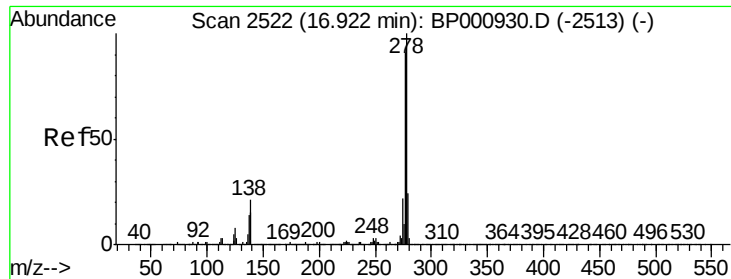





#93
Dibenzo(a,h)anthracene
Concen: 24.077 ng/ul
RT: 16.92 min Scan# 2522
Delta R.T. -0.01 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Instrument :
BNA_P
ClientSampled :
X2J20

Tot Ion	Ratio	Lower	Upper
278	100		
139	15.0	14.2	21.4
279	23.5	19.2	28.8

Manual Integrations
APPROVED

mohammad
10/22/2019 3:28:36 PM

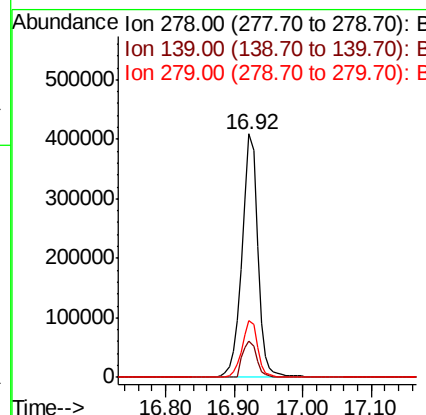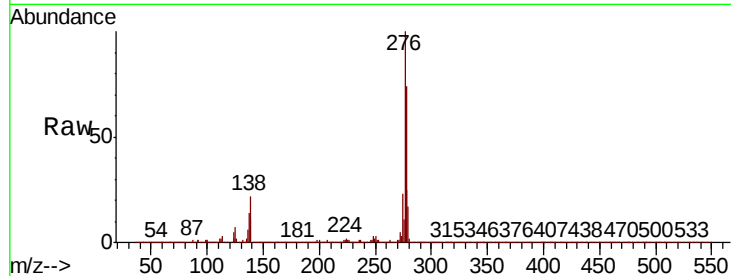

#94
Benzo(g,h,i)perylene
Concen: 38.764 ng/ul
RT: 17.36 min Scan# 2596
Delta R.T. 0.00 min
Lab File: BP000931.D
Acq: 21 Oct 2019 13:12

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.5	18.4	27.6
277	23.7	19.4	29.0

