

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007552.D
 Acq On : 21 Oct 2021 13:29
 Operator : CG/JU
 Sample : M4262-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY68

Quant Time: Oct 21 13:54:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	184497	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	764356	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	494925	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	1074038	20.000	ng/ul	0.00
79) Chrysene-d12	21.421	240	1135706	20.000	ng/ul	0.00
88) Perylene-d12	23.874	264	1154715	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	21000	4.496	ng/uL	0.00
4) Pyridine-d5	3.799	84	175375	13.715	ng/ul	0.00
7) Phenol-d5	7.110	99	124783	8.661	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	229712	26.731	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	247125	21.802	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	216978	19.551	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	154034	31.844	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	140520	31.100	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	278482	25.270	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	420074	28.188	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	1070124	31.253	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	1205895	28.023	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	29978	5.456	ng/ul	0.00
60) Fluorene-d10	15.580	176	943483	32.926	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	72013	16.733	ng/ul	0.00
73) Anthracene-d10	17.439	188	1663520	36.471	ng/ul	0.00
81) Pyrene-d10	19.668	212	2011532	35.429	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.715	264	2010367	34.989	ng/ul	0.00
Target Compounds						
8) Phenol	7.134	94	18587	1.262	ng/ul	97
18) 4-Methylphenol	8.710	108	129334	10.943	ng/ul	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007552.D
Acq On : 21 Oct 2021 13:29
Operator : CG/JU
Sample : M4262-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY68

Quant Time: Oct 21 13:54:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration




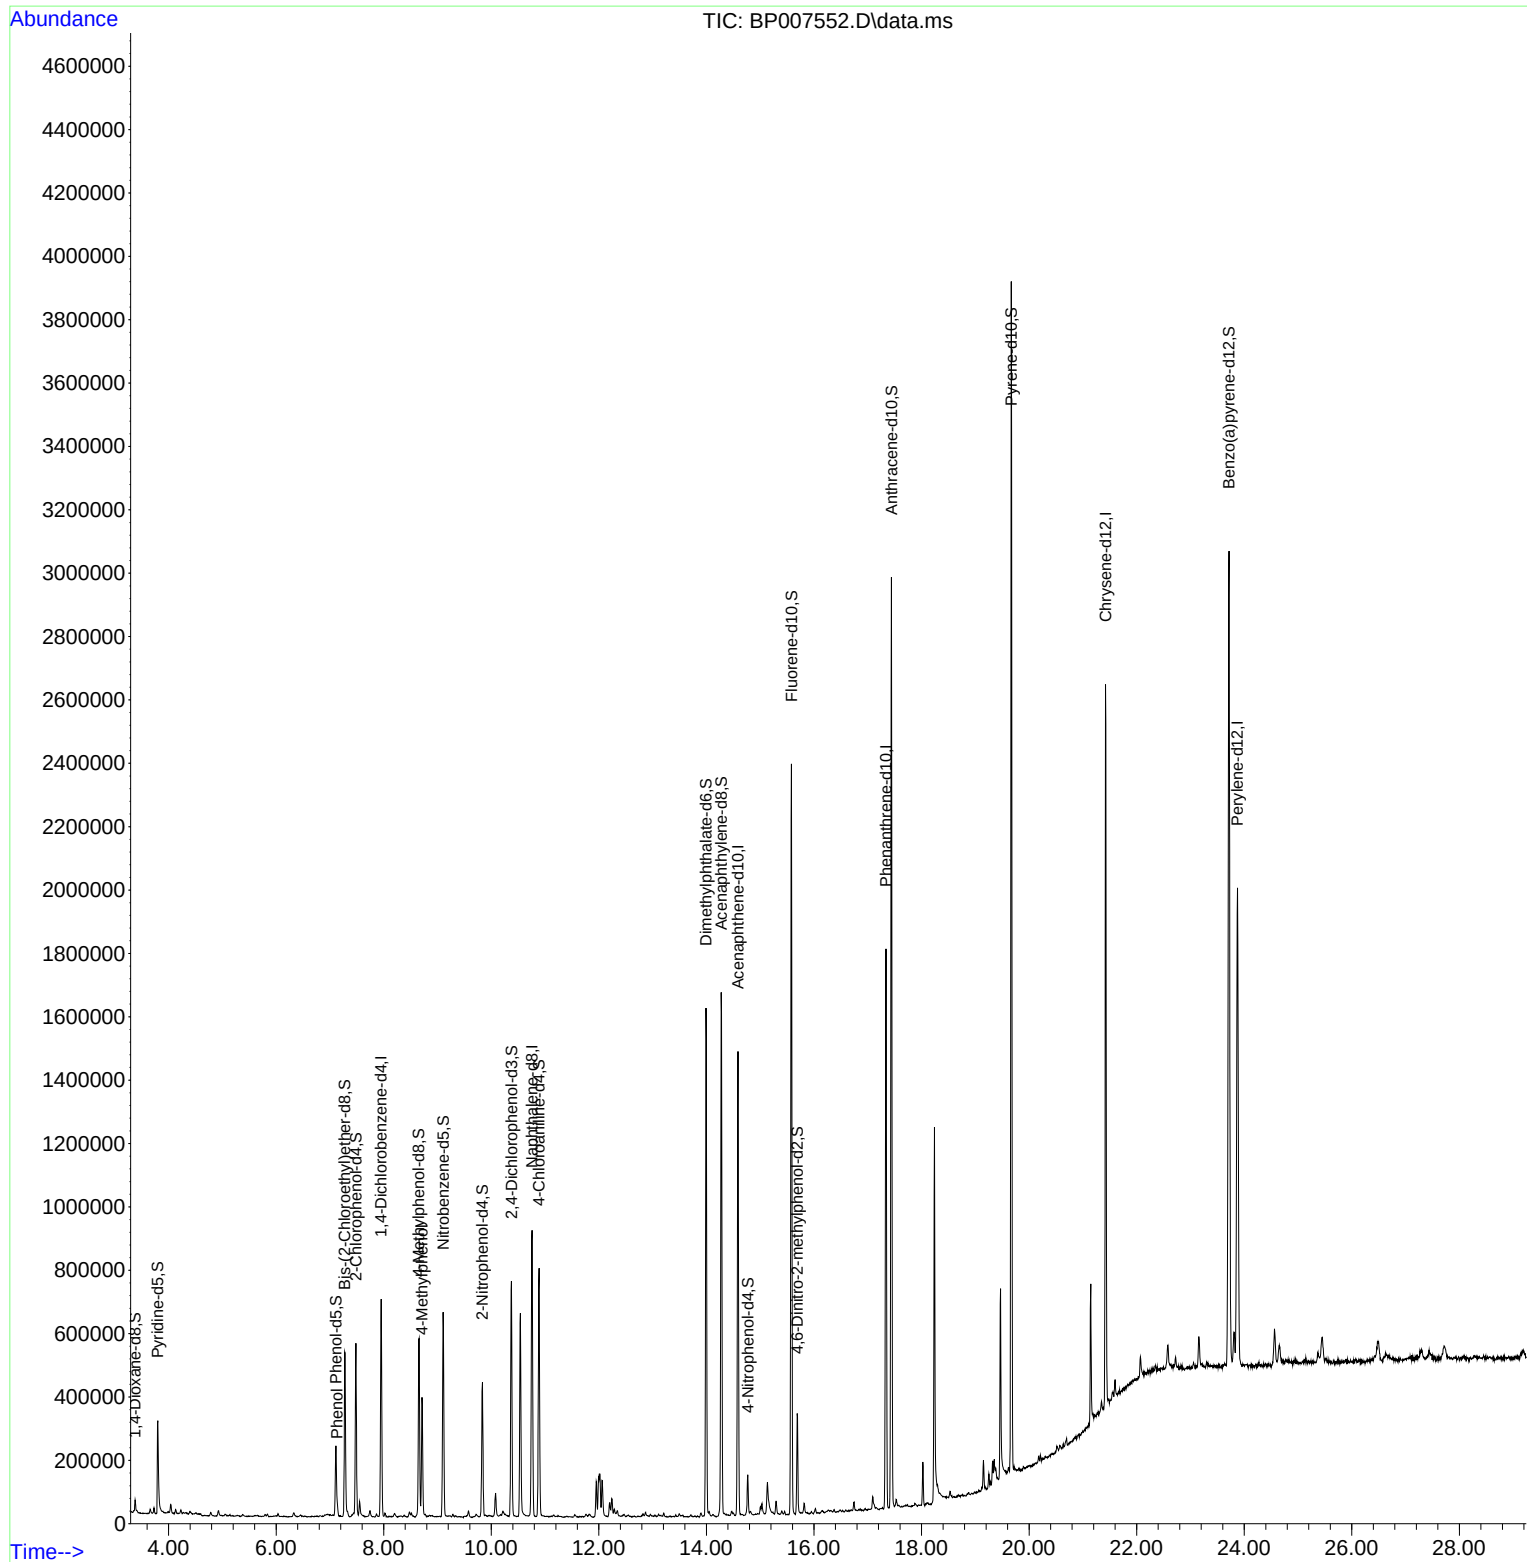


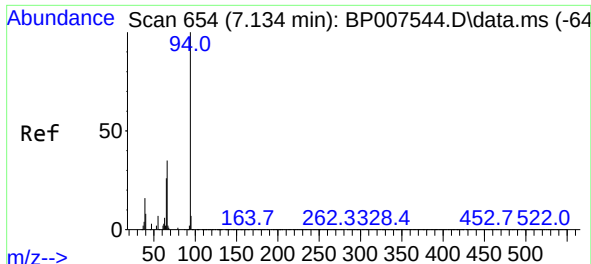

#8
Phenol
Concen: 1.262 ng/ul
RT: 7.134 min Scan# 654
Delta R.T. -0.006 min
Lab File: BP007552.D
Acq: 21 Oct 2021 13:29

Instrument :
BNA_P
ClientSampleId :
BFY68

Tgt Ion: 94 Resp: 18587
Ion Ratio Lower Upper
94 100
65 26.2 21.9 32.9
66 39.5 29.9 44.9

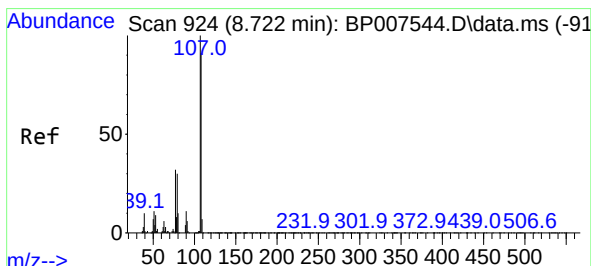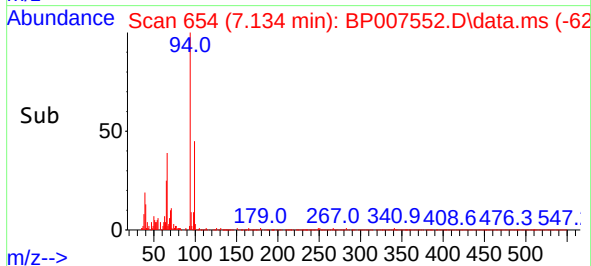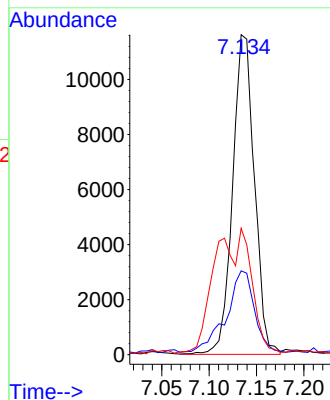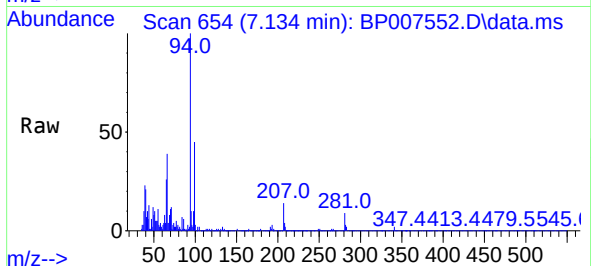

#18
4-Methylphenol
Concen: 10.943 ng/ul
RT: 8.710 min Scan# 922
Delta R.T. -0.012 min
Lab File: BP007552.D
Acq: 21 Oct 2021 13:29

Tgt Ion: 108 Resp: 129334
Ion Ratio Lower Upper
108 100
107 125.6 90.9 136.3

