

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007555.D
 Acq On : 21 Oct 2021 15:11
 Operator : CG/JU
 Sample : M4262-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY78

Quant Time: Oct 21 15:41:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	189124	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	774548	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	492890	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	1065272	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	1115006	20.000	ng/u1	0.00
88) Perylene-d12	23.874	264	1144072	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	25588	5.344	ng/uL	0.00
4) Pyridine-d5	3.799	84	102846	7.846	ng/u1	0.00
7) Phenol-d5	7.111	99	200616	13.583	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	295436	33.537	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	391323	33.679	ng/u1	0.00
15) 4-Methylphenol-d8	8.658	113	312398	27.460	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	196203	40.028	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	205786	44.946	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	400491	35.863	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	454410	30.090	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	1219799	35.771	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	1480766	34.553	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	58959	10.775	ng/u1	0.00
60) Fluorene-d10	15.581	176	1058218	37.083	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	148799	34.860	ng/u1	0.00
73) Anthracene-d10	17.439	188	1835063	40.562	ng/u1	0.00
81) Pyrene-d10	19.675	212	2240468	40.194	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.721	264	2234465	39.252	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.411	88	51578	9.902	ng/uL	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007555.D
Acq On : 21 Oct 2021 15:11
Operator : CG/JU
Sample : M4262-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY78

Quant Time: Oct 21 15:41:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

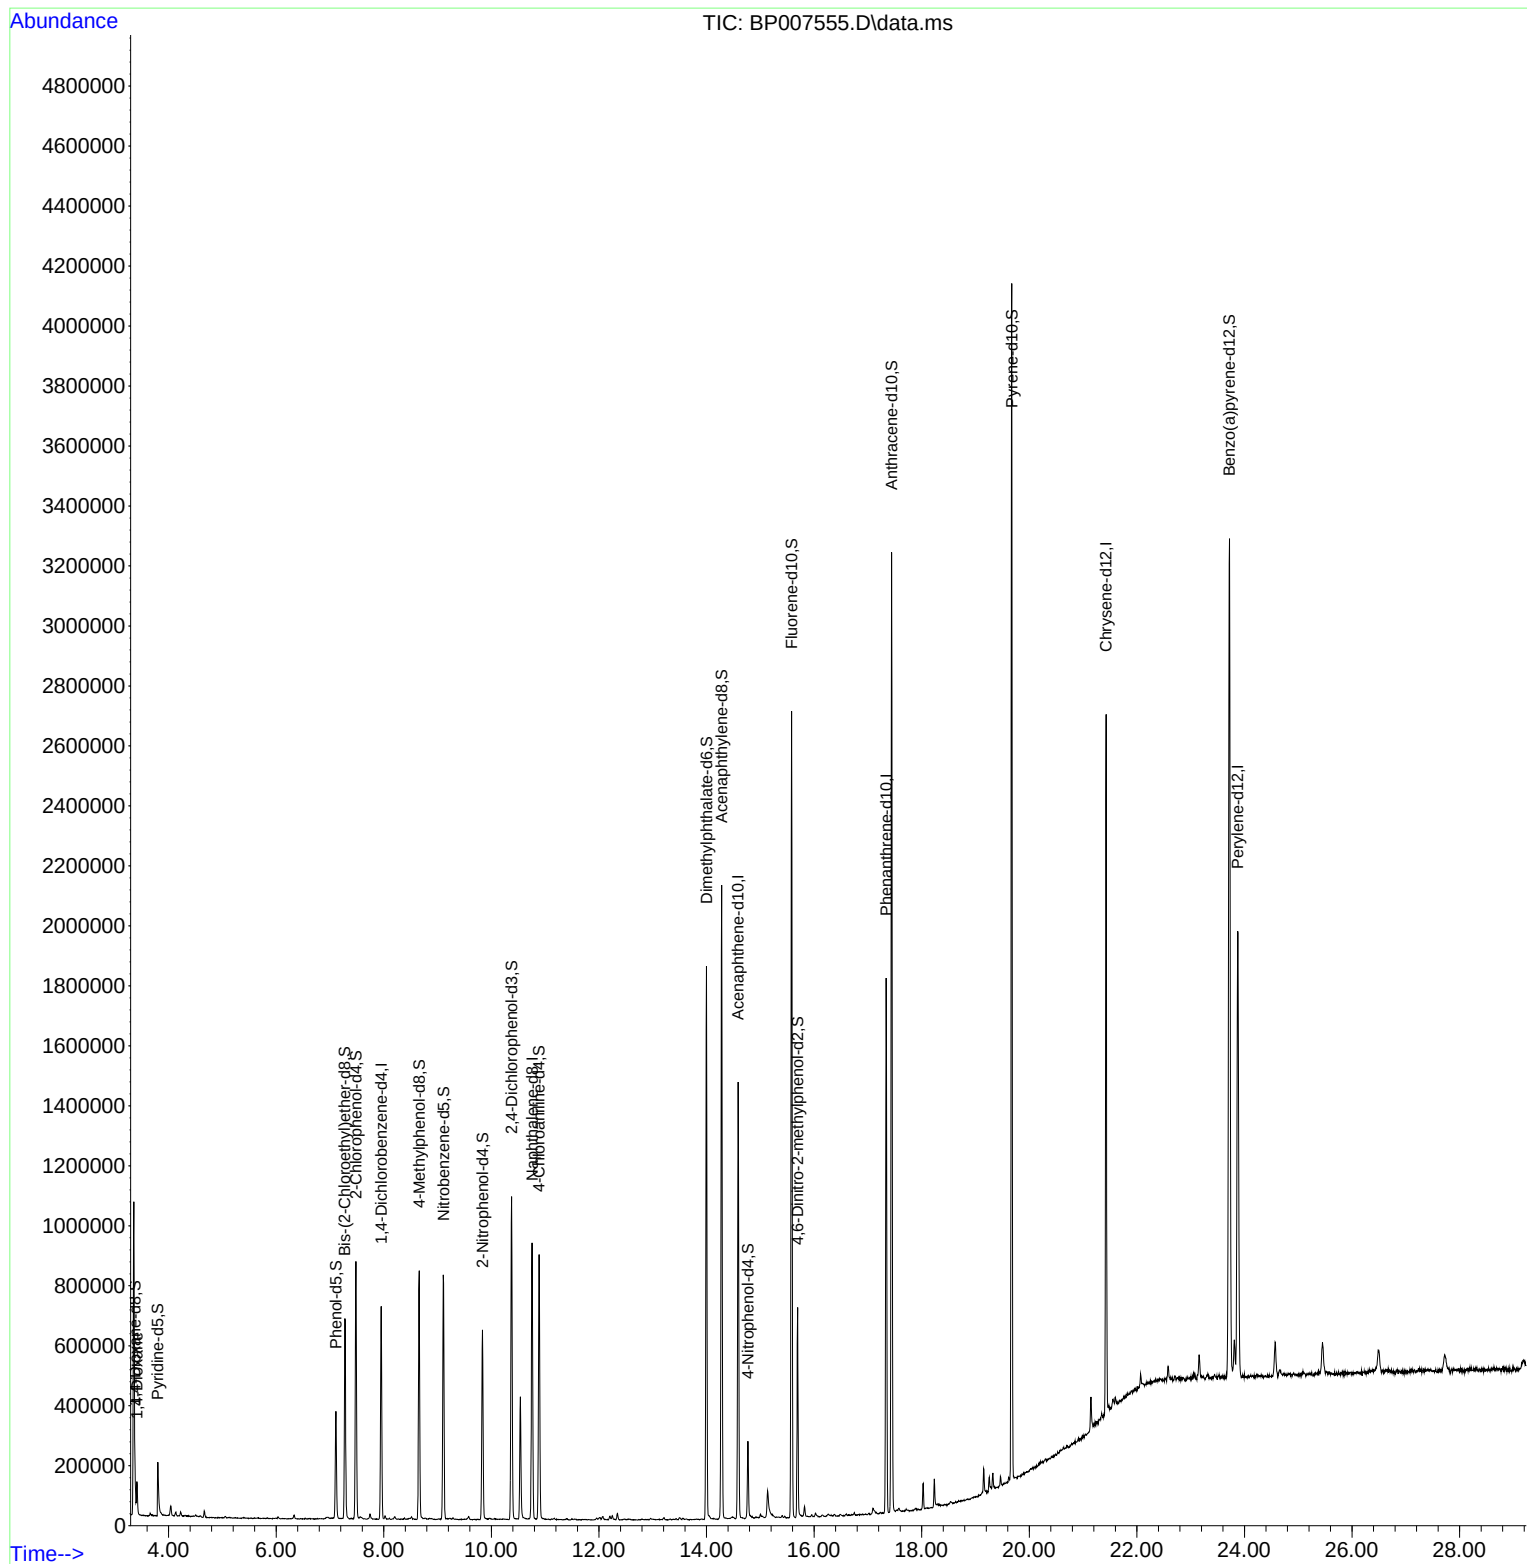

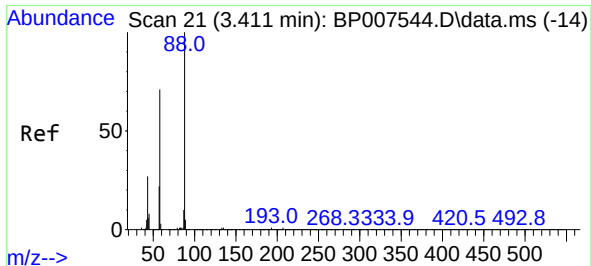

#2
 1,4-Dioxane
 Concen: 9.902 ng/uL
 RT: 3.411 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP007555.D
 Acq: 21 Oct 2021 15:11

Instrument :
 BNA_P
 ClientSampleId :
 BFY78

Tgt Ion: 88 Resp: 51578
 Ion Ratio Lower Upper
 88 100
 43 26.5 24.2 36.2
 58 72.2 62.5 93.7

