

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007556.D
 Acq On : 21 Oct 2021 15:46
 Operator : CG/JU
 Sample : M4262-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY55

Quant Time: Oct 21 16:15:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	168716	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	692736	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	449939	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	972210	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	1030213	20.000	ng/u1	0.00
88) Perylene-d12	23.880	264	1046425	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	23473	5.495	ng/uL	0.00
4) Pyridine-d5	3.793	84	216905	18.549	ng/u1	0.00
7) Phenol-d5	7.110	99	88900	6.747	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	171273	21.794	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	187907	18.129	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	146435	14.428	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	107404	24.499	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	99496	24.298	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	203523	20.377	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	562342	41.635	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	732269	23.524	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	794077	20.298	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	28174	5.641	ng/u1	0.00
60) Fluorene-d10	15.581	176	610935	23.452	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	68293	17.531	ng/u1	0.00
73) Anthracene-d10	17.439	188	1060257	25.679	ng/u1	0.00
81) Pyrene-d10	19.674	212	1307016	25.378	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.721	264	1200407	23.055	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.411	88	73367	15.789	ng/uL 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007556.D
Acq On : 21 Oct 2021 15:46
Operator : CG/JU
Sample : M4262-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY55

Quant Time: Oct 21 16:15:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

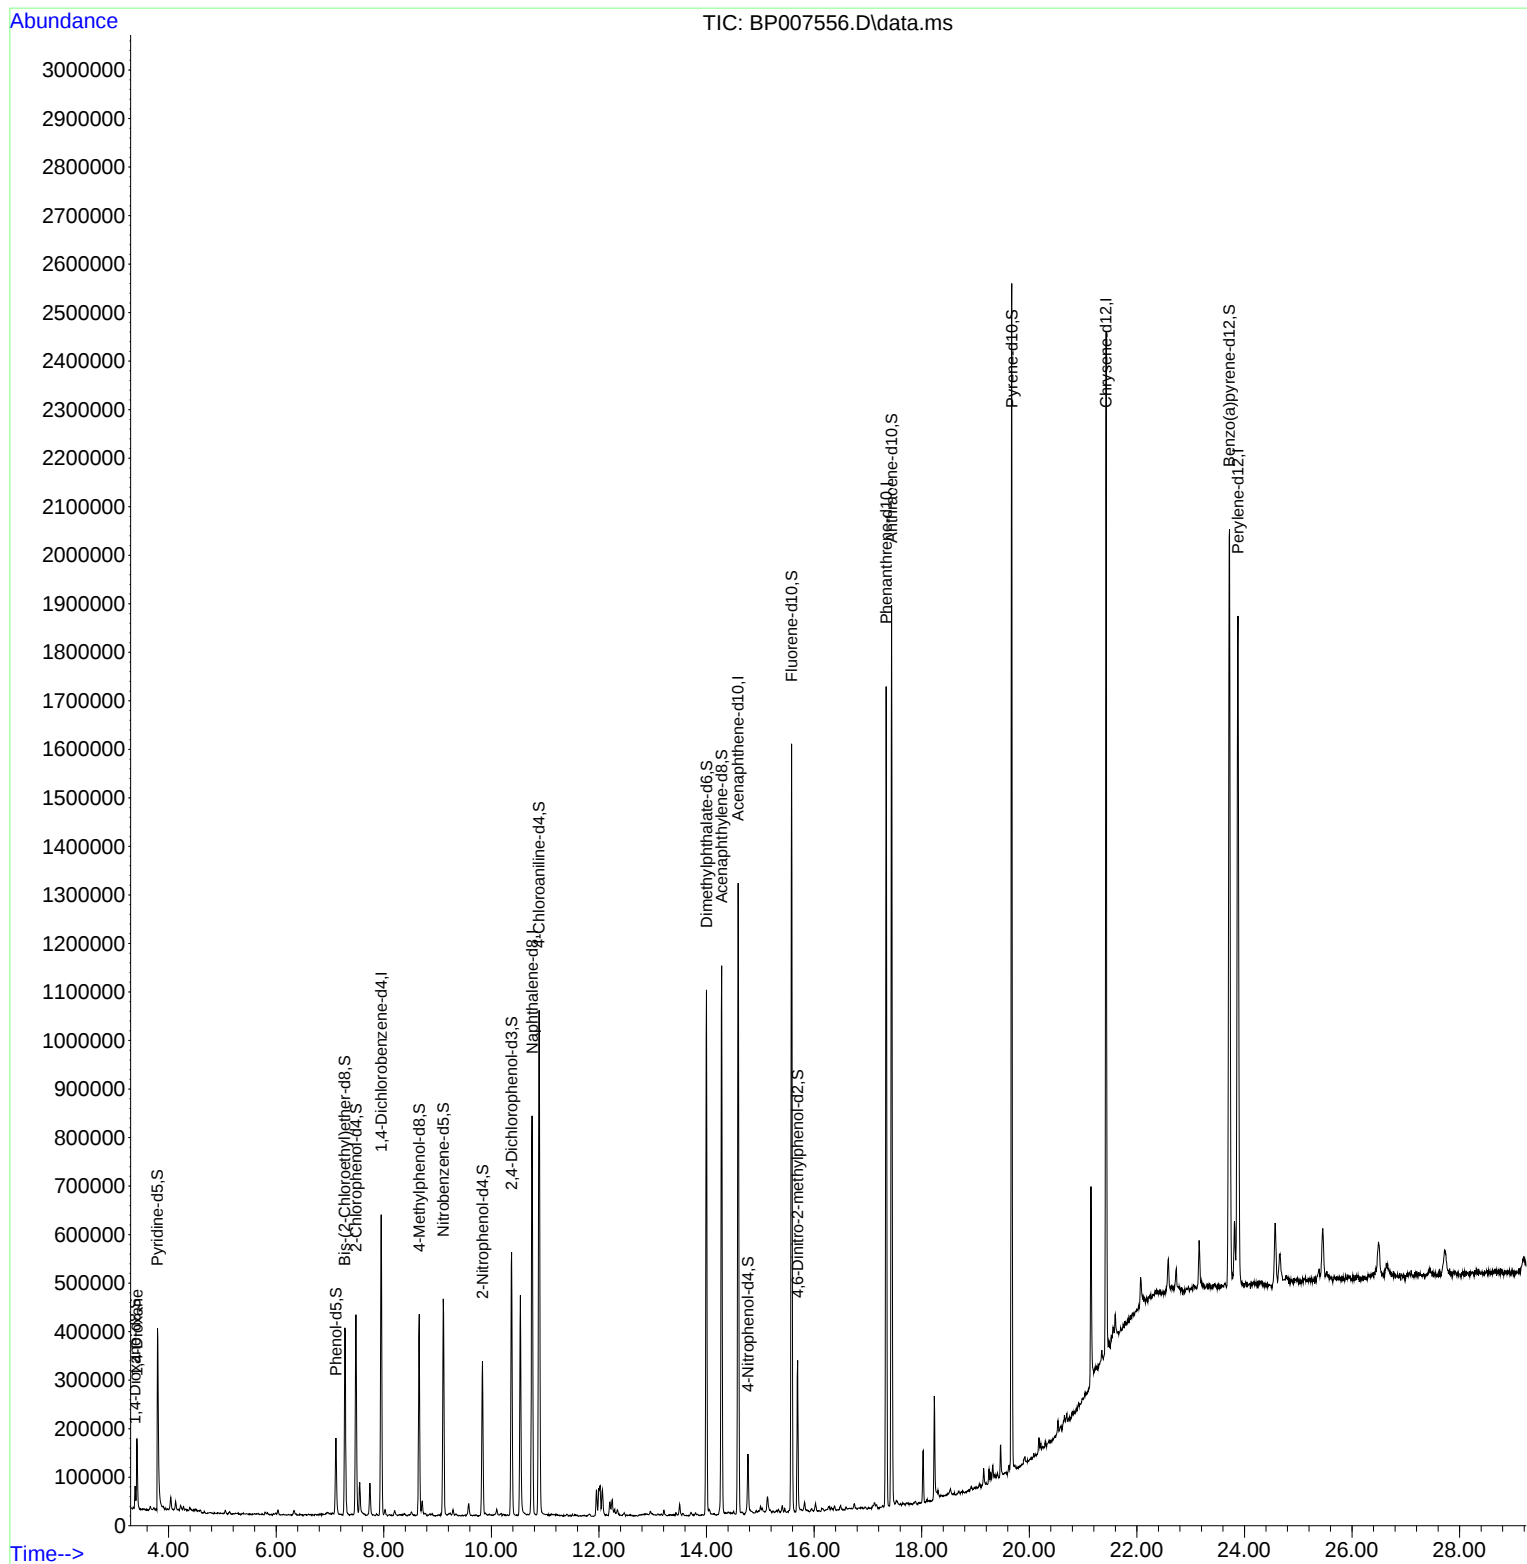

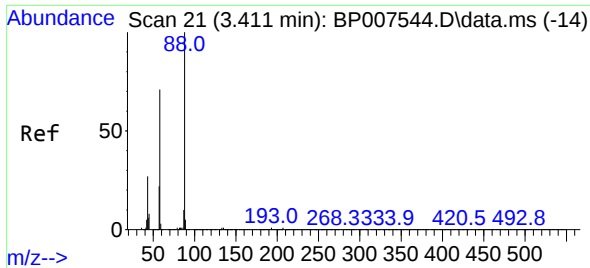

#2
 1,4-Dioxane
 Concen: 15.789 ng/uL
 RT: 3.411 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP007556.D
 Acq: 21 Oct 2021 15:46

Instrument :
 BNA_P
 ClientSampleId :
 BFY55

Tgt Ion: 88 Resp: 73367
 Ion Ratio Lower Upper
 88 100
 43 25.3 24.2 36.2
 58 72.5 62.5 93.7

