

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007564.D
 Acq On : 21 Oct 2021 20:56
 Operator : CG/JU
 Sample : M4262-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY93

Quant Time: Oct 22 00:59:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	190456	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	776698	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	505881	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	1086934	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	1136619	20.000	ng/u1	0.00
88) Perylene-d12	23.868	264	1169438	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	24556	5.092	ng/uL	0.00
4) Pyridine-d5	3.793	84	142402	10.788	ng/u1	0.00
7) Phenol-d5	7.105	99	146272	9.834	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	336301	37.909	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	379254	32.412	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	261682	22.841	ng/u1	0.00
21) Nitrobenzene-d5	9.105	128	230857	46.967	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	234765	51.134	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	439701	39.265	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	528655	34.910	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	1469117	41.976	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1745774	39.691	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	56860	10.125	ng/u1	0.00
60) Fluorene-d10	15.575	176	1256782	42.910	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	171656	39.413	ng/u1	0.00
73) Anthracene-d10	17.434	188	2089415	45.264	ng/u1	0.00
81) Pyrene-d10	19.669	212	2514476	44.252	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.716	264	2524891	43.391	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.411	88	28707	5.473	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007564.D
Acq On : 21 Oct 2021 20:56
Operator : CG/JU
Sample : M4262-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY93

Quant Time: Oct 22 00:59:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

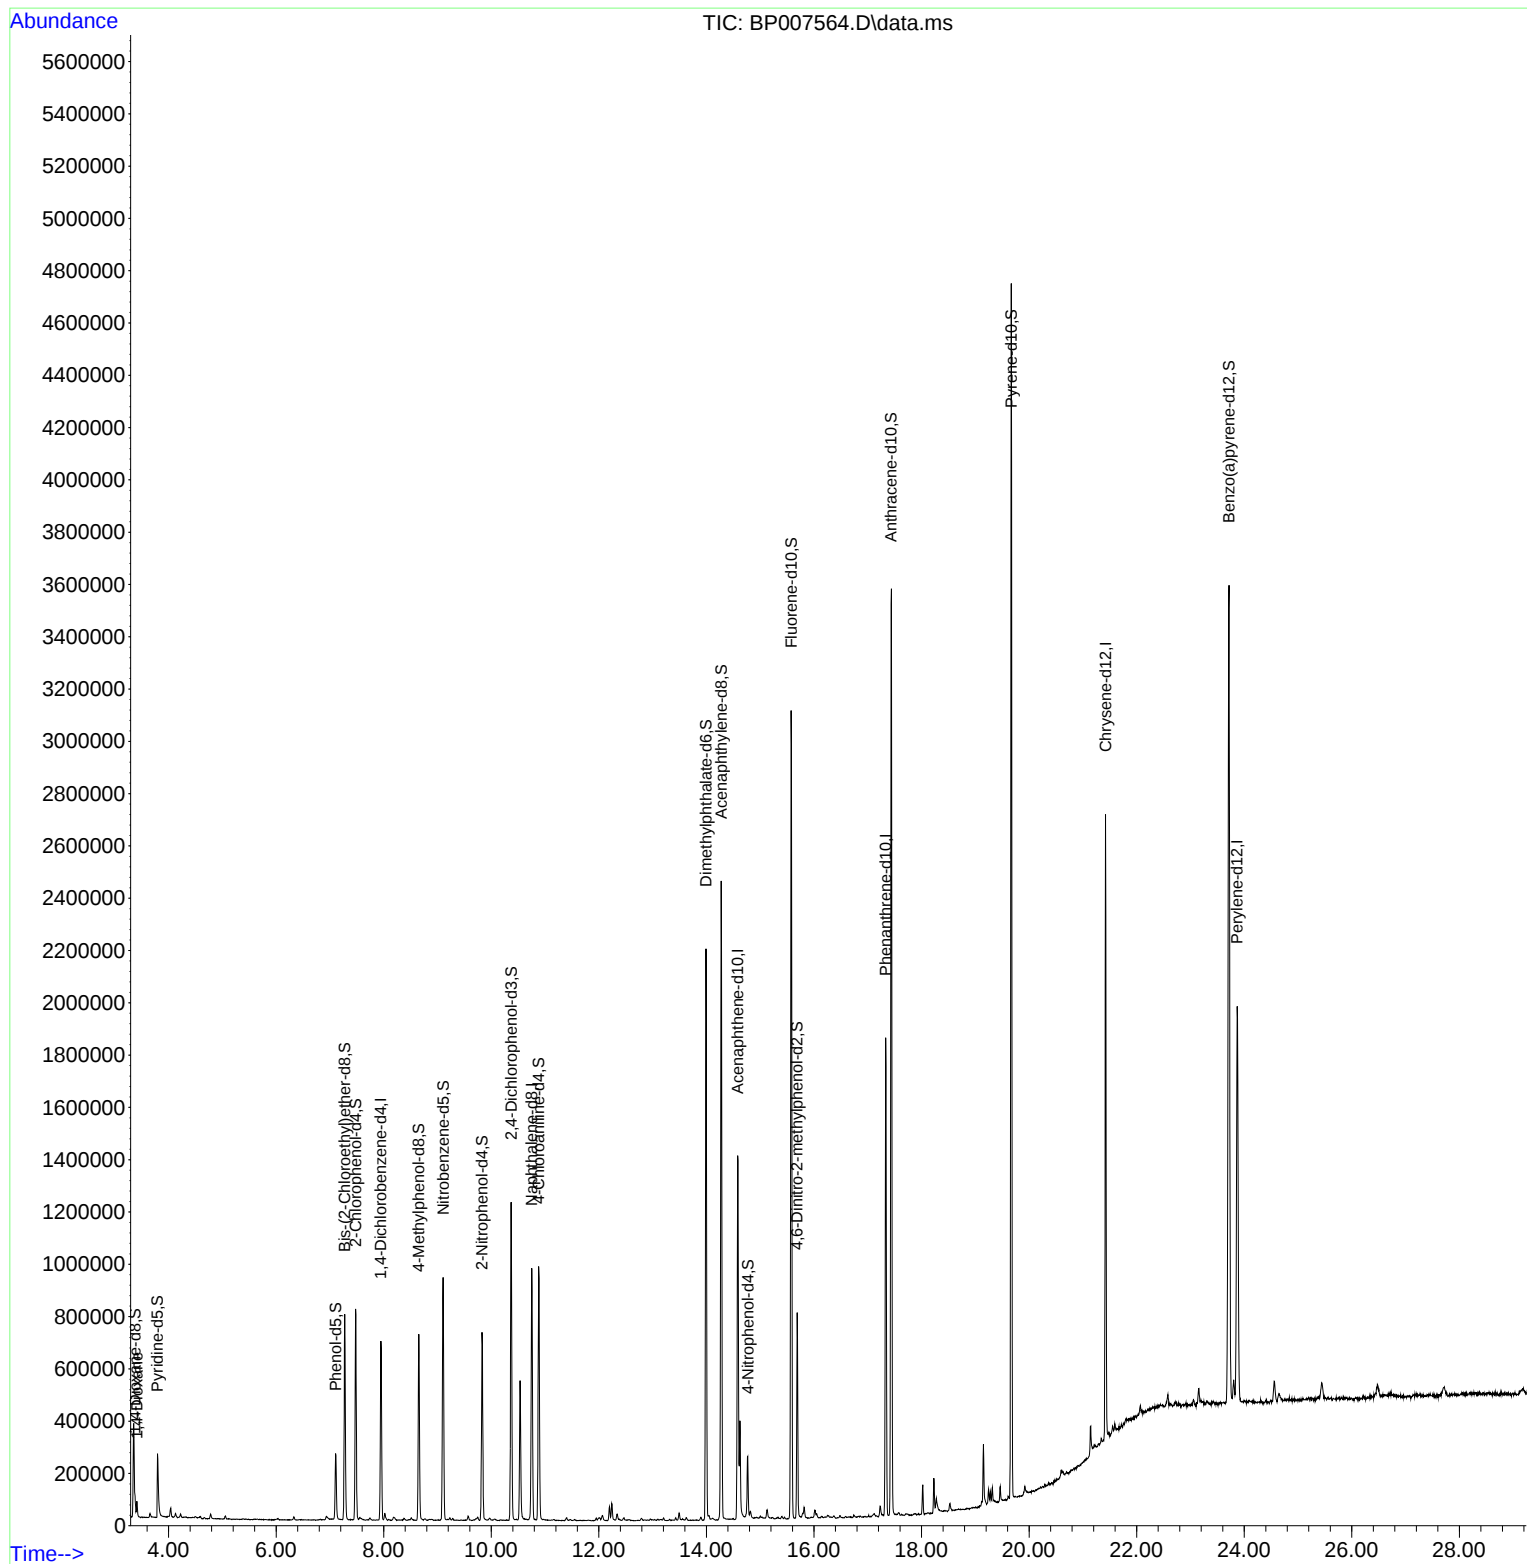

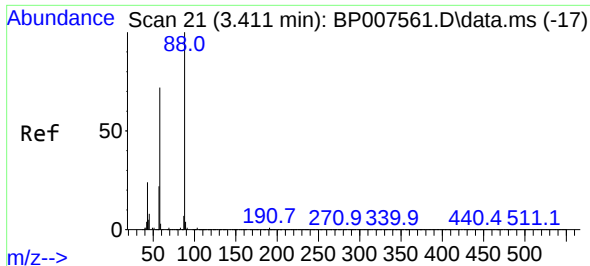

#2
 1,4-Dioxane
 Concen: 5.473 ng/uL
 RT: 3.411 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP007564.D
 Acq: 21 Oct 2021 20:56

Instrument :
 BNA_P
 ClientSampleId :
 BFY93

Tgt Ion: 88	Resp: 28707
Ion Ratio	Lower Upper
88	100
43	25.8 24.2 36.2
58	68.3 62.5 93.7

