

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007573.D
 Acq On : 22 Oct 2021 03:42
 Operator : CG/JU
 Sample : M4217-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGC3

Quant Time: Oct 22 04:27:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	237872	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	960936	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	611267	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.334	188	1307966	20.000	ng/ul	0.00
79) Chrysene-d12	21.422	240	1258849	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	1366742	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	10189	1.692	ng/uL	0.00
4) Pyridine-d5	3.799	84	80987	4.912	ng/ul	0.00
7) Phenol-d5	7.105	99	186341	10.031	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	107518	9.704	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	147253	10.076	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	147655	10.319	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	66904	11.002	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	64138	11.291	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	146157	10.549	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	133615	7.132	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	467684	11.059	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	566657	10.662	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	56068	8.263	ng/ul	-0.01
60) Fluorene-d10	15.575	176	436099	12.322	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	30387	5.798	ng/ul	0.00
73) Anthracene-d10	17.434	188	698022	12.566	ng/ul	0.00
81) Pyrene-d10	19.663	212	757242	12.033	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	786254	11.561	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.769	105	37554	1.716	ng/ul	95
78) Di-n-butylphthalate	18.298	149	421920	5.979	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.345	149	2473382	55.961	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007573.D
Acq On : 22 Oct 2021 03:42
Operator : CG/JU
Sample : M4217-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGC3

Quant Time: Oct 22 04:27:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration




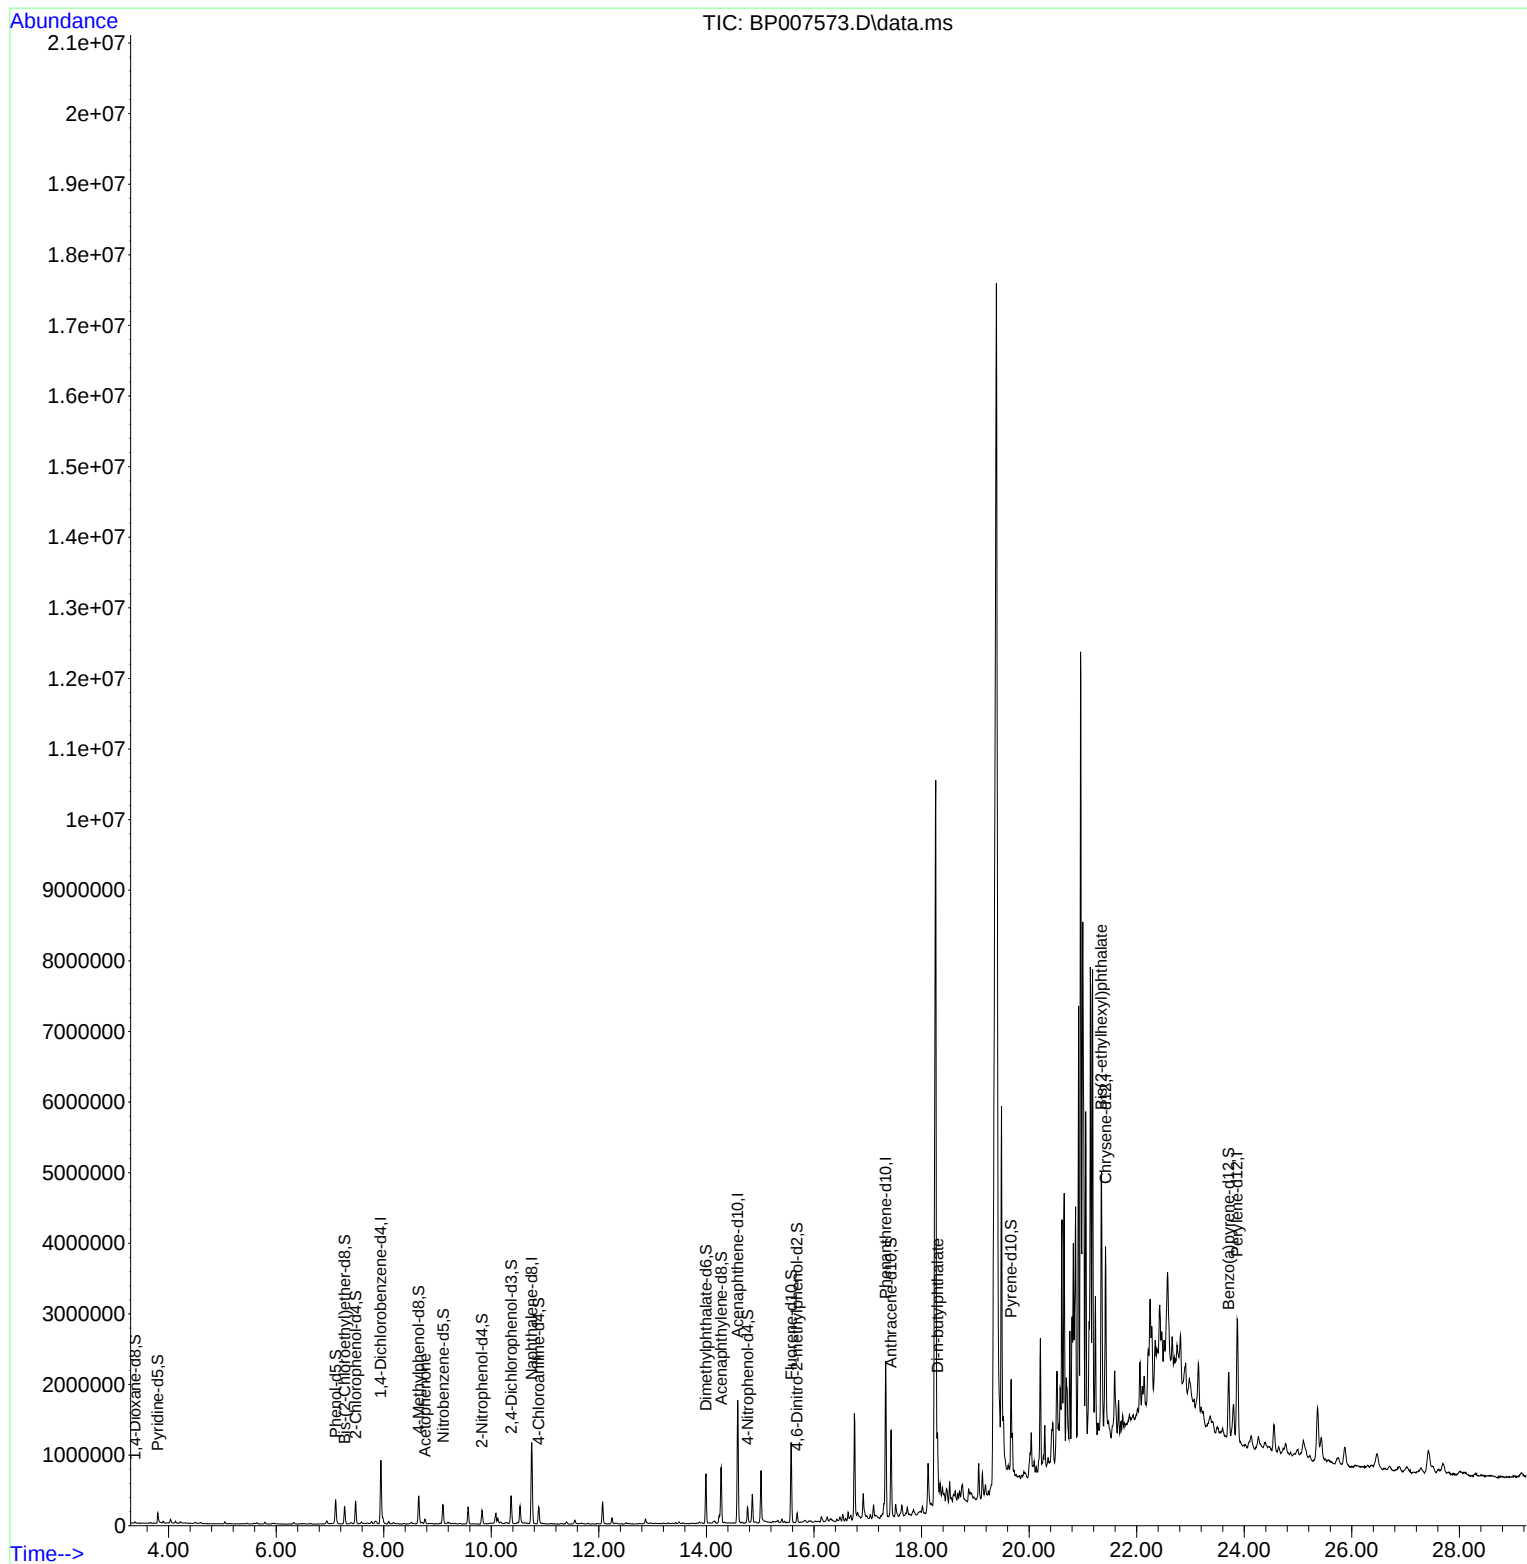


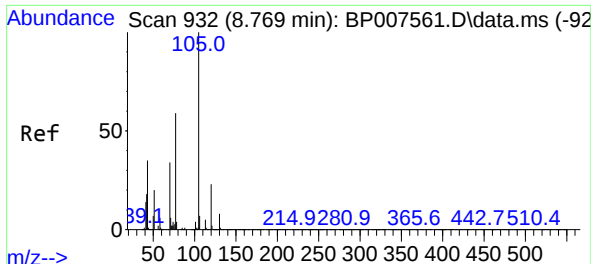

#16
Acetophenone
Concen: 1.716 ng/ul
RT: 8.769 min Scan# 932
Delta R.T. -0.006 min
Lab File: BP007573.D
Acq: 22 Oct 2021 03:42




Instrument :
BNA_P
ClientSampleId :
JDGC3


Tgt Ion:105 Resp: 37554
Ion Ratio Lower Upper
105 100
77 72.1 61.8 92.6
51 27.6 20.8 31.2

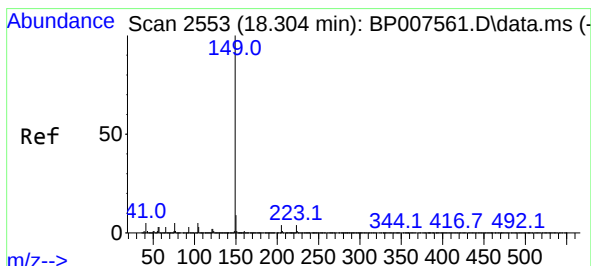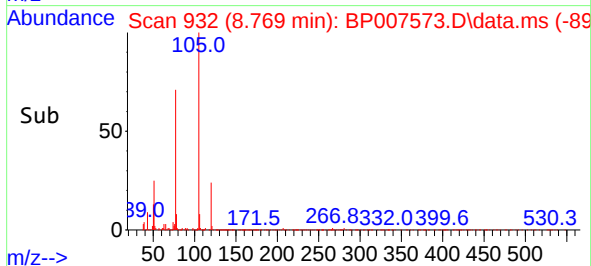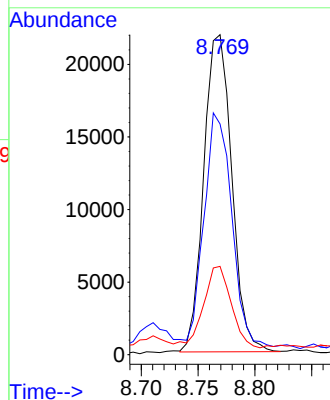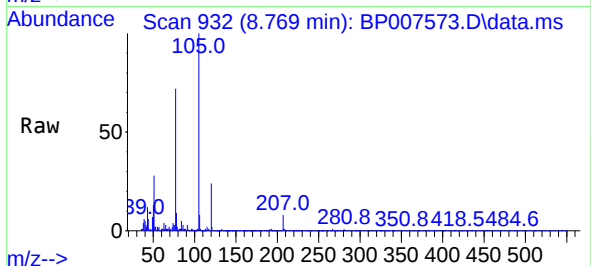

#78
Di-n-butylphthalate
Concen: 5.979 ng/ul
RT: 18.298 min Scan# 2552
Delta R.T. -0.006 min
Lab File: BP007573.D
Acq: 22 Oct 2021 03:42


Tgt Ion:149 Resp: 421920
Ion Ratio Lower Upper
149 100
150 9.1 7.3 10.9
104 5.2 4.2 6.4

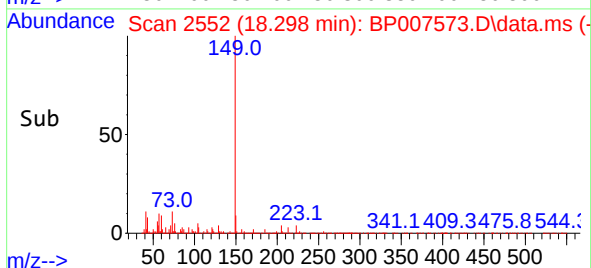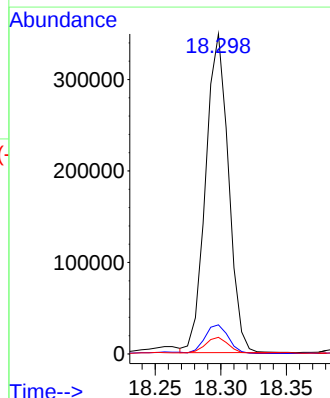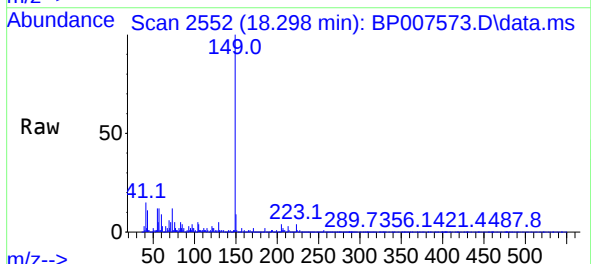

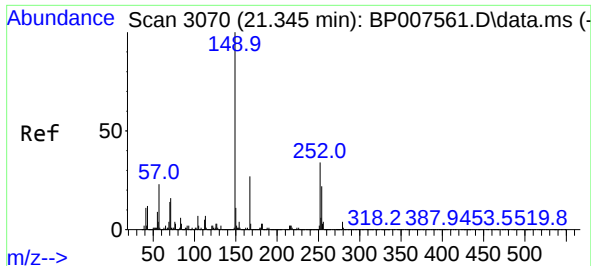

#86
Bis(2-ethylhexyl)phthalate
Concen: 55.961 ng/ul
RT: 21.345 min Scan# 3070
Delta R.T. 0.000 min
Lab File: BP007573.D
Acq: 22 Oct 2021 03:42

Instrument :
BNA_P
ClientSampleId :
JDGC3

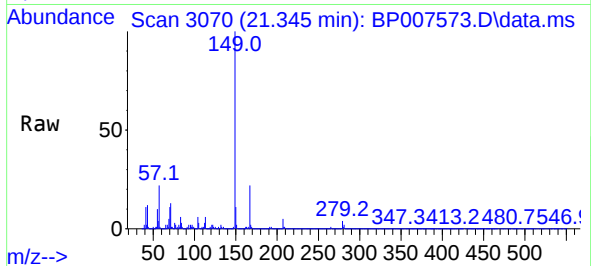

Tgt Ion:149 Resp: 2473382
Ion Ratio Lower Upper
149 100
167 21.6 22.6 33.8#
279 3.9 3.3 4.9

