

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007578.D
 Acq On : 22 Oct 2021 07:39
 Operator : CG/JU
 Sample : M4217-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGD3

Quant Time: Oct 22 08:28:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	220754	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	910236	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	596200	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	1283779	20.000	ng/ul	0.00
79) Chrysene-d12	21.421	240	1362433	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	1407672	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	8078	1.445	ng/uL	0.00
4) Pyridine-d5	3.799	84	70956	4.638	ng/ul	0.00
7) Phenol-d5	7.105	99	144565	8.386	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	86018	8.366	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	116455	8.587	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	67904	5.114	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	53946	9.365	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	53114	9.871	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	107204	8.169	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	136084	7.668	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	362039	8.777	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	425766	8.214	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	43809	6.619	ng/ul	-0.01
60) Fluorene-d10	15.575	176	330824	9.584	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	24290	4.722	ng/ul	0.00
73) Anthracene-d10	17.433	188	528109	9.687	ng/ul	0.00
81) Pyrene-d10	19.663	212	702103	10.308	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	671651	9.589	ng/ul	-0.01
Target Compounds						
					Qvalue	
83) Butylbenzylphthalate	20.574	149	66326	2.120	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.339	149	49747	1.040	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007578.D
Acq On : 22 Oct 2021 07:39
Operator : CG/JU
Sample : M4217-16
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGD3

Quant Time: Oct 22 08:28:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration




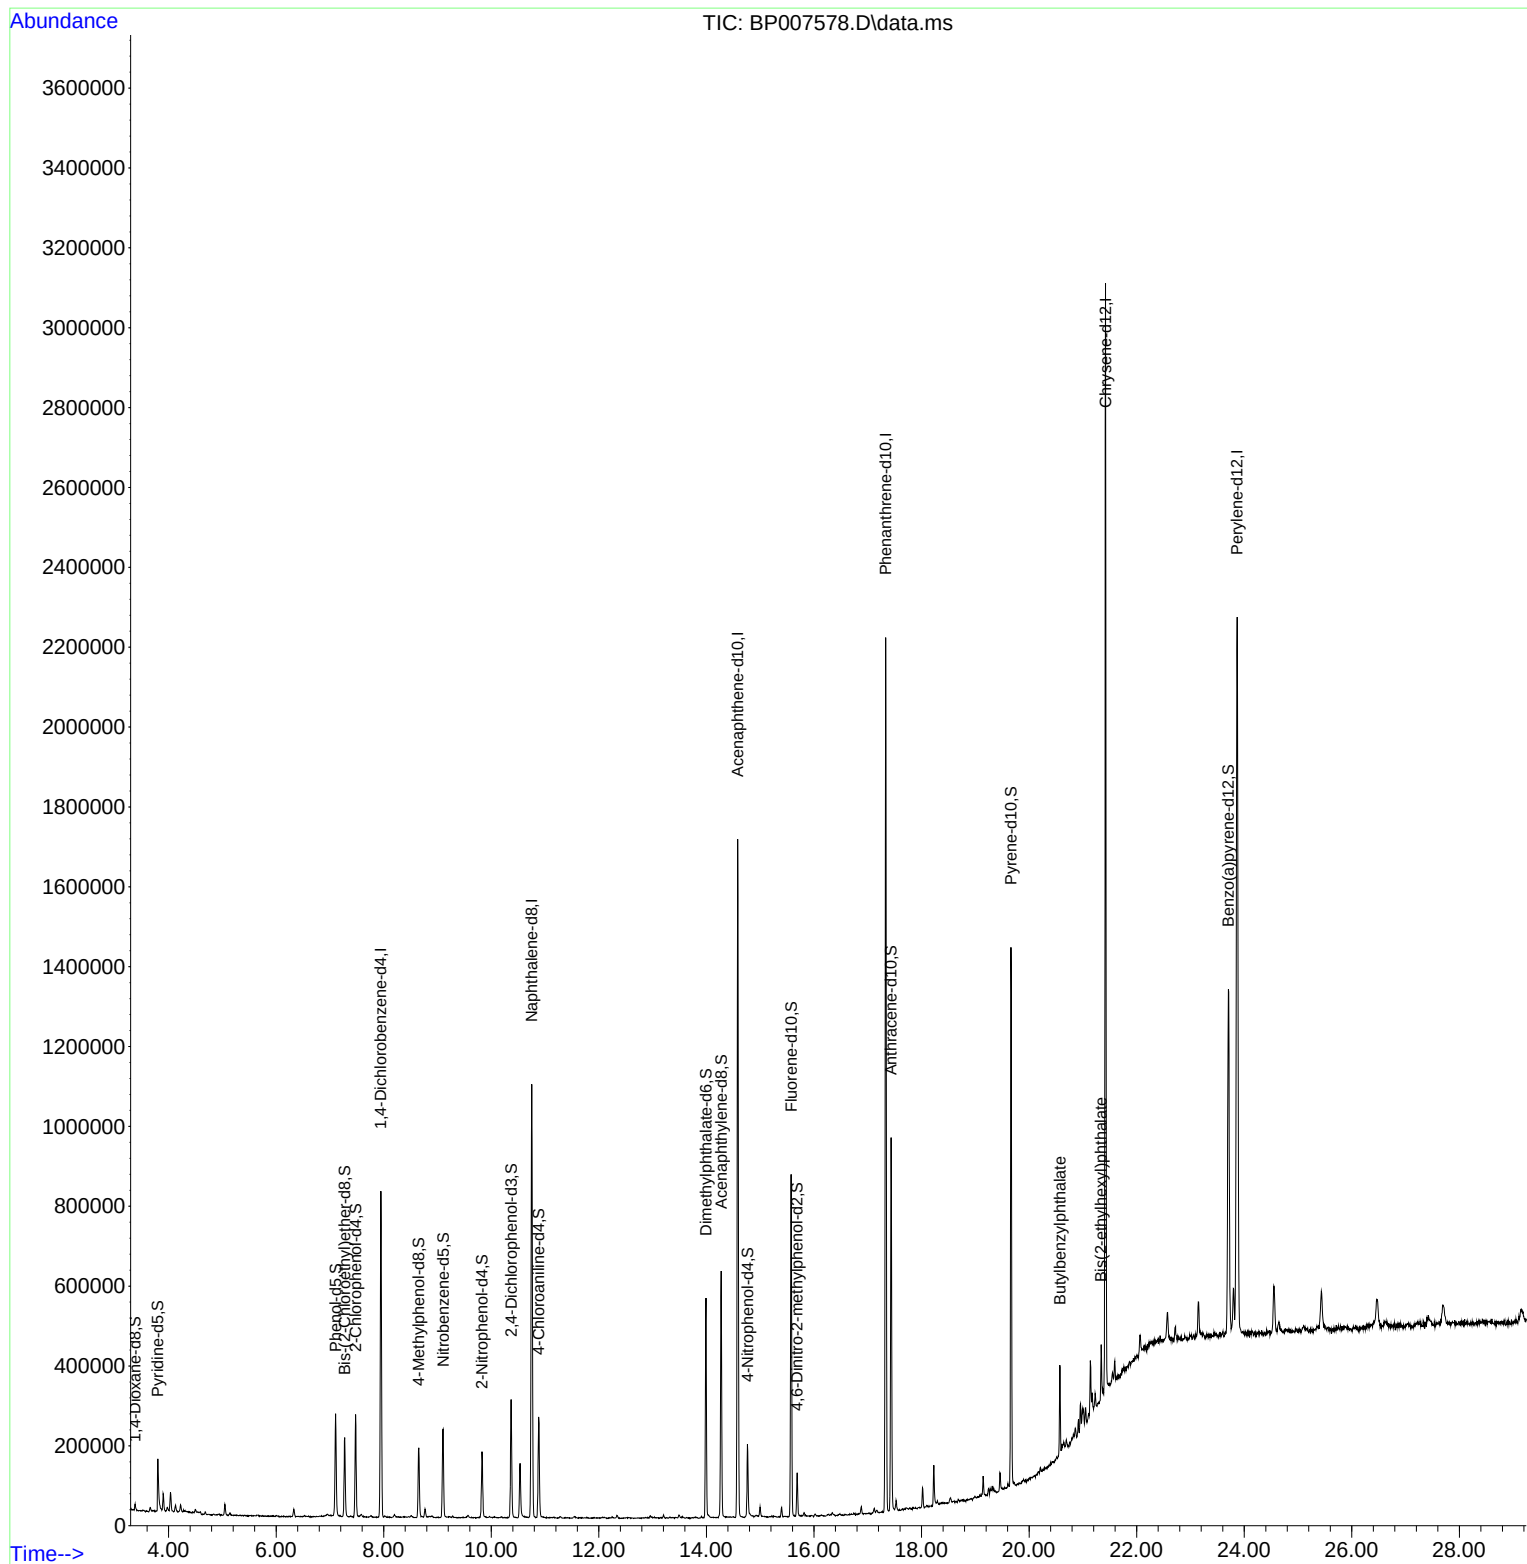


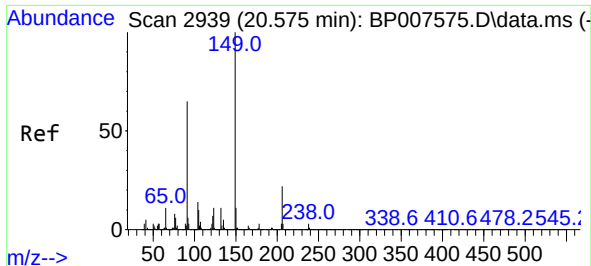

#83
Butylbenzylphthalate
Concen: 2.120 ng/ul
RT: 20.574 min Scan# 2939
Delta R.T. 0.000 min
Lab File: BP007578.D
Acq: 22 Oct 2021 07:39

Instrument :
BNA_P
ClientSampled :
JDGD3

Tgt Ion:	149	Resp:	66326
Ion Ratio	Lower	Upper	
149	100		
91	67.1	55.9	83.9
206	23.1	17.4	26.0

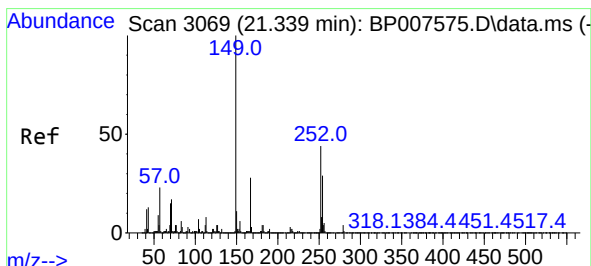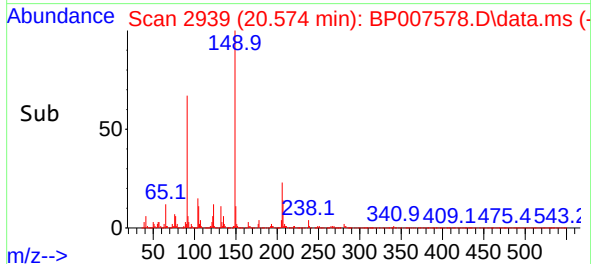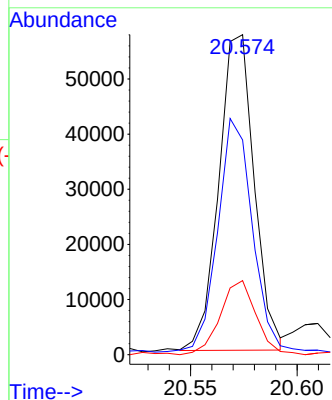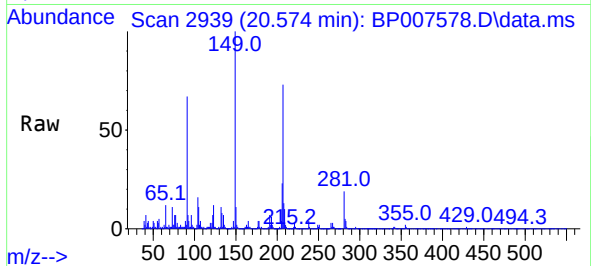

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.040 ng/ul
RT: 21.339 min Scan# 3069
Delta R.T. -0.006 min
Lab File: BP007578.D
Acq: 22 Oct 2021 07:39

Tgt Ion:	149	Resp:	49747
Ion Ratio	Lower	Upper	
149	100		
167	25.3	22.6	33.8
279	4.4	3.3	4.9

