

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007588.D
 Acq On : 22 Oct 2021 14:07
 Operator : CG/JU
 Sample : M4281-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY62

Quant Time: Oct 22 15:16:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	178347	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	723403	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	459371	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.333	188	984598	20.000	ng/u1	0.00
79) Chrysene-d12	21.421	240	1039808	20.000	ng/u1	0.00
88) Perylene-d12	23.868	264	1071583	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	21758	4.818	ng/uL	0.00
4) Pyridine-d5	3.793	84	144996	11.730	ng/u1	0.00
7) Phenol-d5	7.105	99	53043	3.808	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	230505	27.748	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	130656	11.925	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	102135	9.520	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	151595	33.114	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	71328	16.680	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	148303	14.219	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	385171	27.309	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	1075072	33.827	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1208311	30.253	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	14388	2.821	ng/u1	0.00
60) Fluorene-d10	15.575	176	909447	34.195	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	41212	10.446	ng/u1	0.00
73) Anthracene-d10	17.433	188	1557309	37.243	ng/u1	0.00
81) Pyrene-d10	19.669	212	1892252	36.402	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.715	264	1860308	34.890	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.128	94	17027	1.196	ng/u1	96
18) 4-Methylphenol	8.704	108	22076	1.932	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007588.D
Acq On : 22 Oct 2021 14:07
Operator : CG/JU
Sample : M4281-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY62

Quant Time: Oct 22 15:16:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration




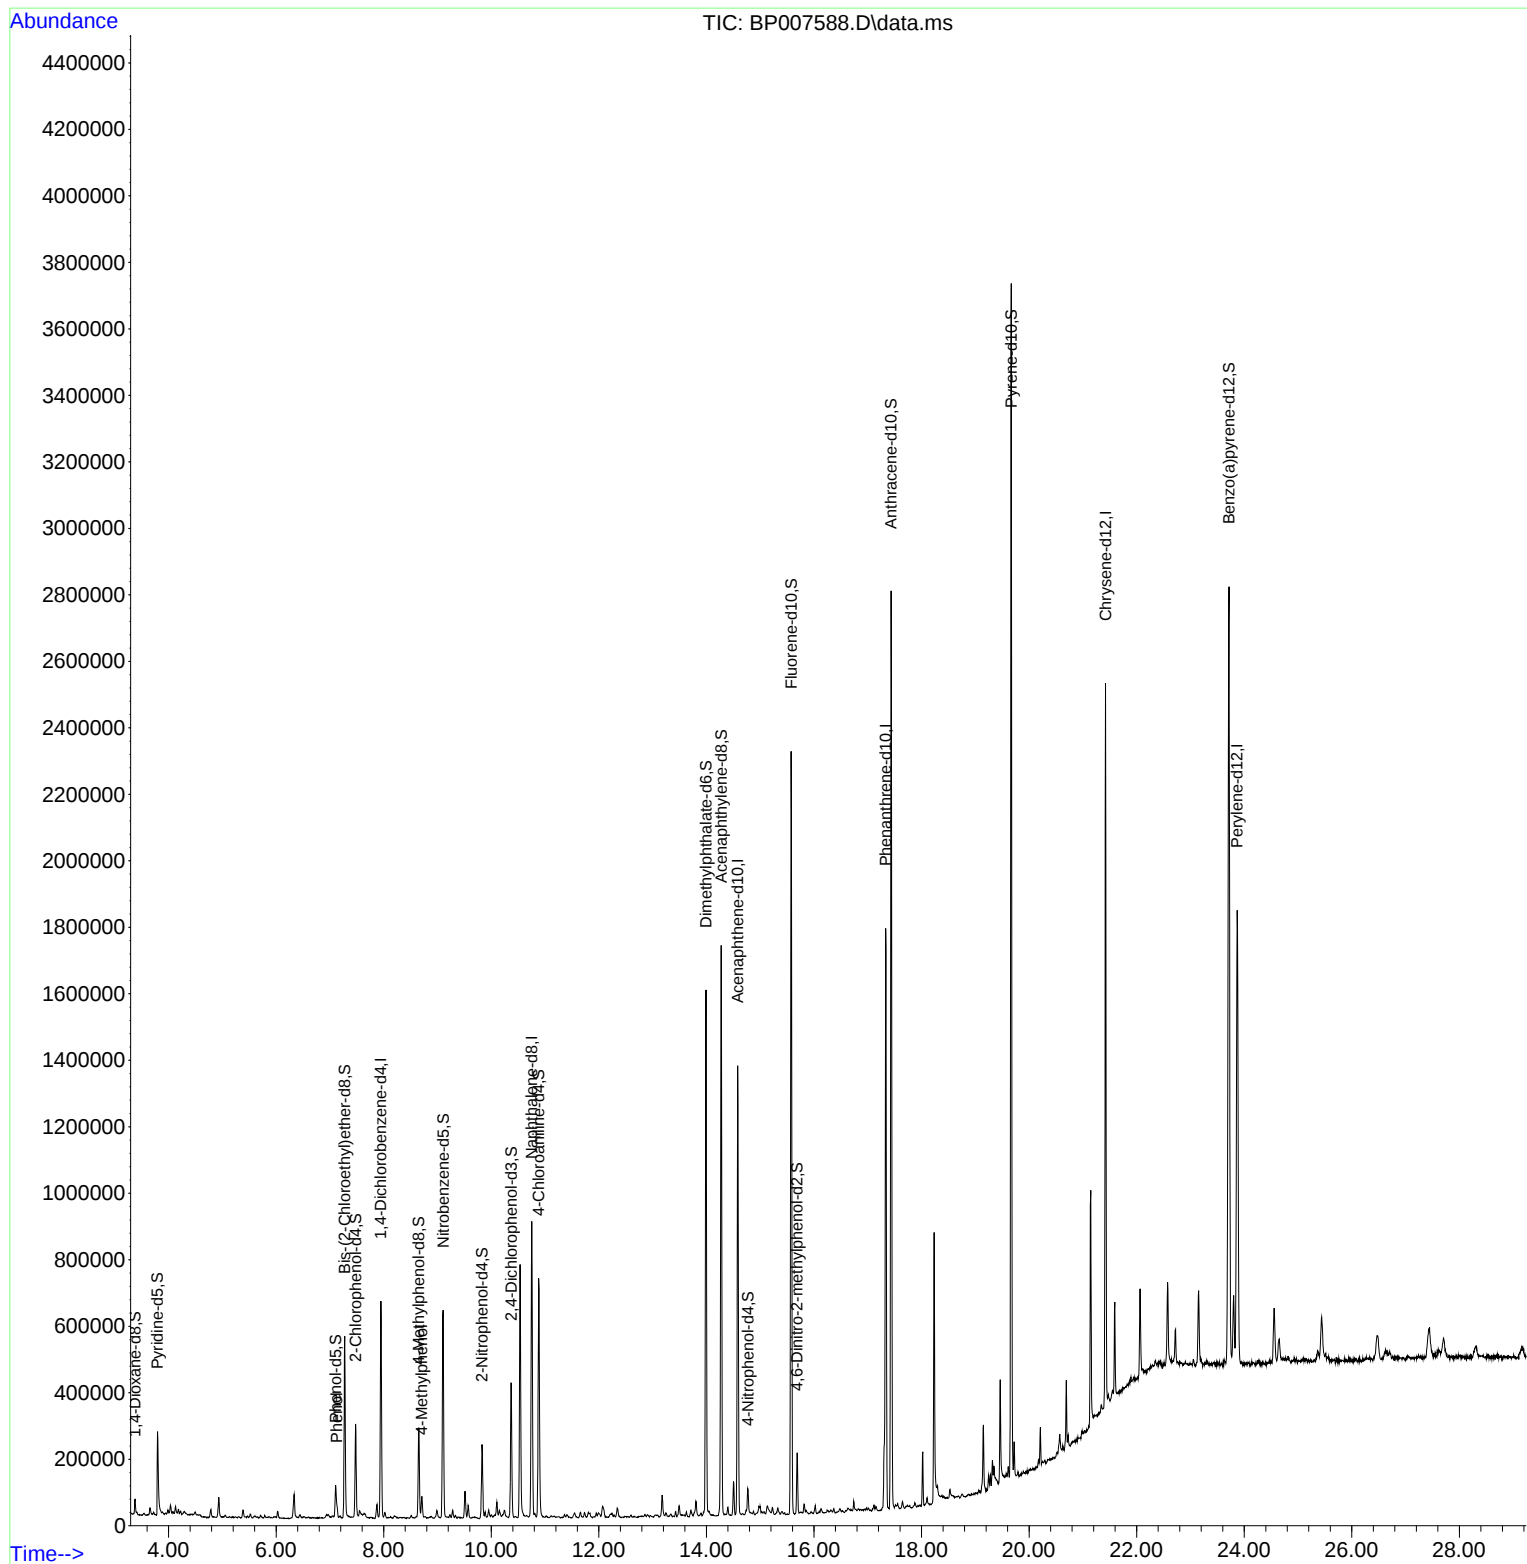


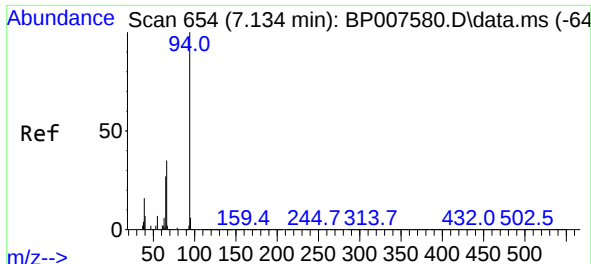

#8
Phenol
Concen: 1.196 ng/ul
RT: 7.128 min Scan# 653
Delta R.T. -0.012 min
Lab File: BP007588.D
Acq: 22 Oct 2021 14:07

Instrument :
BNA_P
ClientSampleId :
BFY62

Tgt Ion: 94	Resp: 17027
Ion Ratio	Lower Upper
94 100	
65 27.6	21.9 32.9
66 41.1	29.9 44.9

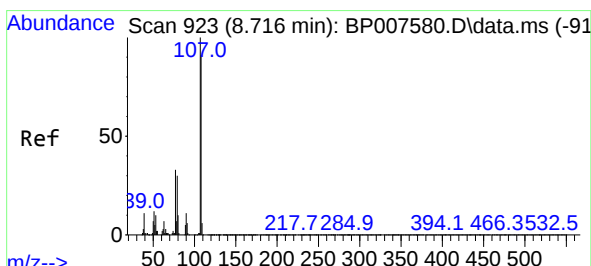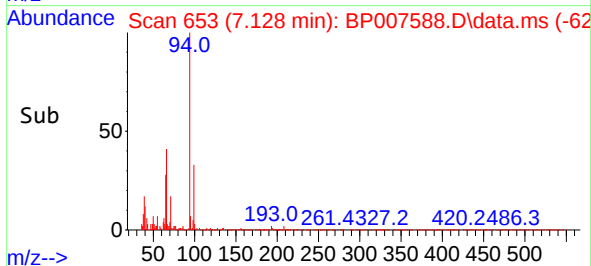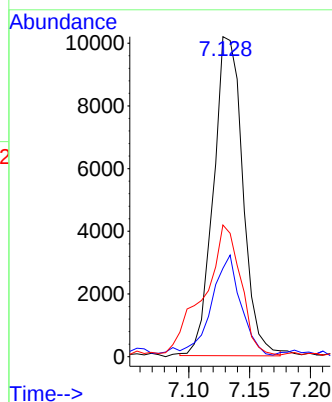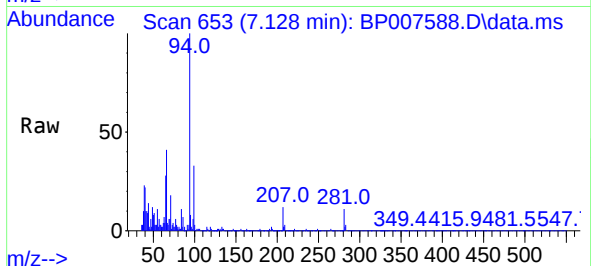

#18
4-Methylphenol
Concen: 1.932 ng/ul
RT: 8.704 min Scan# 921
Delta R.T. -0.018 min
Lab File: BP007588.D
Acq: 22 Oct 2021 14:07

Tgt Ion: 108	Resp: 22076
Ion Ratio	Lower Upper
108 100	
107 115.3	90.9 136.3

