

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007590.D
 Acq On : 22 Oct 2021 15:15
 Operator : CG/JU
 Sample : M4281-08
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY64

Quant Time: Oct 22 16:08:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	161700	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	664239	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	419839	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	915593	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	967025	20.000	ng/u1	0.00
88) Perylene-d12	23.869	264	993091	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	22283	5.443	ng/uL	0.00
4) Pyridine-d5	3.793	84	129555	11.560	ng/u1	0.00
7) Phenol-d5	7.105	99	79911	6.328	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	234171	31.091	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	184244	18.546	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	164226	16.884	ng/u1	0.00
21) Nitrobenzene-d5	9.105	128	154805	36.827	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	107693	27.428	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	220531	23.027	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	365473	28.220	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	1104781	38.035	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1246944	34.160	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	18696	4.011	ng/u1	0.00
60) Fluorene-d10	15.575	176	950949	39.122	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	59172	16.129	ng/u1	0.00
73) Anthracene-d10	17.434	188	1564358	40.232	ng/u1	0.00
81) Pyrene-d10	19.669	212	1917483	39.664	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.716	264	1886922	38.186	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.411	88	33875	7.606	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007590.D
Acq On : 22 Oct 2021 15:15
Operator : CG/JU
Sample : M4281-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY64

Quant Time: Oct 22 16:08:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

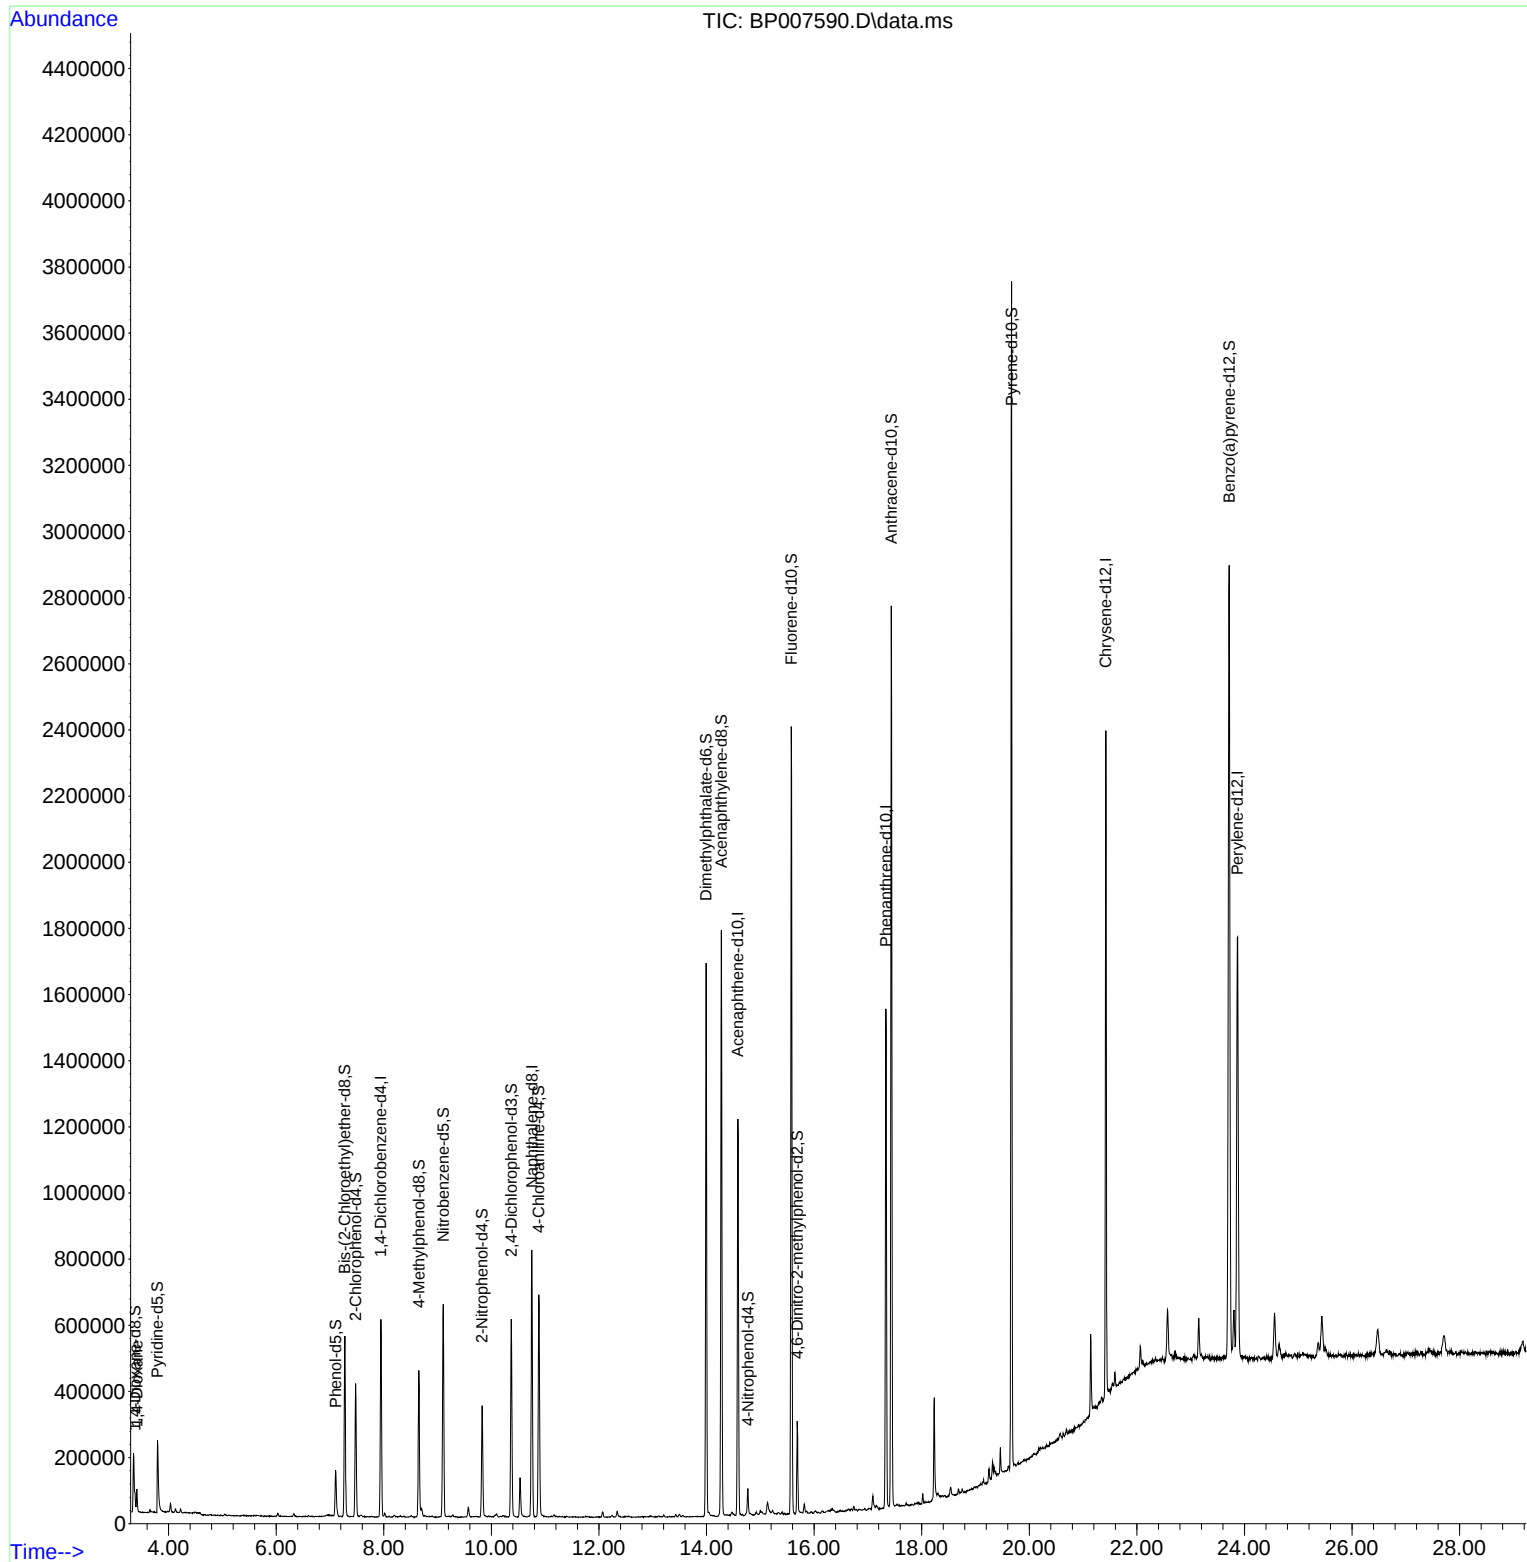

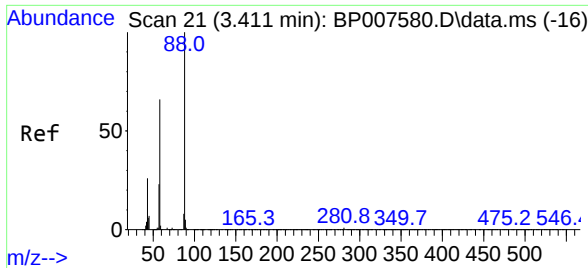

#2
 1,4-Dioxane
 Concen: 7.606 ng/uL
 RT: 3.411 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP007590.D
 Acq: 22 Oct 2021 15:15

Instrument :
 BNA_P
 ClientSampleId :
 BFY64

Tgt Ion: 88 Resp: 33875
 Ion Ratio Lower Upper
 88 100
 43 25.2 24.2 36.2
 58 68.8 62.5 93.7

