

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007596.D
 Acq On : 22 Oct 2021 18:39
 Operator : CG/JU
 Sample : M4281-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY72

Quant Time: Oct 22 23:54:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	193407	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	792251	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	515474	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	1124037	20.000	ng/ul	0.00
79) Chrysene-d12	21.421	240	1188958	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	1241323	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	24984	5.102	ng/uL	0.00
4) Pyridine-d5	3.799	84	147459	11.001	ng/ul	0.00
7) Phenol-d5	7.110	99	134575	8.910	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	288835	32.062	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	348742	29.350	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	240514	20.673	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	205331	40.954	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	227374	48.551	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	413256	36.179	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	471473	30.523	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	1351133	37.887	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	1560596	34.820	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	56745	9.916	ng/ul	0.00
60) Fluorene-d10	15.575	176	1145220	38.373	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	52503	11.657	ng/ul	0.00
73) Anthracene-d10	17.433	188	1945356	40.752	ng/ul	0.00
81) Pyrene-d10	19.669	212	2321614	39.059	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	2400489	38.864	ng/ul	0.00
Target Compounds						
					Qvalue	
18) 4-Methylphenol	8.710	108	320539	25.871	ng/ul	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007596.D
Acq On : 22 Oct 2021 18:39
Operator : CG/JU
Sample : M4281-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY72

Quant Time: Oct 22 23:54:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration

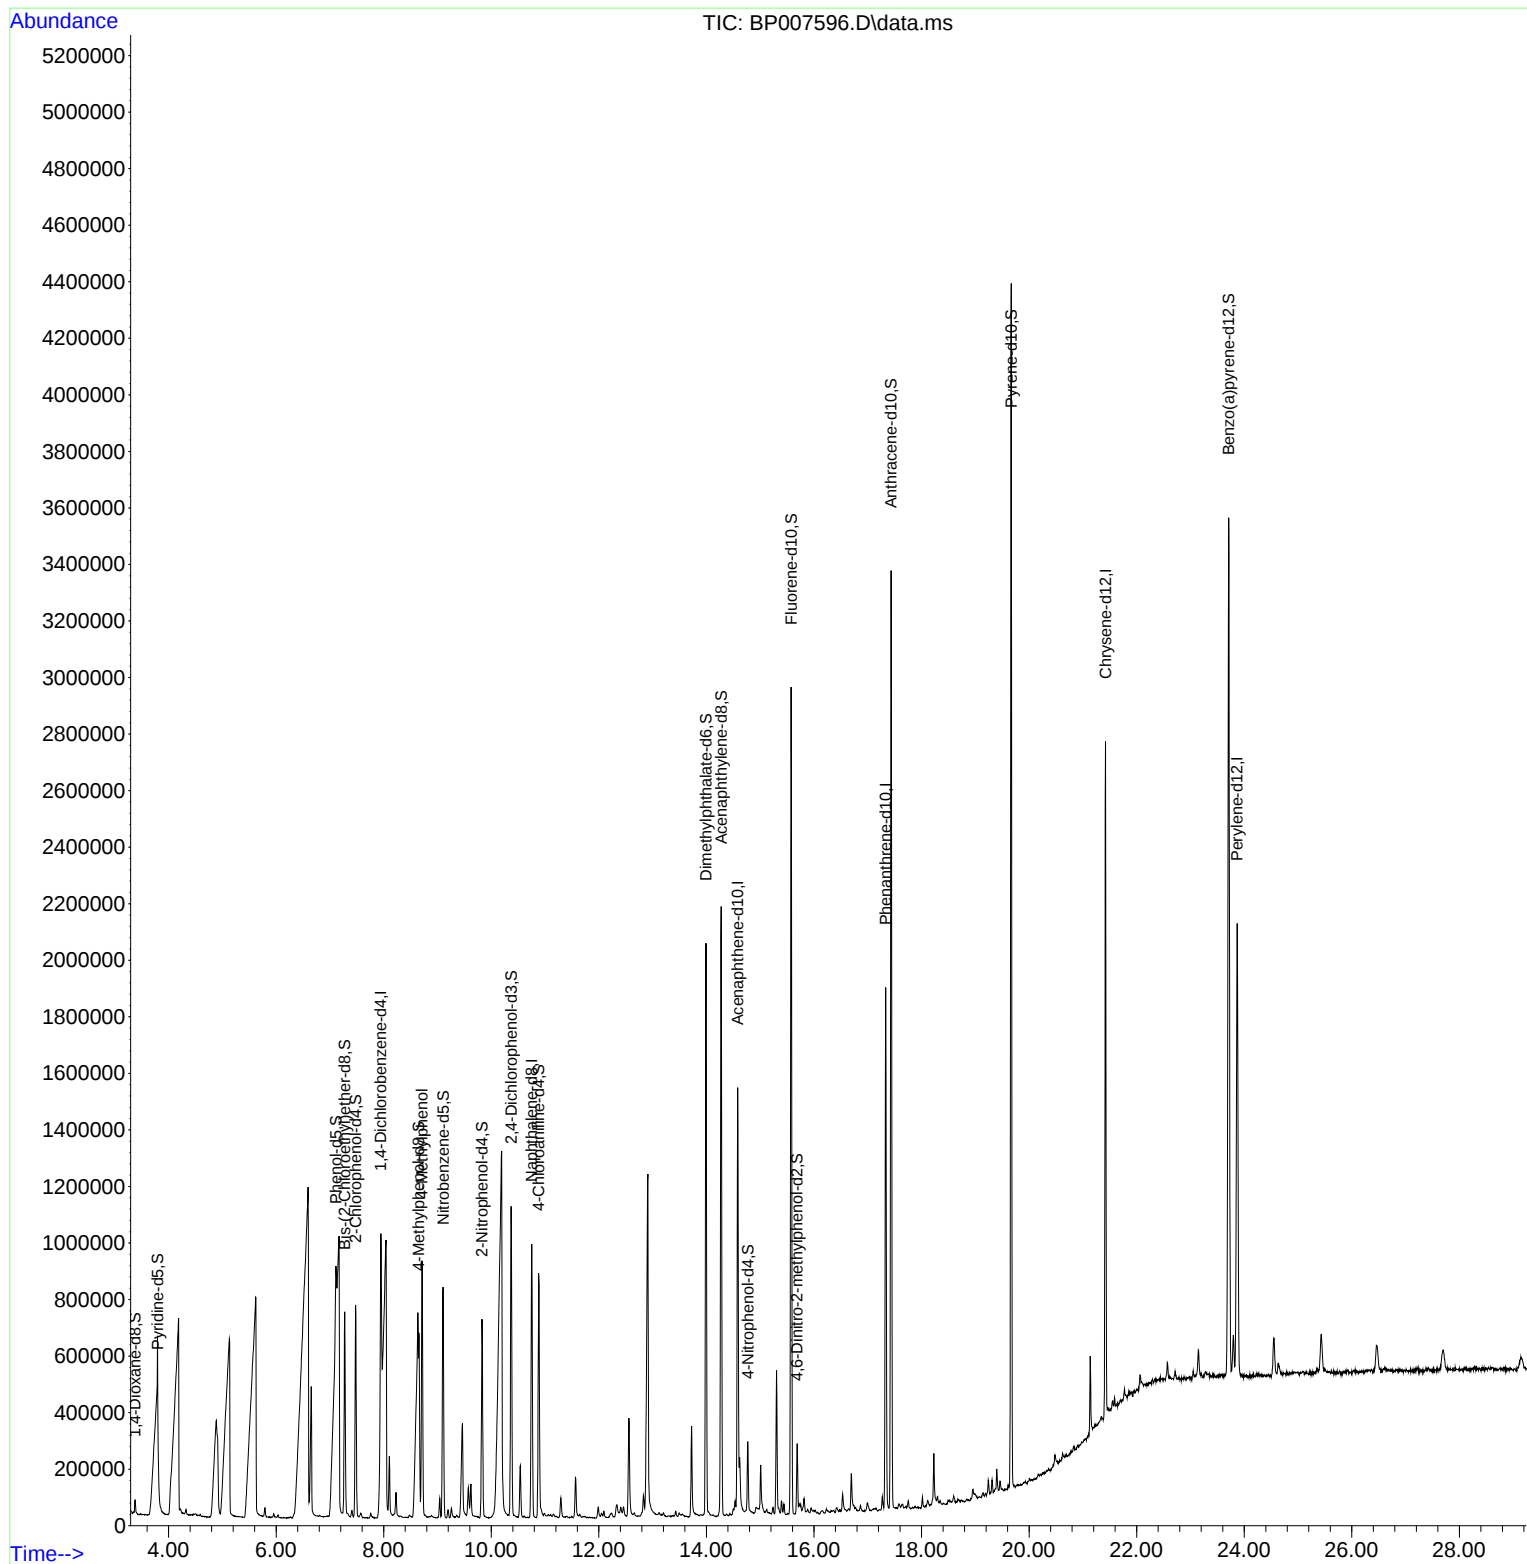

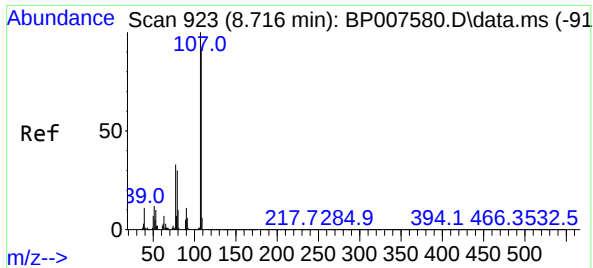

#18
4-Methylphenol
Concen: 25.871 ng/ul
RT: 8.710 min Scan# 922
Delta R.T. -0.012 min
Lab File: BP007596.D
Acq: 22 Oct 2021 18:39

Instrument :
BNA_P
ClientSampleId :
BFY72

Tgt Ion:108 Resp: 320539
Ion Ratio Lower Upper
108 100
107 127.3 90.9 136.3

