

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
 Data File : BP007604.D
 Acq On : 22 Oct 2021 23:44
 Operator : CG/JU
 Sample : M4281-13
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFY71

Quant Time: Oct 23 00:45:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 20 10:49:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	207303	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	831138	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	538309	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	1152152	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	1217281	20.000	ng/u1	0.00
88) Perylene-d12	23.863	264	1260859	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	23693	4.514	ng/uL	0.00
4) Pyridine-d5	3.793	84	125375	8.726	ng/u1	0.00
7) Phenol-d5	7.105	99	110359	6.817	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	263283	27.267	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.475	132	291651	22.900	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	198384	15.909	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	179636	34.152	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.828	143	183268	37.303	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	348756	29.103	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	353576	21.819	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	1201608	32.265	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1374758	29.373	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	42818	7.165	ng/u1	0.00
60) Fluorene-d10	15.575	176	1017419	32.645	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	81155	17.579	ng/u1	0.00
73) Anthracene-d10	17.434	188	1706777	34.882	ng/u1	0.00
81) Pyrene-d10	19.663	212	2146129	35.267	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	2137400	34.069	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.134	94	16968	1.025	ng/u1	96
18) 4-Methylphenol	8.705	108	41905	3.156	ng/u1	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102121\
Data File : BP007604.D
Acq On : 22 Oct 2021 23:44
Operator : CG/JU
Sample : M4281-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFY71

Quant Time: Oct 23 00:45:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP101421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 20 10:49:33 2021
Response via : Initial Calibration




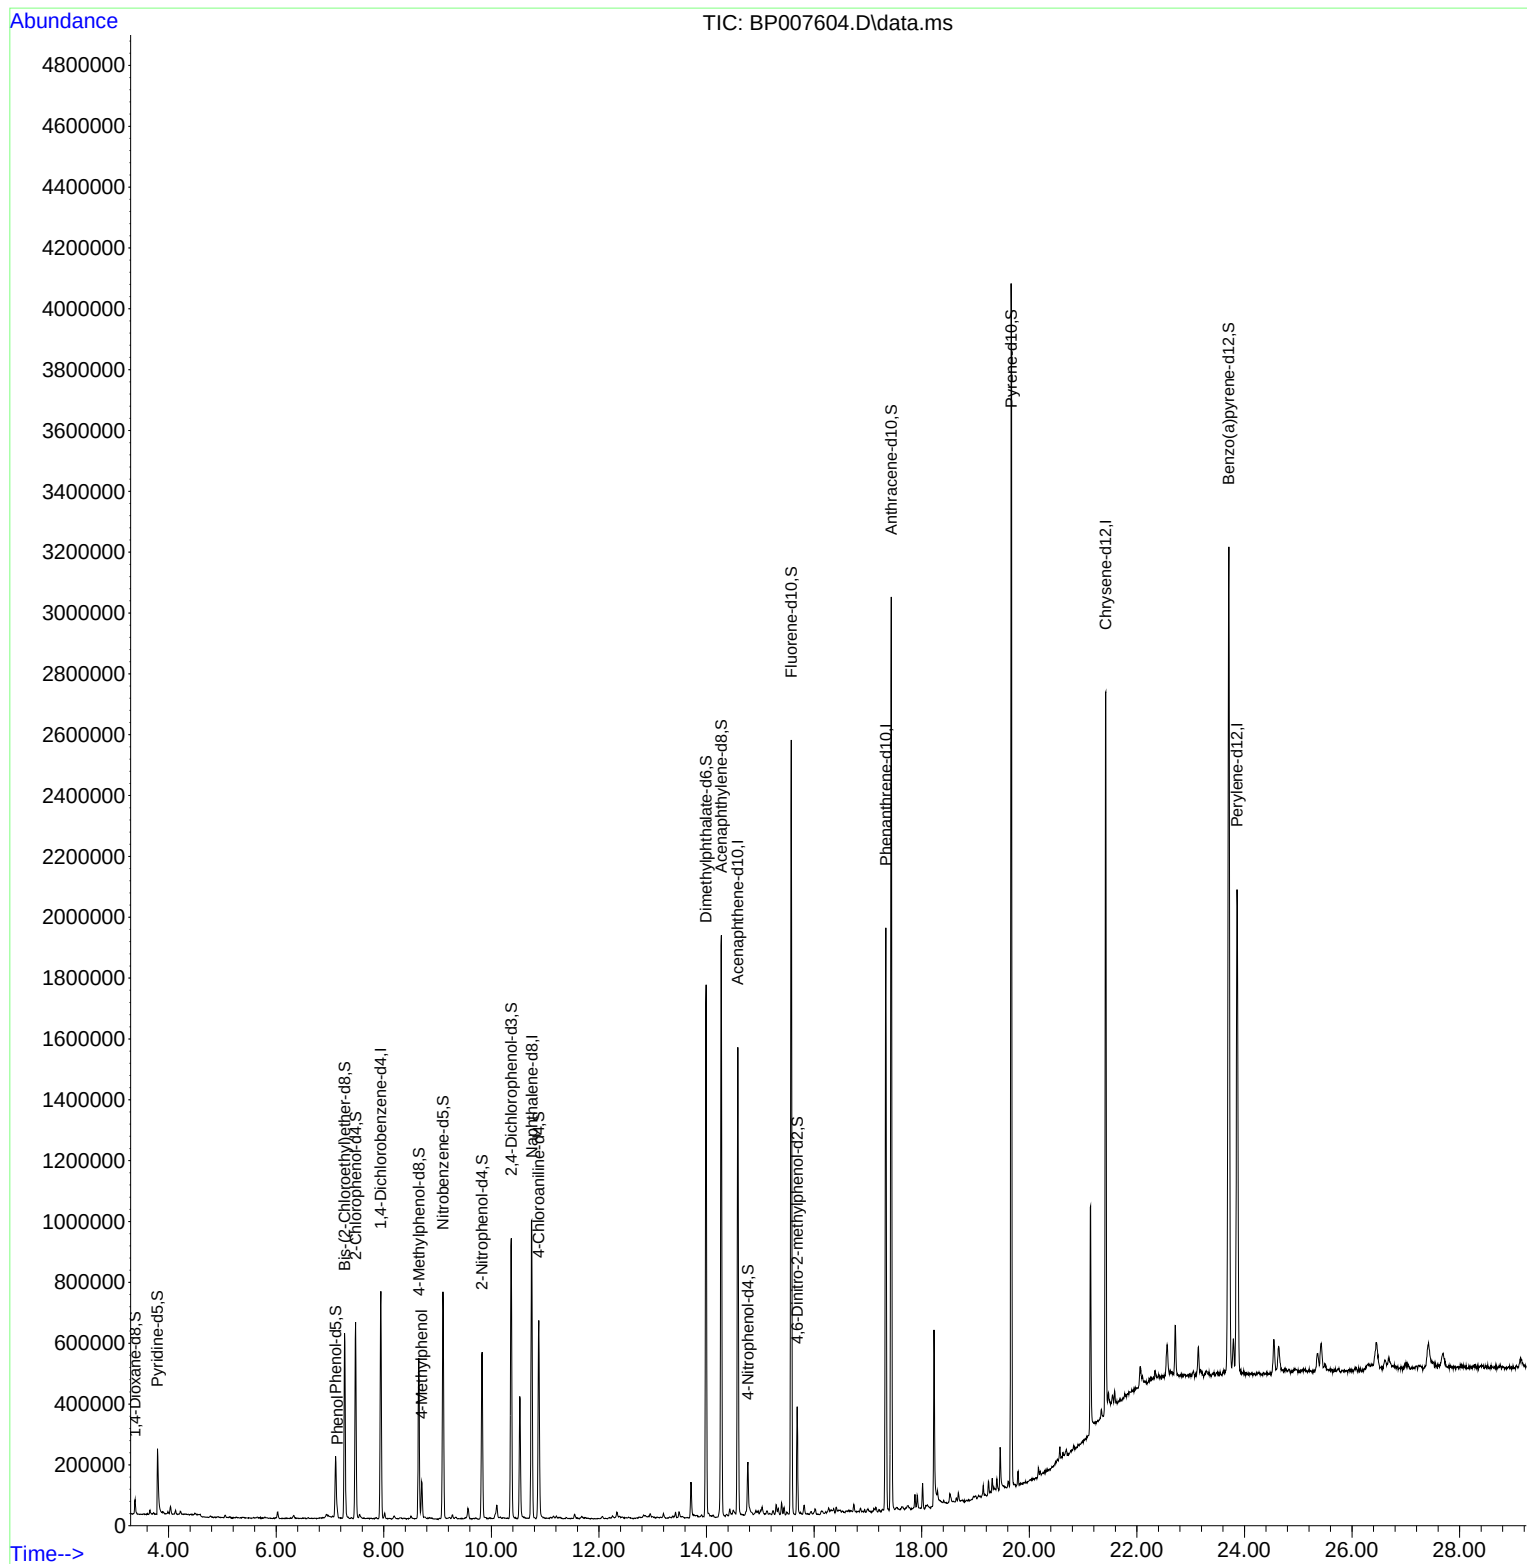


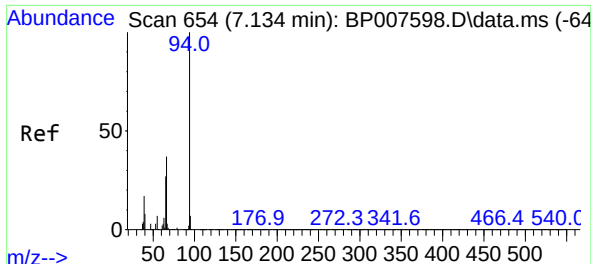

#8
Phenol
Concen: 1.025 ng/ul
RT: 7.134 min Scan# 654
Delta R.T. -0.006 min
Lab File: BP007604.D
Acq: 22 Oct 2021 23:44

Instrument :
BNA_P
ClientSampleId :
BFY71

Tgt Ion:	94	Resp:	16968
Ion	Ratio	Lower	Upper
94	100		
65	31.8	21.9	32.9
66	38.1	29.9	44.9

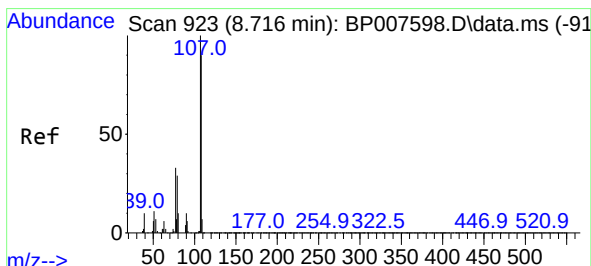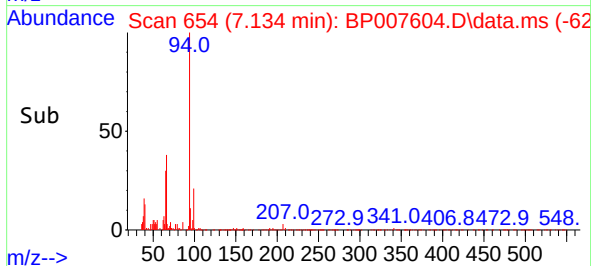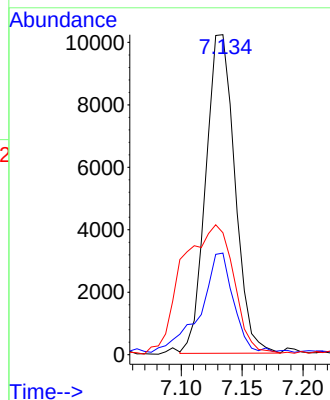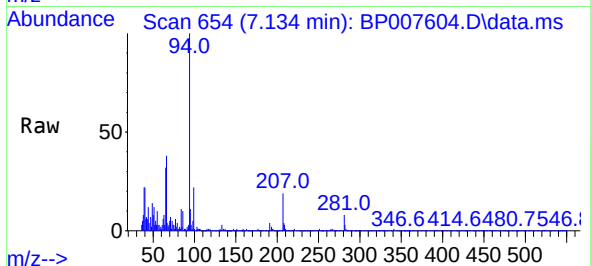

#18
4-Methylphenol
Concen: 3.156 ng/ul
RT: 8.705 min Scan# 921
Delta R.T. -0.017 min
Lab File: BP007604.D
Acq: 22 Oct 2021 23:44

Tgt Ion:	108	Resp:	41905
Ion	Ratio	Lower	Upper
108	100		
107	126.2	90.9	136.3

